

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U062620\
 Data File : VU039154.D
 Acq On : 26 Jun 2020 10:28
 Operator : SY/MD
 Sample : VU0626WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK22

Quant Time: Jun 27 00:03:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Jun 26 23:52:58 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	232892	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	238869	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.82	152	102495	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	64597	3.79	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.80%
7) Chloroethane-d5	1.93	69	64126	4.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.00%
11) 1,1-Dichloroethene-d2	2.59	63	101547	3.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.00%
20) 2-Butanone-d5	4.68	46	349407	56.77	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.54%
24) Chloroform-d	5.10	84	164199	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
26) 1,2-Dichloroethane-d4	5.74	65	103789	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
32) Benzene-d6	5.76	84	293569	4.43	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.60%
36) 1,2-Dichloropropane-d6	6.72	67	103773	4.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.20%
41) Toluene-d8	7.92	98	217663	3.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.60%
43) trans-1,3-Dichloropropene-	8.20	79	41348	4.27	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.40%
46) 2-Hexanone-d5	8.65	63	250493	50.17	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	100.34%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	98065	4.74	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.80%
64) 1,2-Dichlorobenzene-d4	12.20	152	95537	5.00	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.00%


Target Compounds					Ovalue
16) Methylene chloride	3.08	84	2637	0.133 ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU062620\
Data File : VU039154.D
Acq On : 26 Jun 2020 10:28
Operator : SY/MD
Sample : VU0626WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK22

Quant Time: Jun 27 00:03:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jun 26 23:52:58 2020
Response via : Initial Calibration

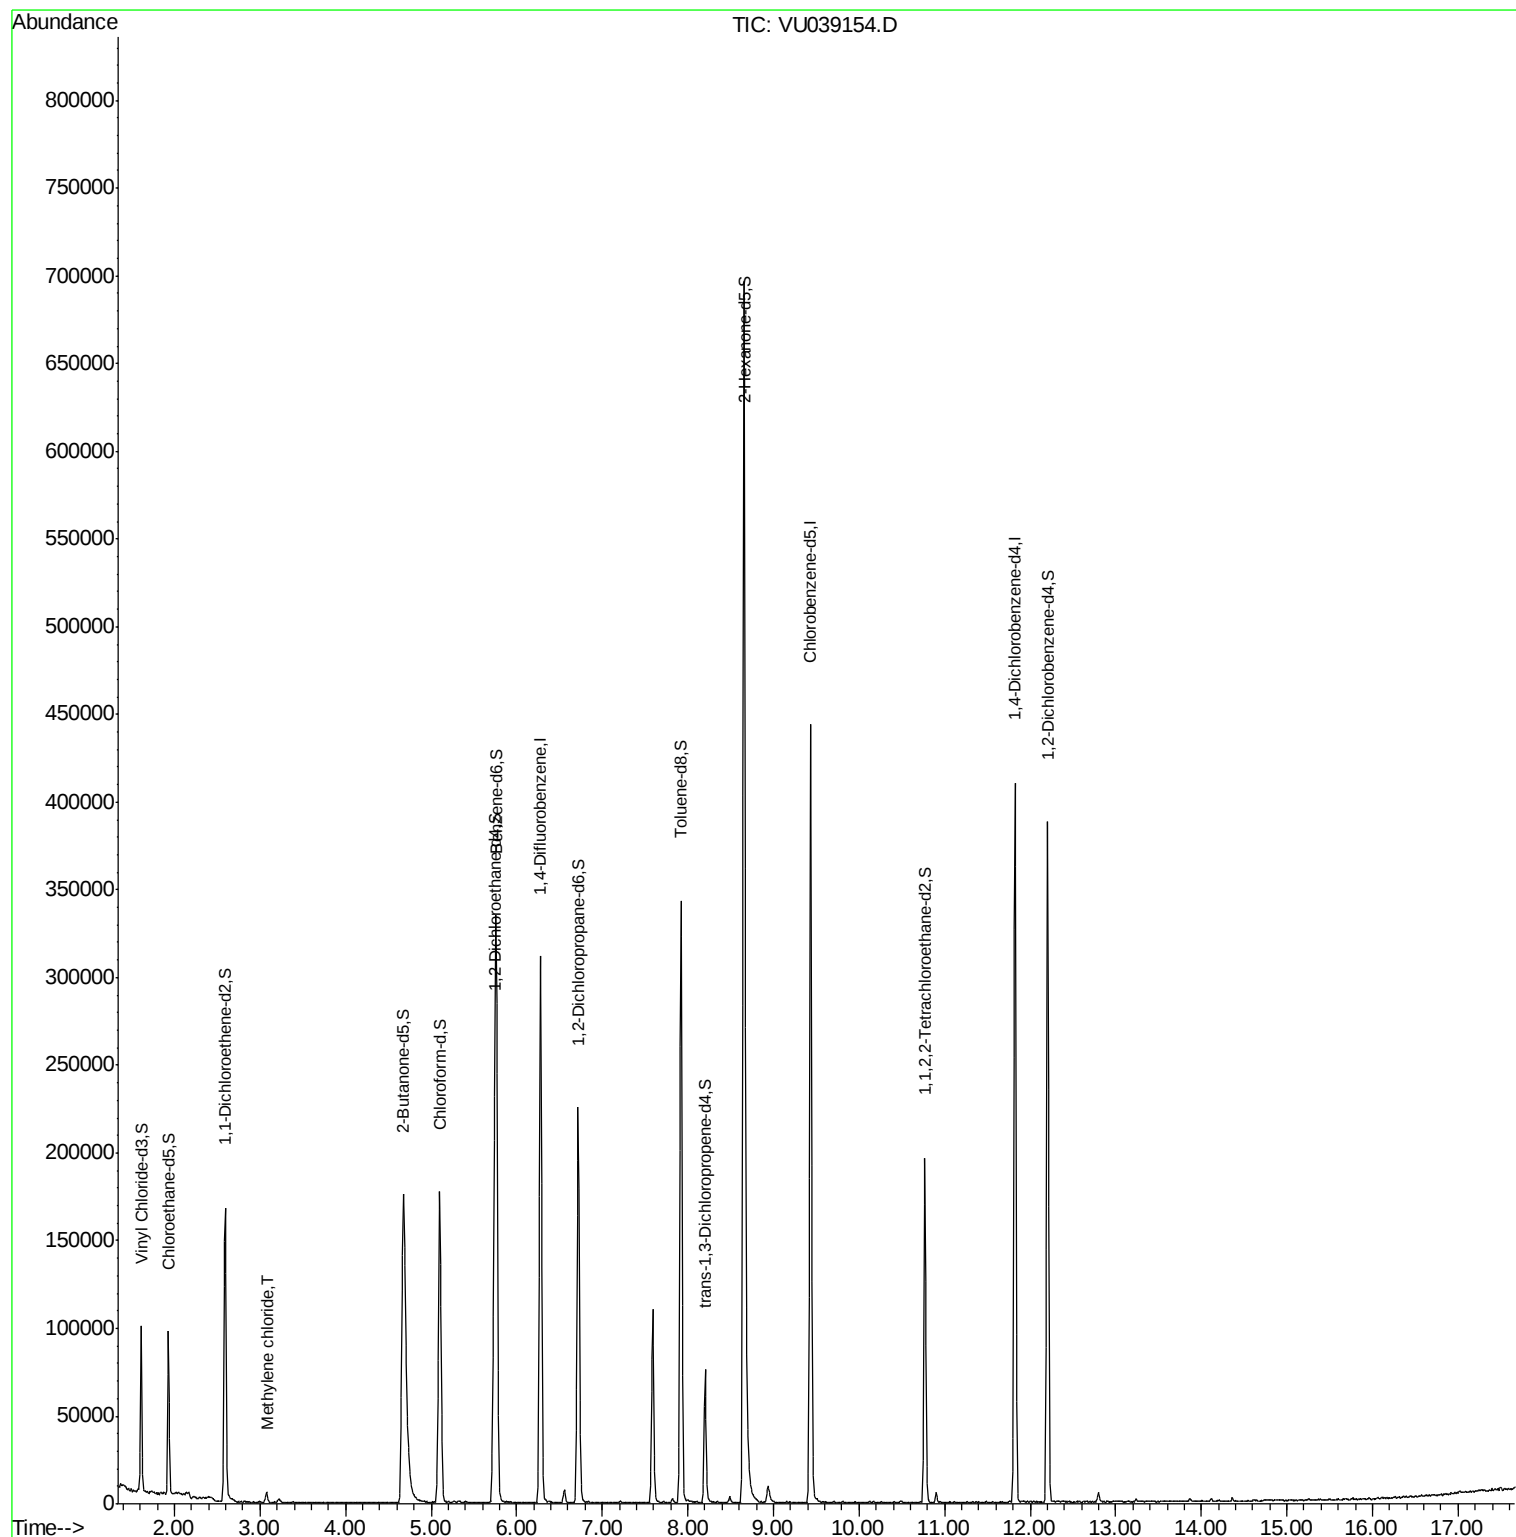

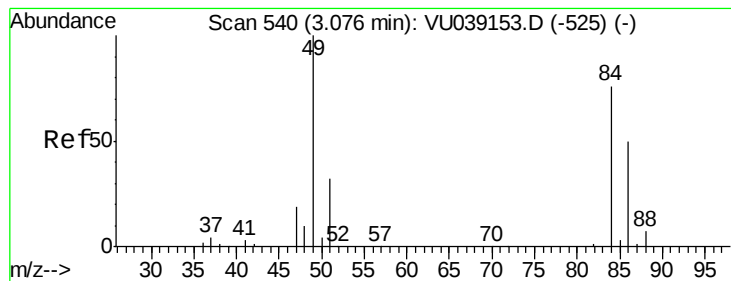

#16
Methylene chloride
Concen: 0.133 ug/L
RT: 3.08 min Scan# 541
Delta R.T. 0.00 min
Lab File: VU039154.D
Acq: 26 Jun 2020 10:28

Instrument :
MSVOA_U
ClientSampleId :
VBLK22

Tot Ion: 84 Resp: 2637

Ion	Ratio	Lower	Upper
84	100		
86	54.3	44.1	81.9
49	117.8	93.1	172.9

