


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062620\
 Data File : VU039152.D
 Acq On : 26 Jun 2020 08:55
 Operator : SY/MD
 Sample : BFB22
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB22

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Jun 26 23:52:58 2020

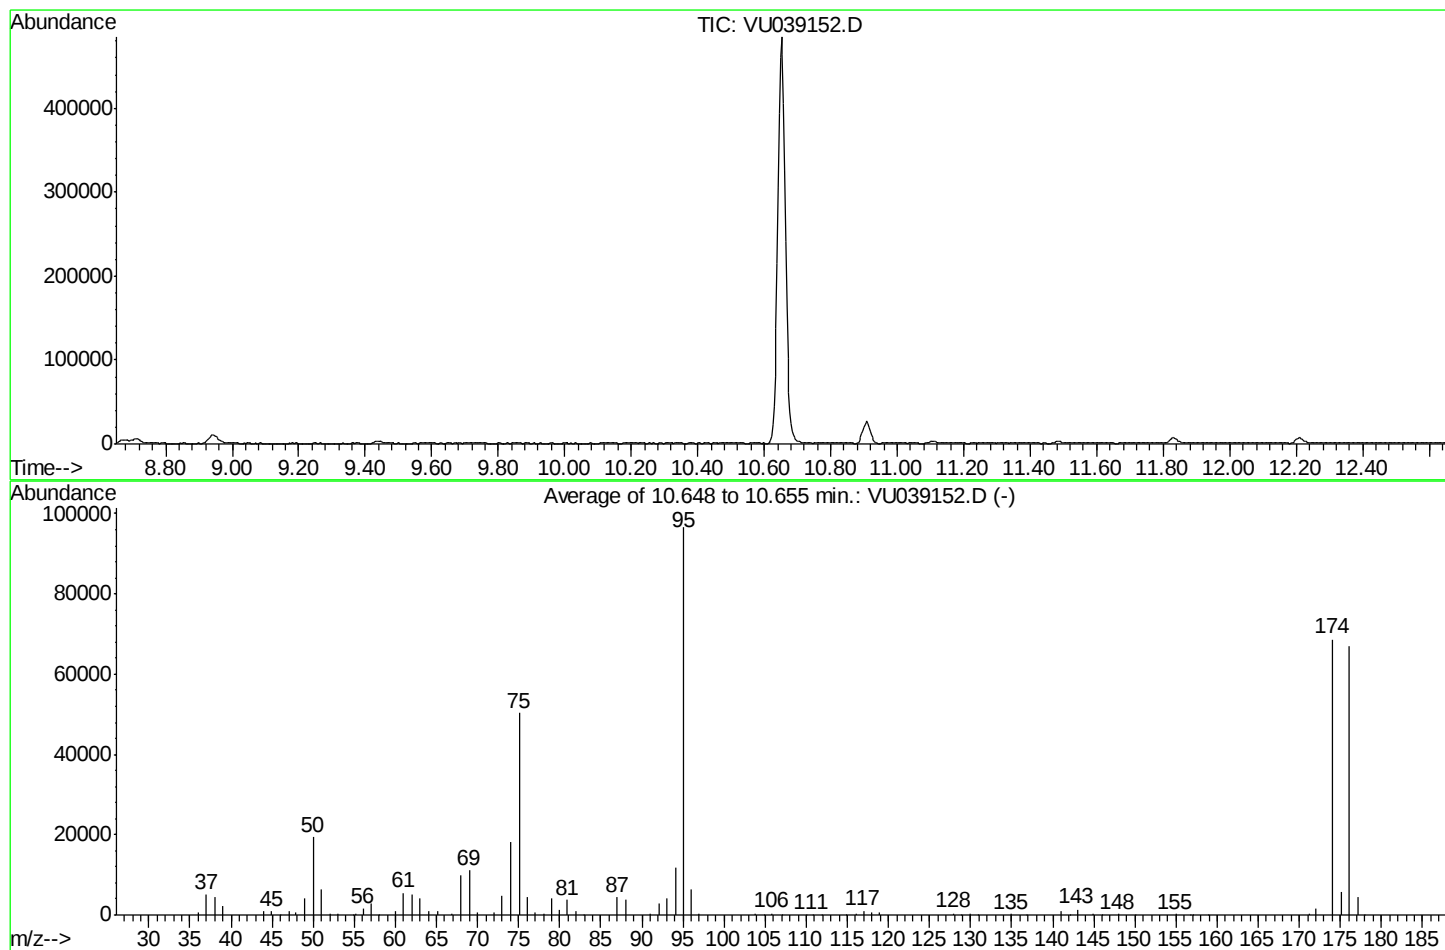

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2881

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	19312	PASS
75	95	30	80	52.1	50362	PASS
95	95	100	100	100.0	96597	PASS
96	95	5	9	6.7	6485	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.1	68666	PASS
175	174	5	9	8.2	5636	PASS
176	174	95	101	97.4	66850	PASS
177	176	5	9	6.8	4542	PASS

m/z	Abundance
36.00	769.0
37.00	5137.0
38.00	4645.0
39.00	2176.0
40.00	250.0
43.90	1547.0
44.90	1019.0
46.20	173.0
47.00	997.0
47.90	699.0
49.00	4128.0
50.00	19104.0
51.00	6149.0
52.00	328.0
53.00	216.0
54.80	241.0
55.20	235.0
56.10	1454.0
57.10	2929.0
58.00	105.0
59.90	988.0
61.00	5490.0
62.10	4982.0
63.00	4130.0
64.00	907.0
65.10	1058.0
66.90	227.0
68.00	10090.0
69.00	10907.0
70.00	618.0
71.90	588.0
73.00	4911.0
74.00	18352.0
75.10	50272.0
76.00	4243.0
77.00	522.0
78.10	534.0
79.00	4145.0
79.90	1328.0
81.00	3872.0
81.90	1065.0
82.90	117.0
87.00	4502.0
88.00	3643.0
91.00	382.0
92.10	2884.0
93.00	4082.0
94.10	11719.0
95.10	94584.0
96.10	6242.0
96.90	163.0
103.90	444.0
104.80	158.0
105.90	434.0
110.70	108.0
116.10	277.0
116.90	954.0
117.90	473.0
118.90	692.0
127.90	421.0
128.90	176.0
130.00	277.0
131.00	122.0
135.00	221.0
136.80	111.0
141.00	1079.0
142.00	110.0
143.00	1452.0
145.00	554.0
145.90	166.0
147.90	261.0
150.00	143.0
155.00	181.0
158.90	160.0
171.20	256.0
172.10	1255.0
174.10	66160.0
175.10	5386.0
176.10	63640.0
177.10	4587.0
177.90	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
36.00	812.0
37.00	5227.0
38.00	4735.0
39.00	2108.0
40.00	311.0
43.90	1347.0
44.90	1002.0
46.00	159.0
47.00	1145.0
47.90	707.0
49.00	4336.0
50.00	19976.0
51.00	6462.0
52.00	399.0
52.90	195.0
54.80	271.0
55.10	272.0
56.10	1649.0
57.00	2912.0
58.00	115.0
60.00	1042.0
61.00	5831.0
62.00	5273.0
63.00	4377.0
64.00	1068.0
65.10	1072.0
66.90	321.0
68.00	10350.0
69.00	11518.0
70.00	647.0
71.90	634.0
73.00	5015.0
74.00	18888.0
75.10	51872.0
76.10	4541.0
77.10	532.0
78.90	4342.0
80.00	1429.0
81.00	3859.0
81.90	986.0
82.90	142.0
87.00	4434.0
88.00	3922.0
91.10	447.0
92.10	2964.0
93.00	4430.0
94.10	12217.0
95.10	99832.0
96.00	6767.0
97.00	178.0
103.90	458.0
104.90	157.0
105.90	500.0
107.00	106.0
110.00	106.0
110.70	128.0
114.80	100.0
116.10	349.0
117.00	1044.0
117.90	601.0
119.00	632.0
128.00	348.0
128.90	179.0
129.90	239.0
131.00	153.0
134.90	245.0
136.80	134.0
141.00	1142.0
142.10	157.0
143.00	1430.0
145.00	449.0
146.00	119.0
148.00	280.0
155.00	248.0
156.70	115.0
158.80	189.0
171.20	301.0
172.10	1537.0
174.10	70696.0
175.10	5866.0
176.10	69032.0
177.10	4770.0
177.90	183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
36.10	800.0
37.00	4640.0
38.00	4436.0
39.00	2036.0
40.00	347.0
43.90	1080.0
44.90	802.0
45.90	166.0
47.00	1224.0
47.90	617.0
49.00	4068.0
50.00	18856.0
51.00	6100.0
52.00	432.0
52.90	150.0
55.00	284.0
56.00	1661.0
57.00	2772.0
60.00	995.0
61.00	5182.0
62.00	5130.0
63.00	4290.0
64.00	1061.0
65.10	1120.0
66.90	375.0
68.00	9582.0
69.00	10802.0
70.00	683.0
72.00	615.0
73.00	4699.0
74.00	17496.0
75.10	48944.0
76.10	4459.0
77.00	529.0
78.90	4035.0
80.00	1385.0
80.90	3660.0
81.90	921.0
82.90	167.0
87.00	4055.0
88.00	3757.0
91.10	455.0
92.00	2820.0
93.00	4313.0
94.00	11709.0
95.10	95376.0
96.00	6446.0
97.00	229.0
103.80	406.0
105.00	163.0
105.80	520.0
107.00	143.0
110.00	102.0
110.80	110.0
111.80	127.0
114.80	184.0
116.00	373.0
116.90	929.0
117.90	575.0
119.00	580.0
128.00	329.0
128.90	143.0
130.00	217.0
130.90	185.0
134.90	251.0
136.80	175.0
141.00	1029.0
142.10	182.0
143.00	1420.0
144.90	396.0
148.00	293.0
154.90	273.0
157.10	123.0
158.80	132.0
171.20	288.0
172.00	1558.0
174.10	69144.0
175.10	5658.0
176.10	67880.0
177.10	4270.0
177.90	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

Scan 2881 (10.603 min): VU039152.D
BFB22

m/z	Abundance
39.90	302.0
43.90	491.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22