


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062718\
Data File : VU024954.D
Acq On : 27 Jun 2018 09:37
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Title : SW846 8260
Last Update : Wed Jun 13 13:55:26 2018

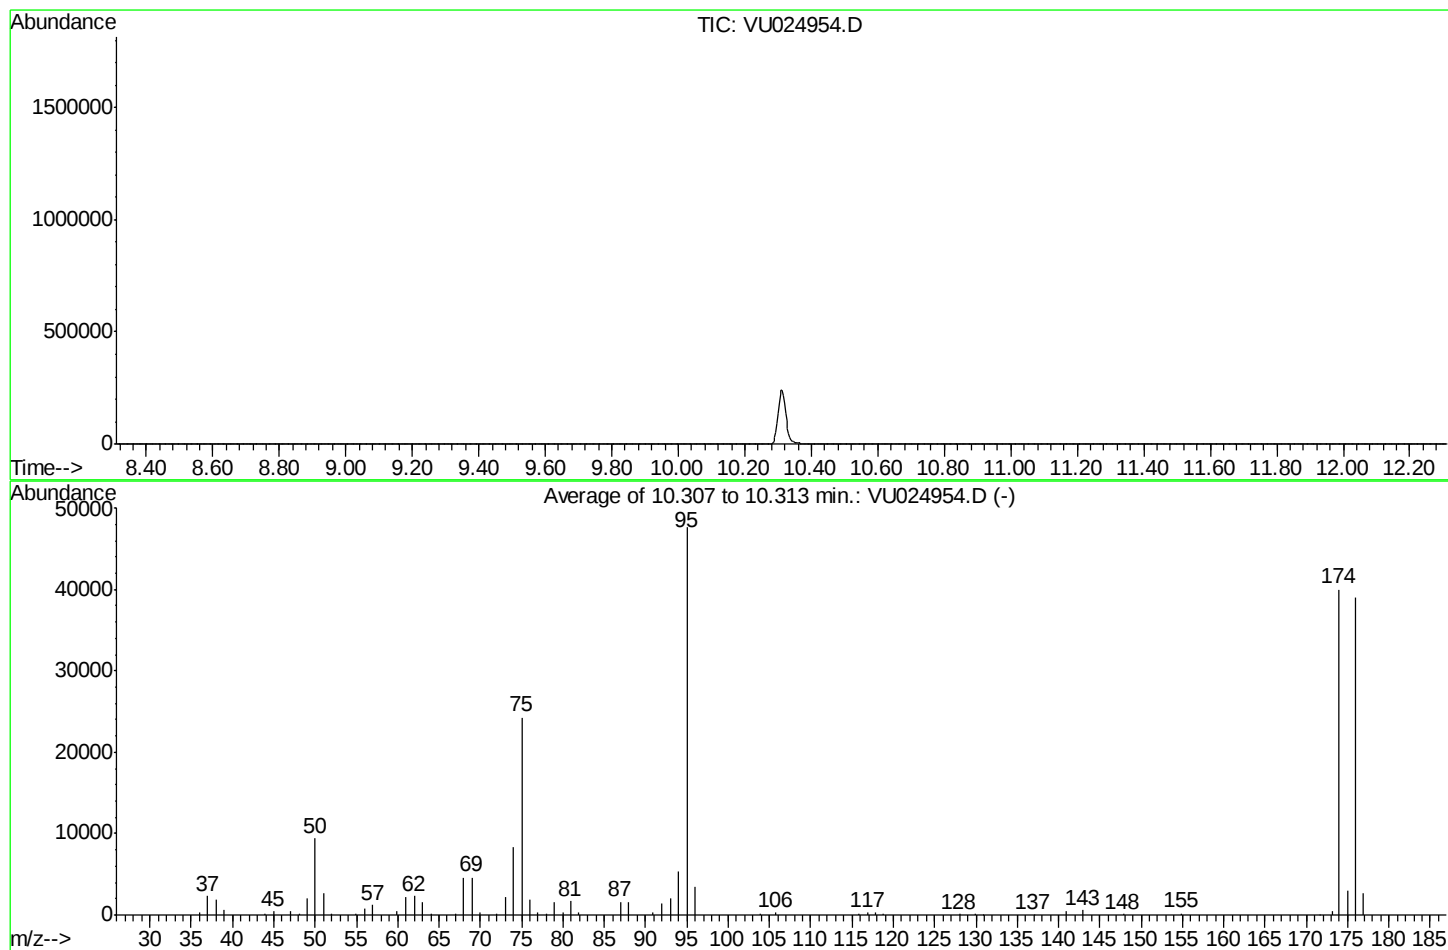

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	9412	PASS
75	95	30	60	51.0	24288	PASS
95	95	100	100	100.0	47629	PASS
96	95	5	9	7.2	3447	PASS
173	174	0.00	2	1.3	502	PASS
174	95	50	100	84.0	40008	PASS
175	174	5	9	7.4	2953	PASS
176	174	95	101	97.5	38989	PASS
177	176	5	9	6.9	2699	PASS