


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062719\
Data File : VU033052.D
Acq On : 27 Jun 2019 09:10
Operator : JC/SP
Sample : BFB21
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB21

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Jun 29 03:29:42 2019

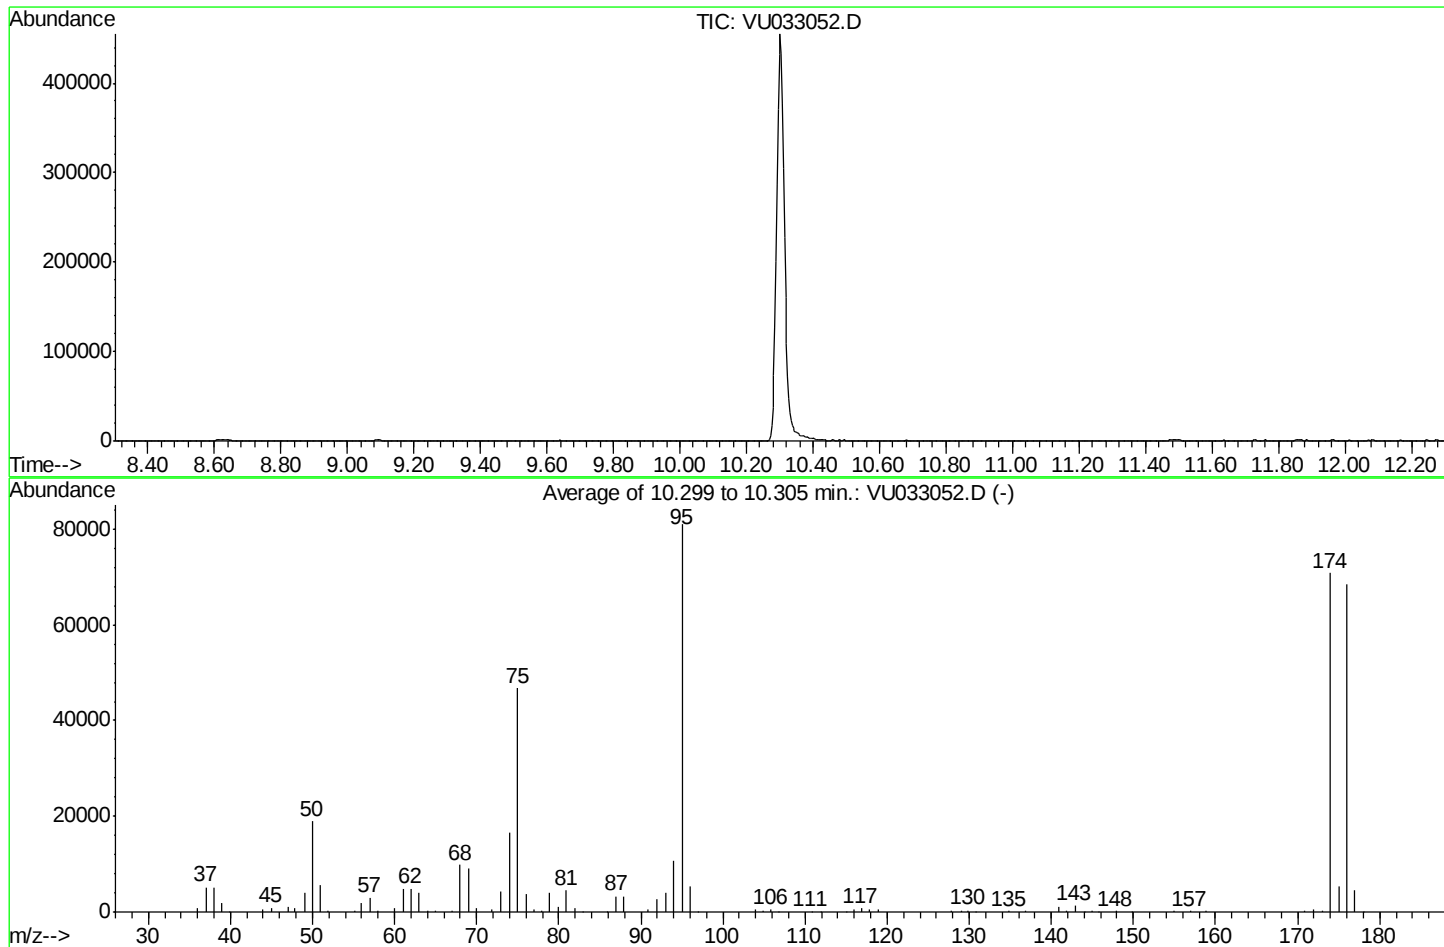

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	18896	PASS
75	95	30	80	57.7	46714	PASS
95	95	100	100	100.0	80994	PASS
96	95	5	9	6.7	5434	PASS
173	174	0.00	2	0.5	329	PASS
174	95	50	120	87.4	70818	PASS
175	174	5	9	7.6	5401	PASS
176	174	95	101	96.7	68448	PASS
177	176	5	9	6.6	4503	PASS

Scan 2851 (10.257 min): VU033052.D
BFB21

m/z	Abundance
39.90	123.0
43.90	405.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
36.00	939.0
37.00	5111.0
38.00	5226.0
39.00	1858.0
39.90	219.0
44.00	1048.0
45.00	803.0
47.00	1023.0
47.90	709.0
49.00	3931.0
50.00	19048.0
51.00	5740.0
51.90	212.0
55.10	300.0
56.00	1854.0
57.00	3055.0
58.00	139.0
60.00	881.0
61.00	4870.0
62.00	4821.0
63.00	4052.0
64.00	337.0
65.00	391.0
67.10	222.0
68.00	9482.0
69.00	8999.0
69.90	787.0
71.90	510.0
73.00	4343.0
74.00	16616.0
75.00	46792.0
76.00	4019.0
77.00	555.0
77.90	309.0
78.90	4036.0
79.90	1051.0
80.90	4217.0
81.90	829.0
85.80	104.0
87.00	3457.0
87.90	3197.0
90.90	432.0
92.00	2715.0
93.00	3863.0
94.00	10595.0
95.00	79704.0
96.00	5382.0
97.00	122.0
103.90	364.0
104.90	156.0
105.90	534.0
106.80	108.0
115.00	110.0
115.90	458.0
116.90	720.0
117.90	417.0
118.90	577.0
127.90	339.0
129.00	159.0
129.80	415.0
130.80	118.0
134.80	157.0
136.90	203.0
140.90	1162.0
141.90	165.0
142.90	1303.0
144.90	248.0
145.80	104.0
147.80	201.0
155.10	146.0
156.90	182.0
158.90	156.0
170.80	145.0
172.00	549.0
174.00	68304.0
175.00	5325.0
176.00	65360.0
177.00	4373.0
178.10	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
36.00	901.0
37.00	5249.0
38.00	5198.0
39.00	1944.0
39.90	195.0
44.00	994.0
45.00	849.0
47.00	1094.0
47.90	705.0
49.00	4261.0
50.00	19616.0
51.00	5916.0
51.90	242.0
55.10	297.0
56.00	1892.0
57.00	3101.0
58.00	150.0
60.00	968.0
61.00	5003.0
62.00	5044.0
63.00	4158.0
64.00	391.0
65.00	355.0
67.00	254.0
68.00	10162.0
69.00	9345.0
69.90	742.0
71.90	589.0
73.00	4325.0
74.00	17088.0
75.00	48352.0
76.00	3957.0
77.00	504.0
77.90	316.0
78.90	4285.0
79.90	1124.0
80.90	4565.0
81.90	828.0
82.90	123.0
85.90	101.0
87.00	3402.0
87.90	3312.0
90.90	482.0
92.00	2934.0
93.00	4281.0
94.00	11037.0
95.00	83368.0
96.00	5573.0
97.00	123.0
103.90	430.0
104.90	162.0
105.90	552.0
106.80	111.0
110.80	107.0
115.90	463.0
116.90	720.0
117.90	441.0
118.90	606.0
127.90	347.0
129.00	151.0
129.90	402.0
130.80	122.0
134.90	196.0
136.80	190.0
141.00	1141.0
141.90	199.0
142.90	1372.0
144.10	105.0
144.90	263.0
145.80	131.0
147.90	199.0
149.80	122.0
154.90	177.0
156.90	217.0
158.90	176.0
170.80	153.0
171.90	614.0
173.10	987.0
174.00	73400.0
175.00	5585.0
176.00	70688.0
177.00	4684.0
177.90	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21

m/z	Abundance
36.00	865.0
37.00	5034.0
38.00	4817.0
39.00	1865.0
39.90	179.0
44.00	904.0
45.00	842.0
47.00	962.0
47.90	637.0
49.00	4121.0
50.00	18024.0
51.00	5485.0
51.90	242.0
55.10	268.0
56.00	1808.0
57.00	2889.0
58.00	144.0
60.00	994.0
61.00	4593.0
62.00	4775.0
63.00	3768.0
64.00	405.0
65.10	327.0
67.00	263.0
68.00	9755.0
69.00	9133.0
70.00	670.0
71.90	605.0
73.00	3872.0
74.00	16229.0
75.00	45000.0
76.00	3668.0
77.00	431.0
77.90	317.0
78.90	4134.0
79.90	1084.0
80.90	4521.0
81.90	776.0
82.90	137.0
87.00	2996.0
87.90	3020.0
90.90	443.0
92.00	2760.0
93.00	4174.0
94.00	10701.0
95.00	79912.0
96.00	5349.0
97.00	115.0
103.90	445.0
104.90	151.0
105.90	507.0
110.80	121.0
111.90	104.0
115.90	383.0
116.90	639.0
117.90	399.0
118.90	587.0
127.80	320.0
129.00	138.0
129.90	322.0
130.90	116.0
134.80	214.0
136.80	163.0
141.00	1109.0
141.80	217.0
142.90	1335.0
144.90	242.0
145.80	142.0
147.90	192.0
149.90	131.0
154.90	182.0
156.90	222.0
158.90	157.0
170.80	136.0
171.90	625.0
174.00	70752.0
175.00	5294.0
176.00	69296.0
177.00	4454.0

Instrument :
MSVOA_U
ClientSampleId :
BFB21