


Chloromethane

Response Ratio

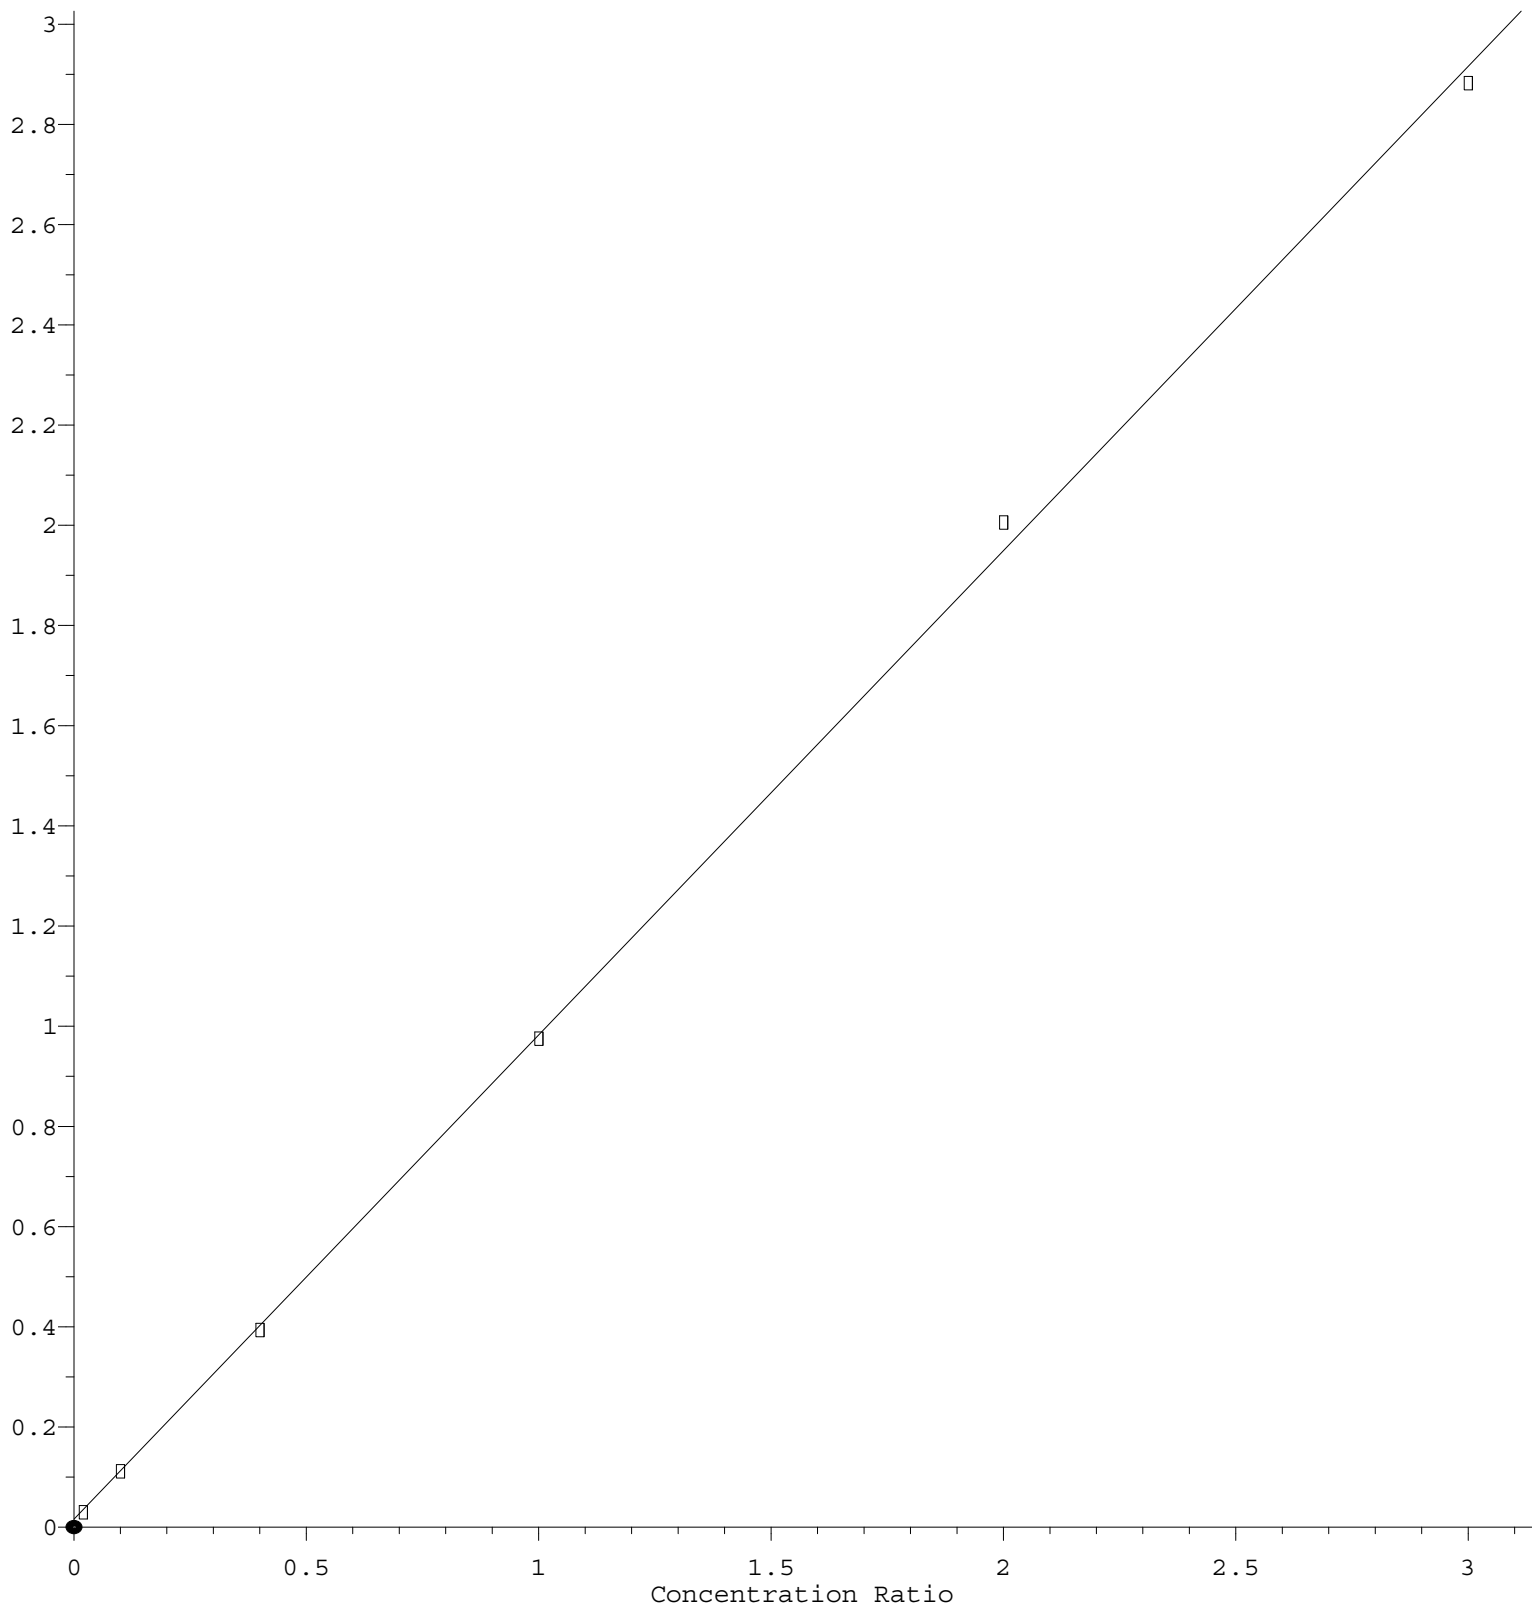

$$\text{Response} = 9.668\text{e-}001 * \text{Amt} + 1.569\text{e-}002$$


Coef of Det (r^2) = 0.999330 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U062722W.M

Calibration Table Last Updated: Tue Jun 28 10:35:43 2022

Chloroethane

Response Ratio

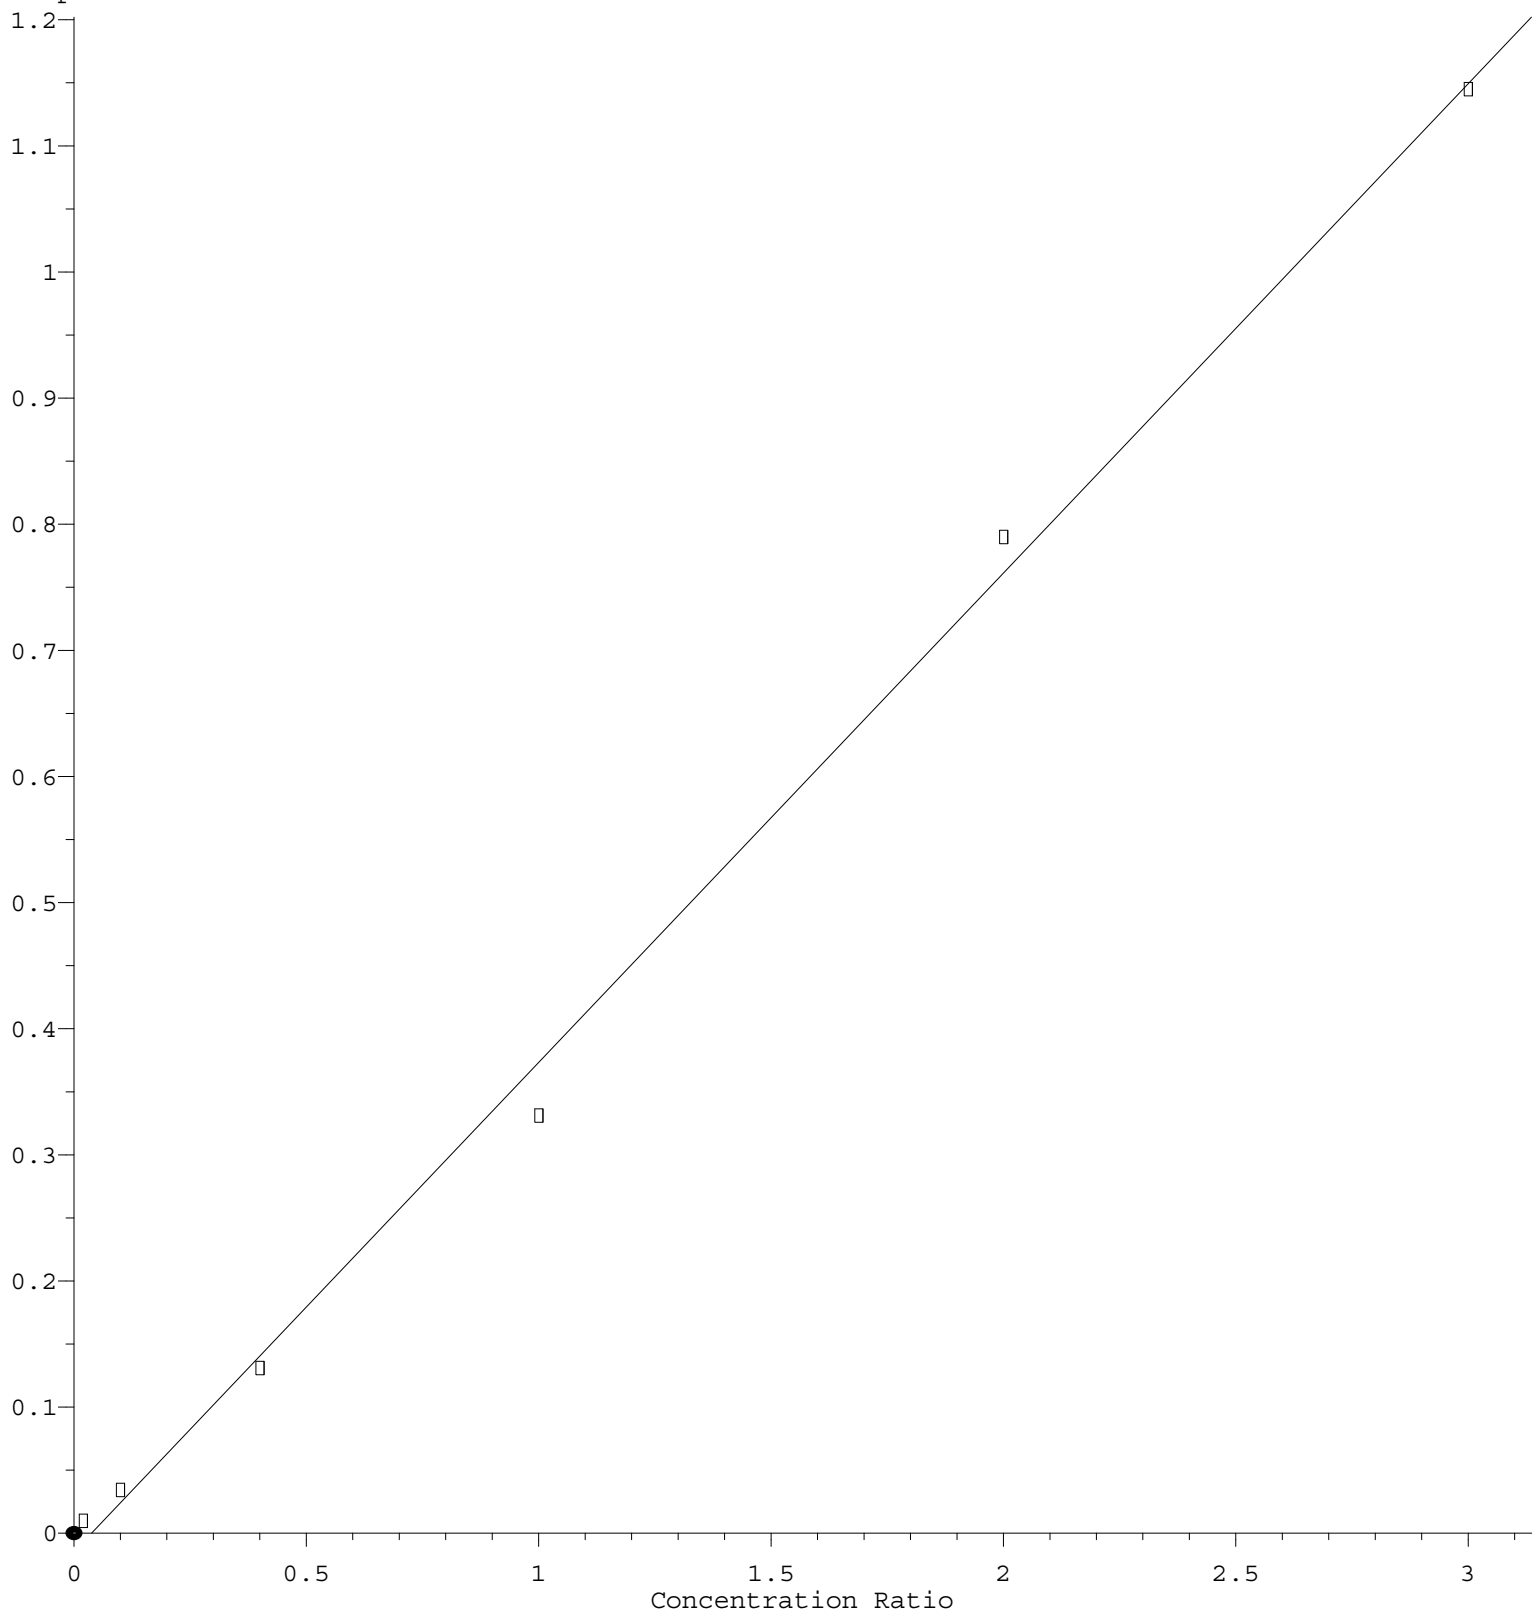

$$\text{Response} = 3.880\text{e-}001 * \text{Amt} - 1.486\text{e-}002$$


Coef of Det (r^2) = 0.997111 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U062722W.M

Calibration Table Last Updated: Tue Jun 28 10:35:43 2022

Methyl Iodide

Response Ratio

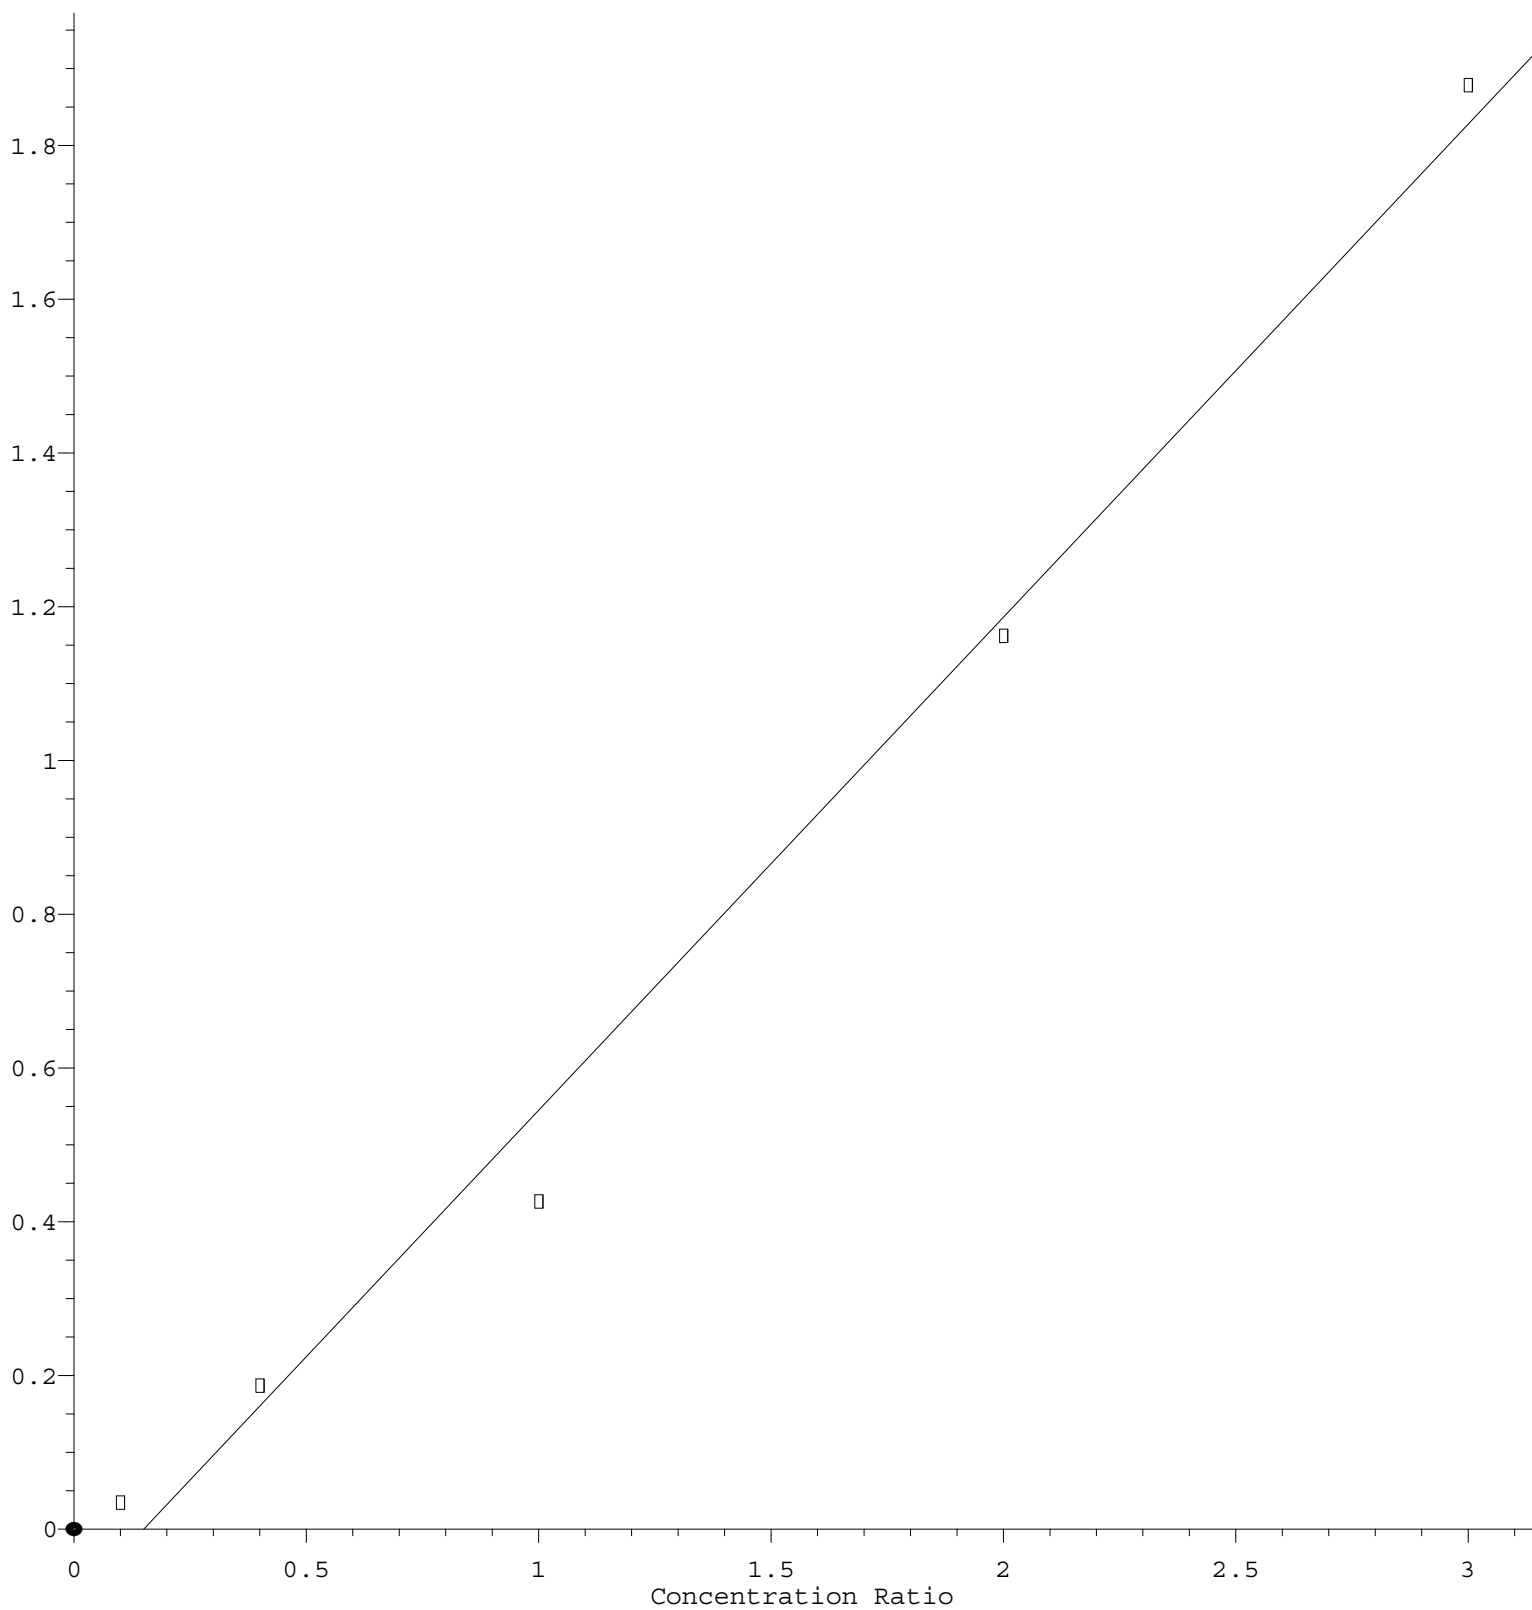

$$\text{Response} = 6.415\text{e-}001 * \text{Amt} - 9.639\text{e-}002$$


Coef of Det (r^2) = 0.990560 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U062722W.M

Calibration Table Last Updated: Tue Jun 28 10:35:43 2022

Methylene Chloride

Response Ratio

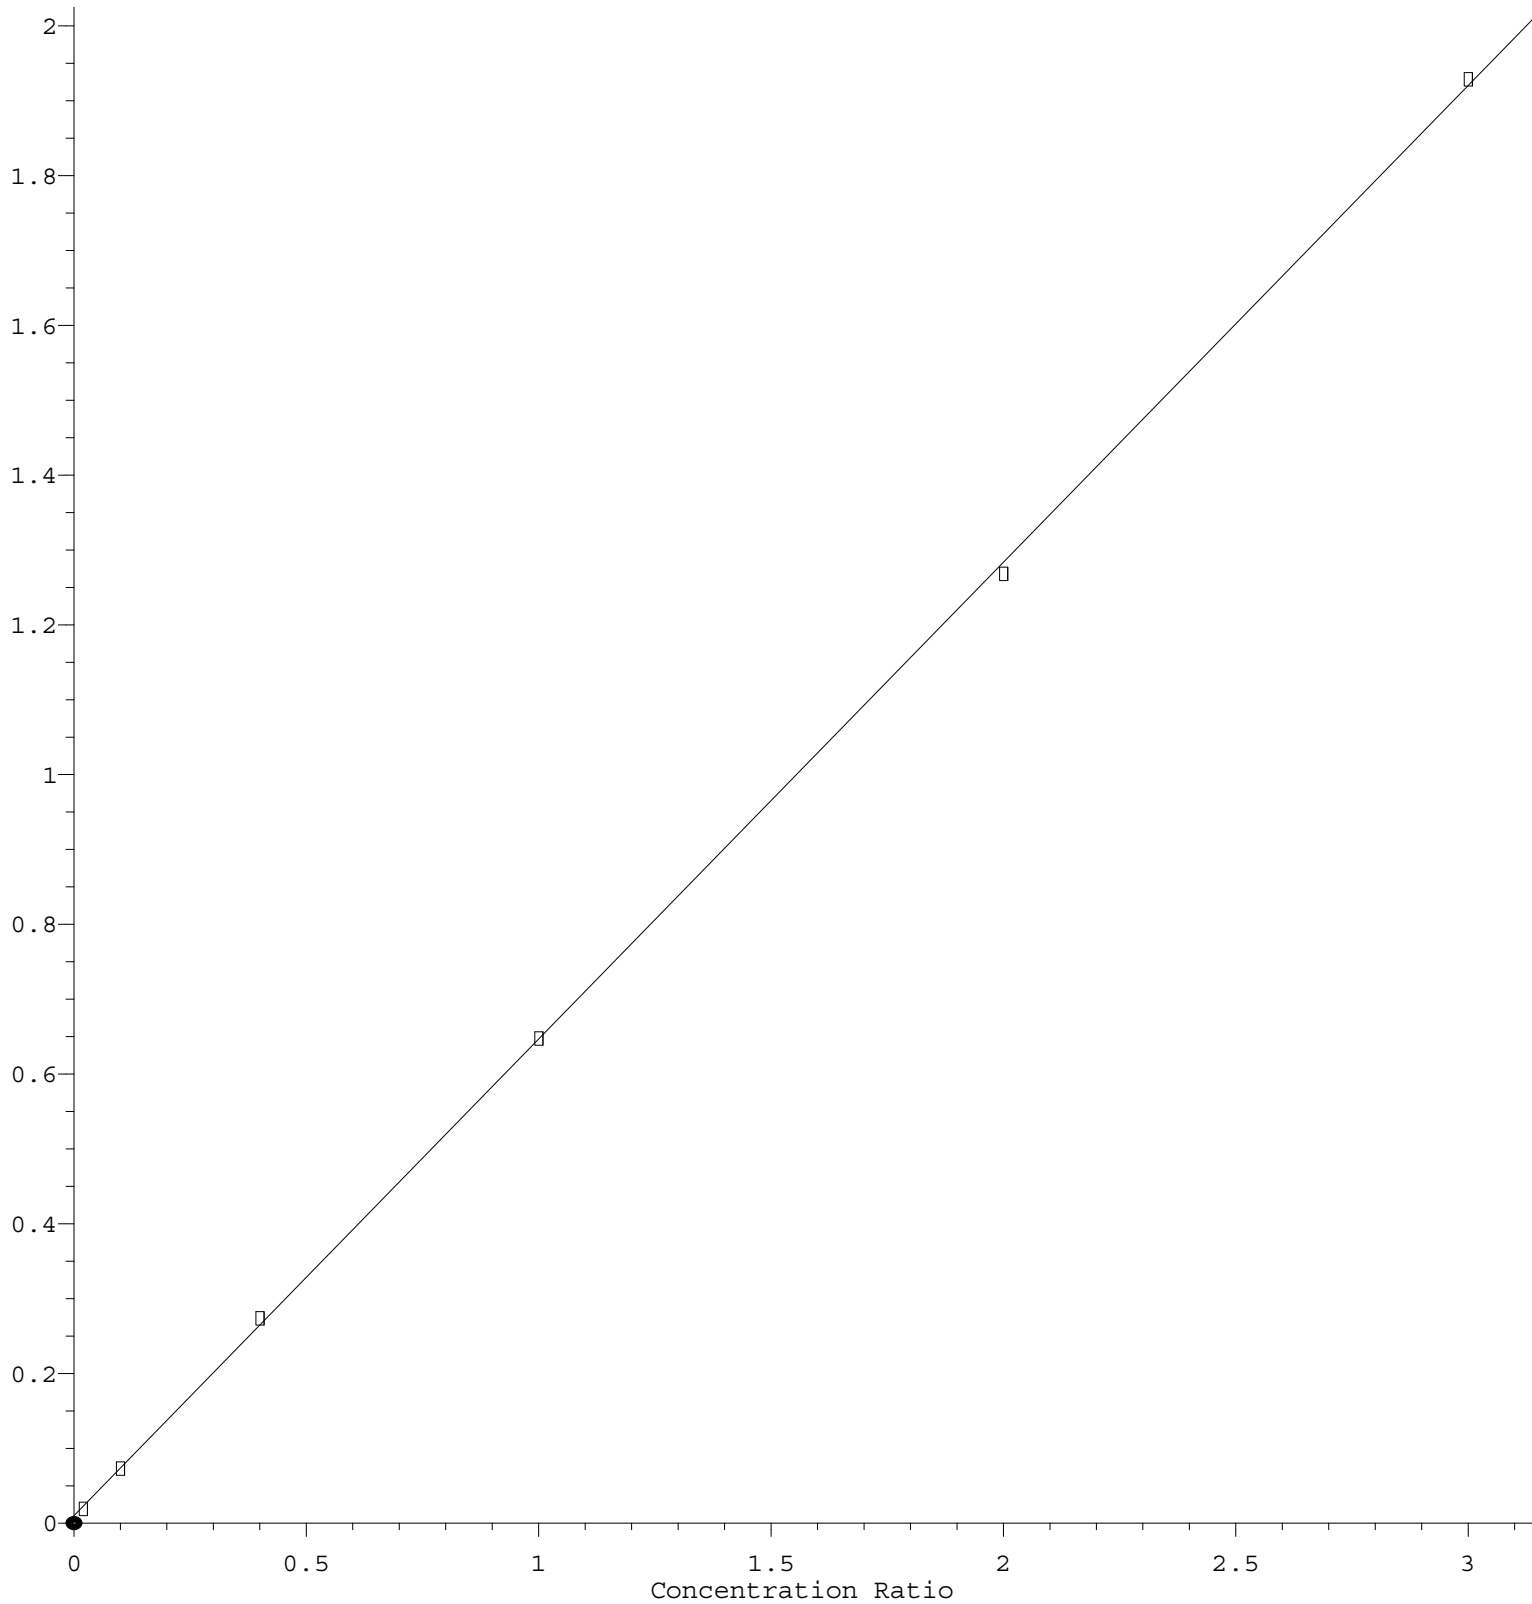


$$\text{Response} = 6.368\text{e-}001 * \text{Amt} + 9.601\text{e-}003$$

Coef of Det (r^2) = 0.999859 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U062722W.M

Calibration Table Last Updated: Tue Jun 28 10:35:43 2022


2-Chloroethyl Vinyl ether

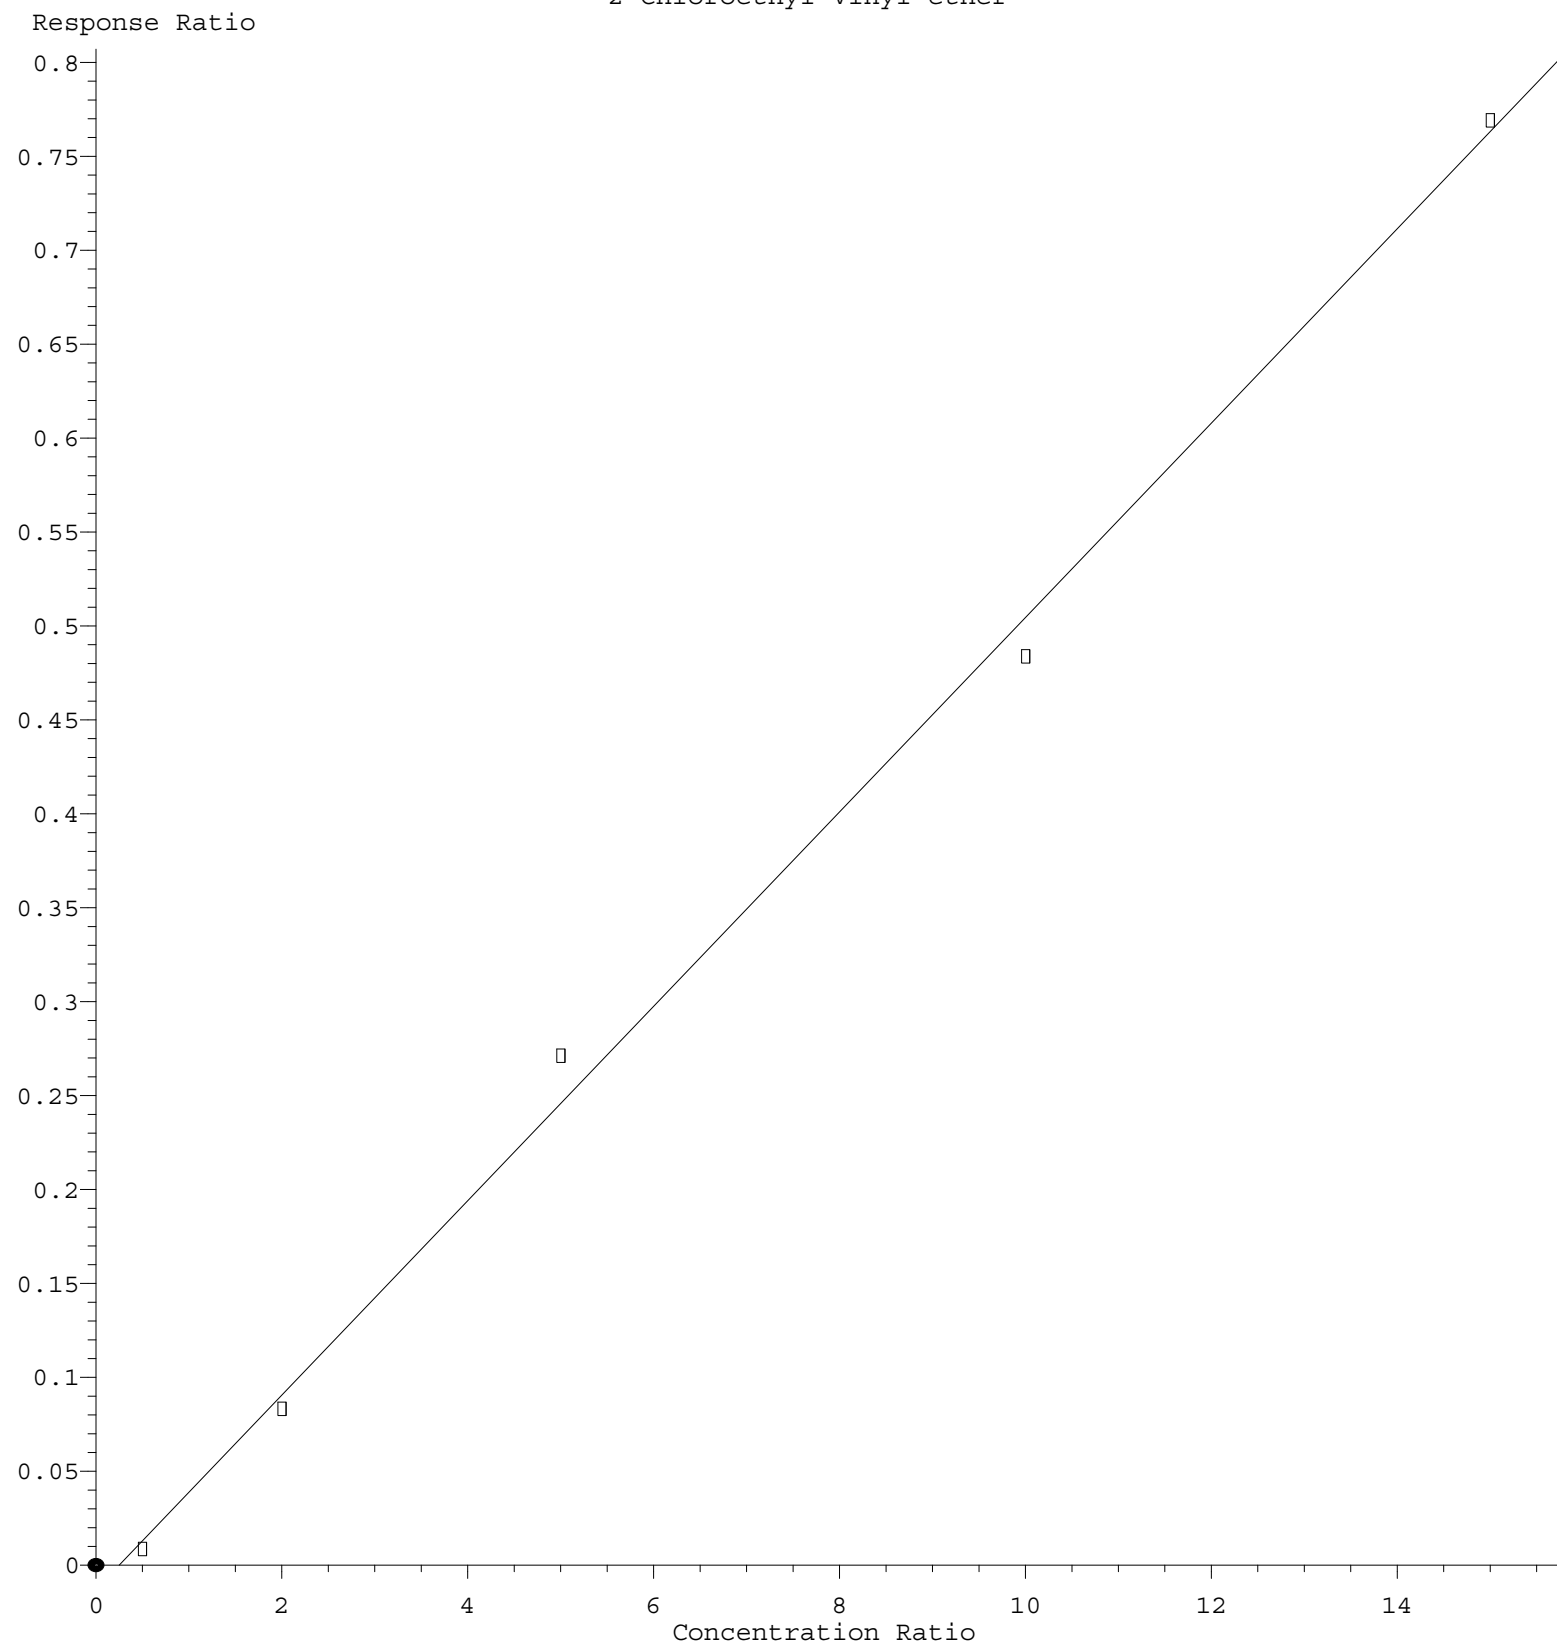

Response = $5.173 \times 10^{-2} \times \text{Amt} - 1.309 \times 10^{-2}$
Coef of Det (r^2) = 0.996921 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U062722W.M
Calibration Table Last Updated: Tue Jun 28 10:35:43 2022

1,2,4-Trichlorobenzene

Response Ratio

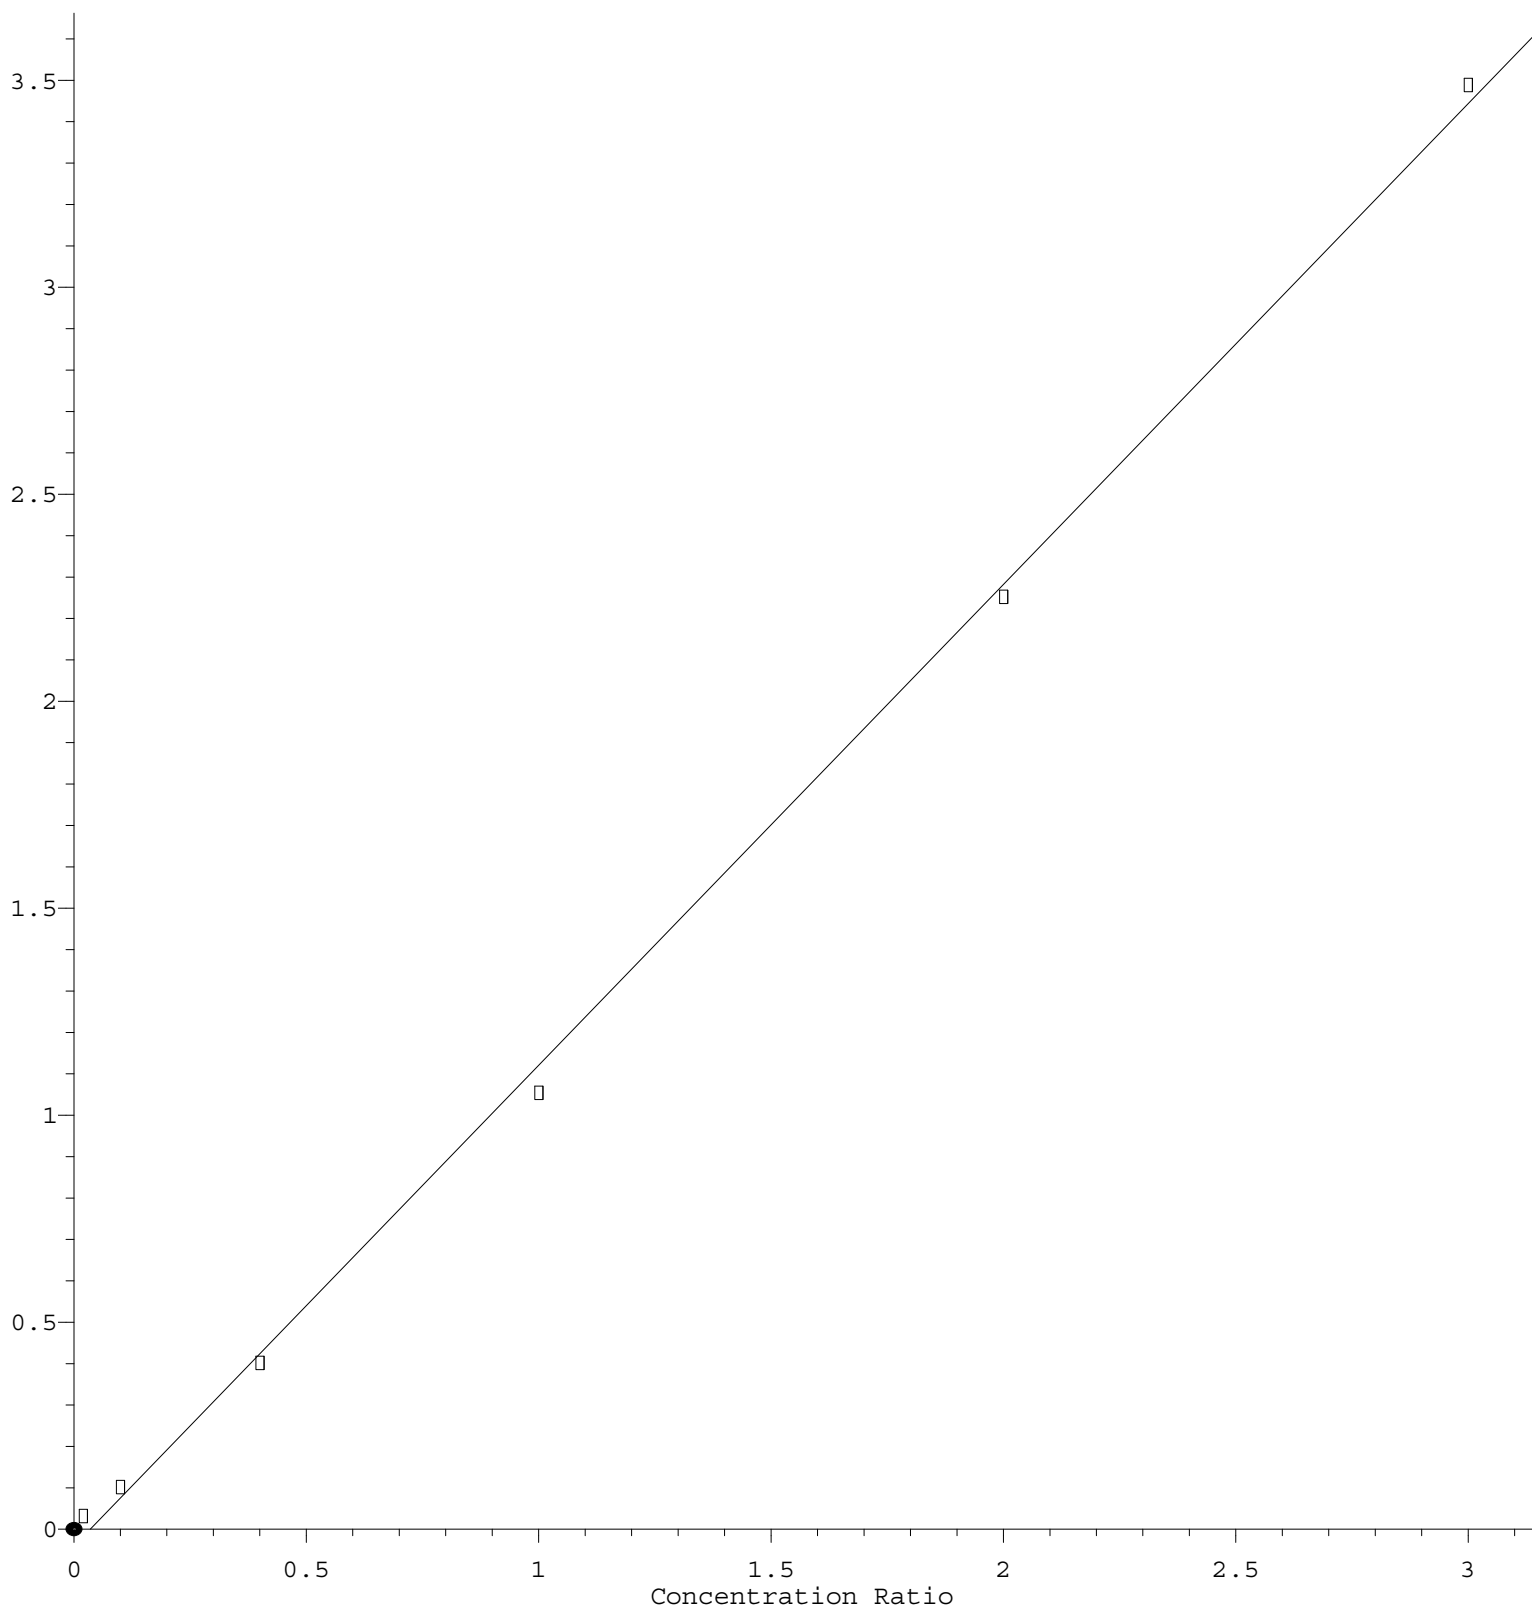

$$\text{Response} = 1.162\text{e}+000 * \text{Amt} - 4.074\text{e}-002$$


Coef of Det (r^2) = 0.998850 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U062722W.M

Calibration Table Last Updated: Tue Jun 28 10:35:43 2022

Naphthalene


Response Ratio

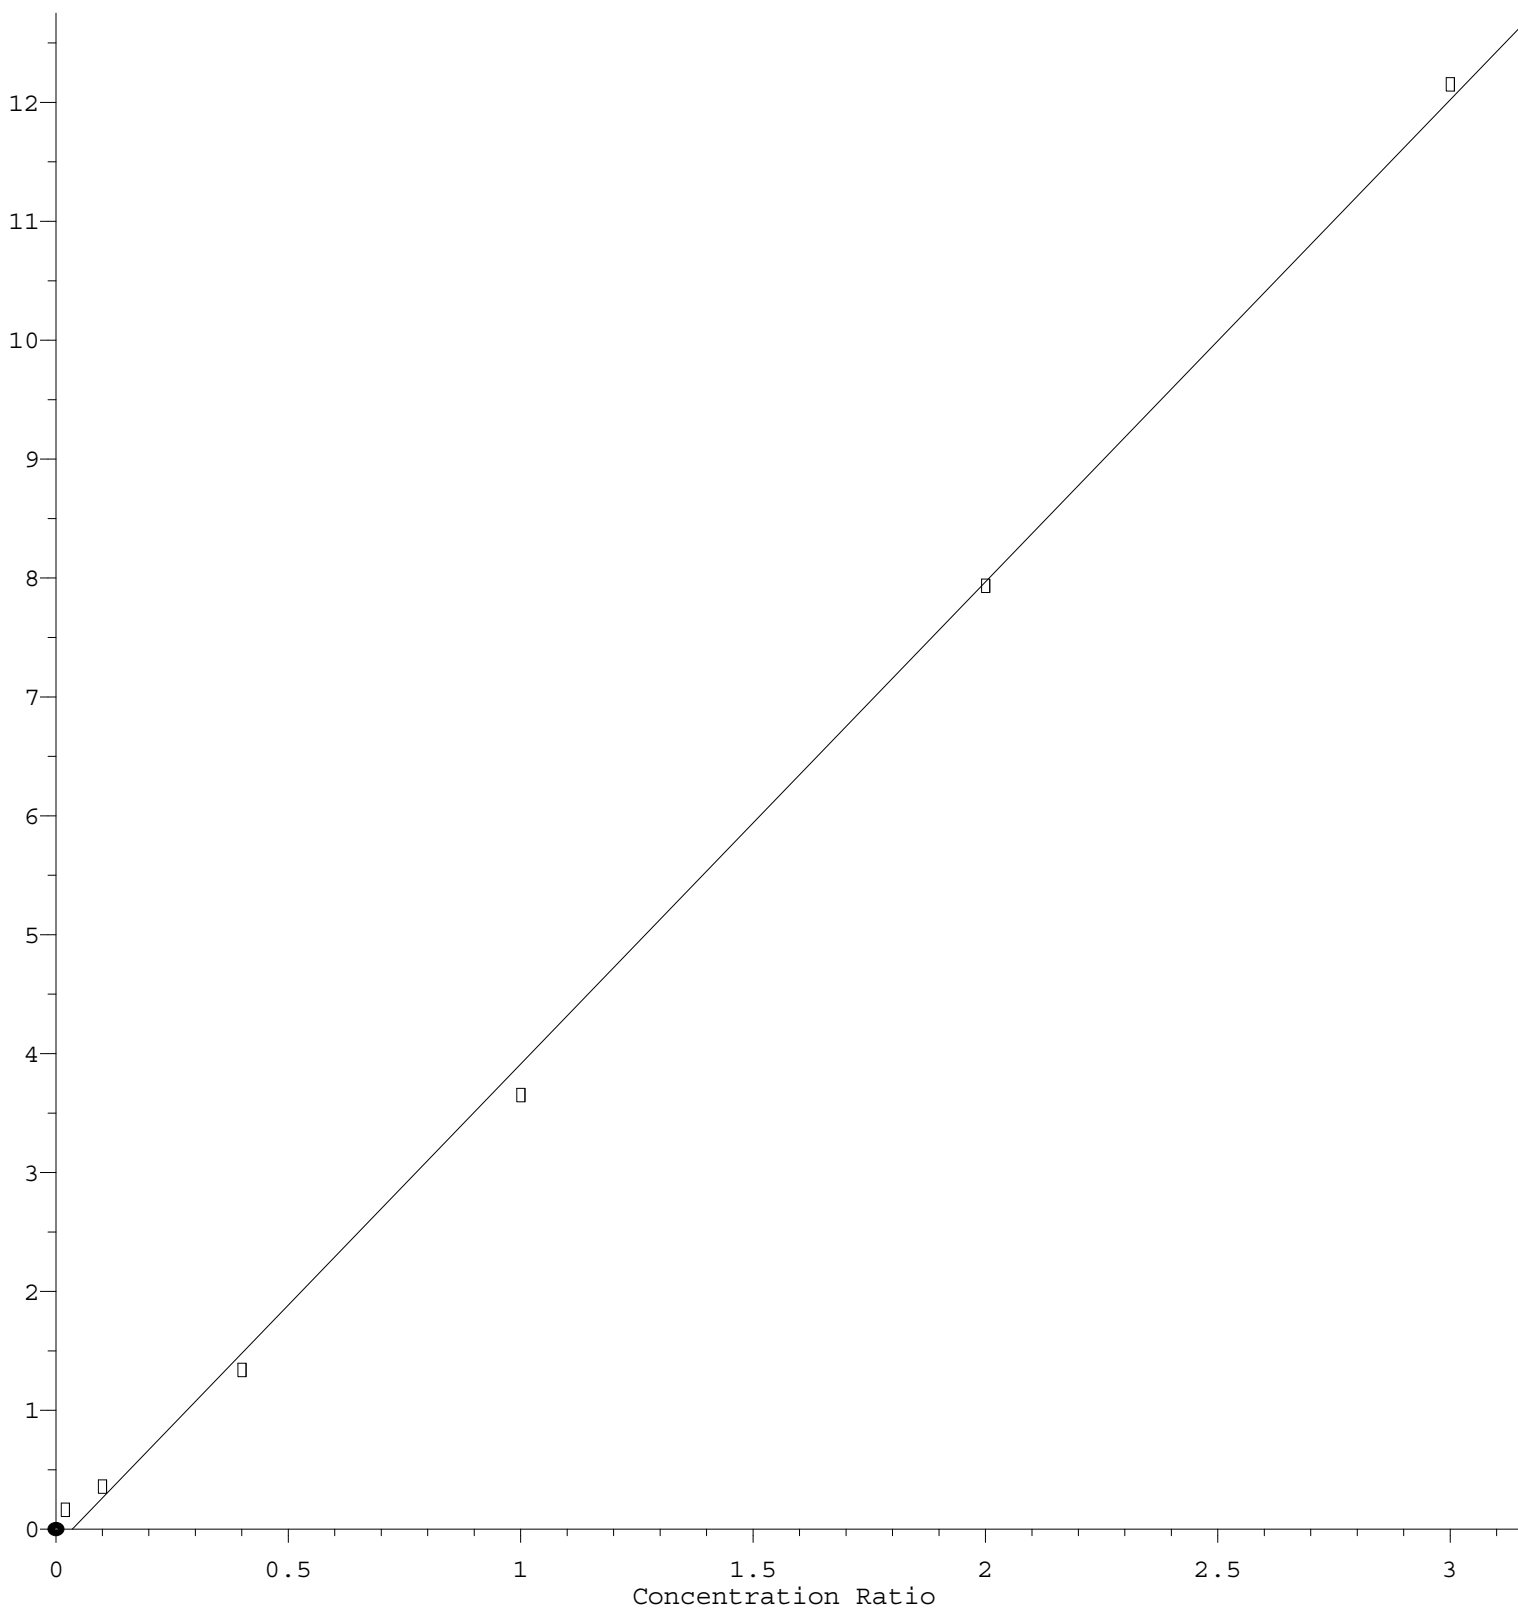

Response = 4.055e+000 * Amt - 1.408e-001
 Coef of Det (r^2) = 0.998582 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U062722W.M
 Calibration Table Last Updated: Tue Jun 28 10:35:43 2022

1,2,3-Trichlorobenzene

Response Ratio

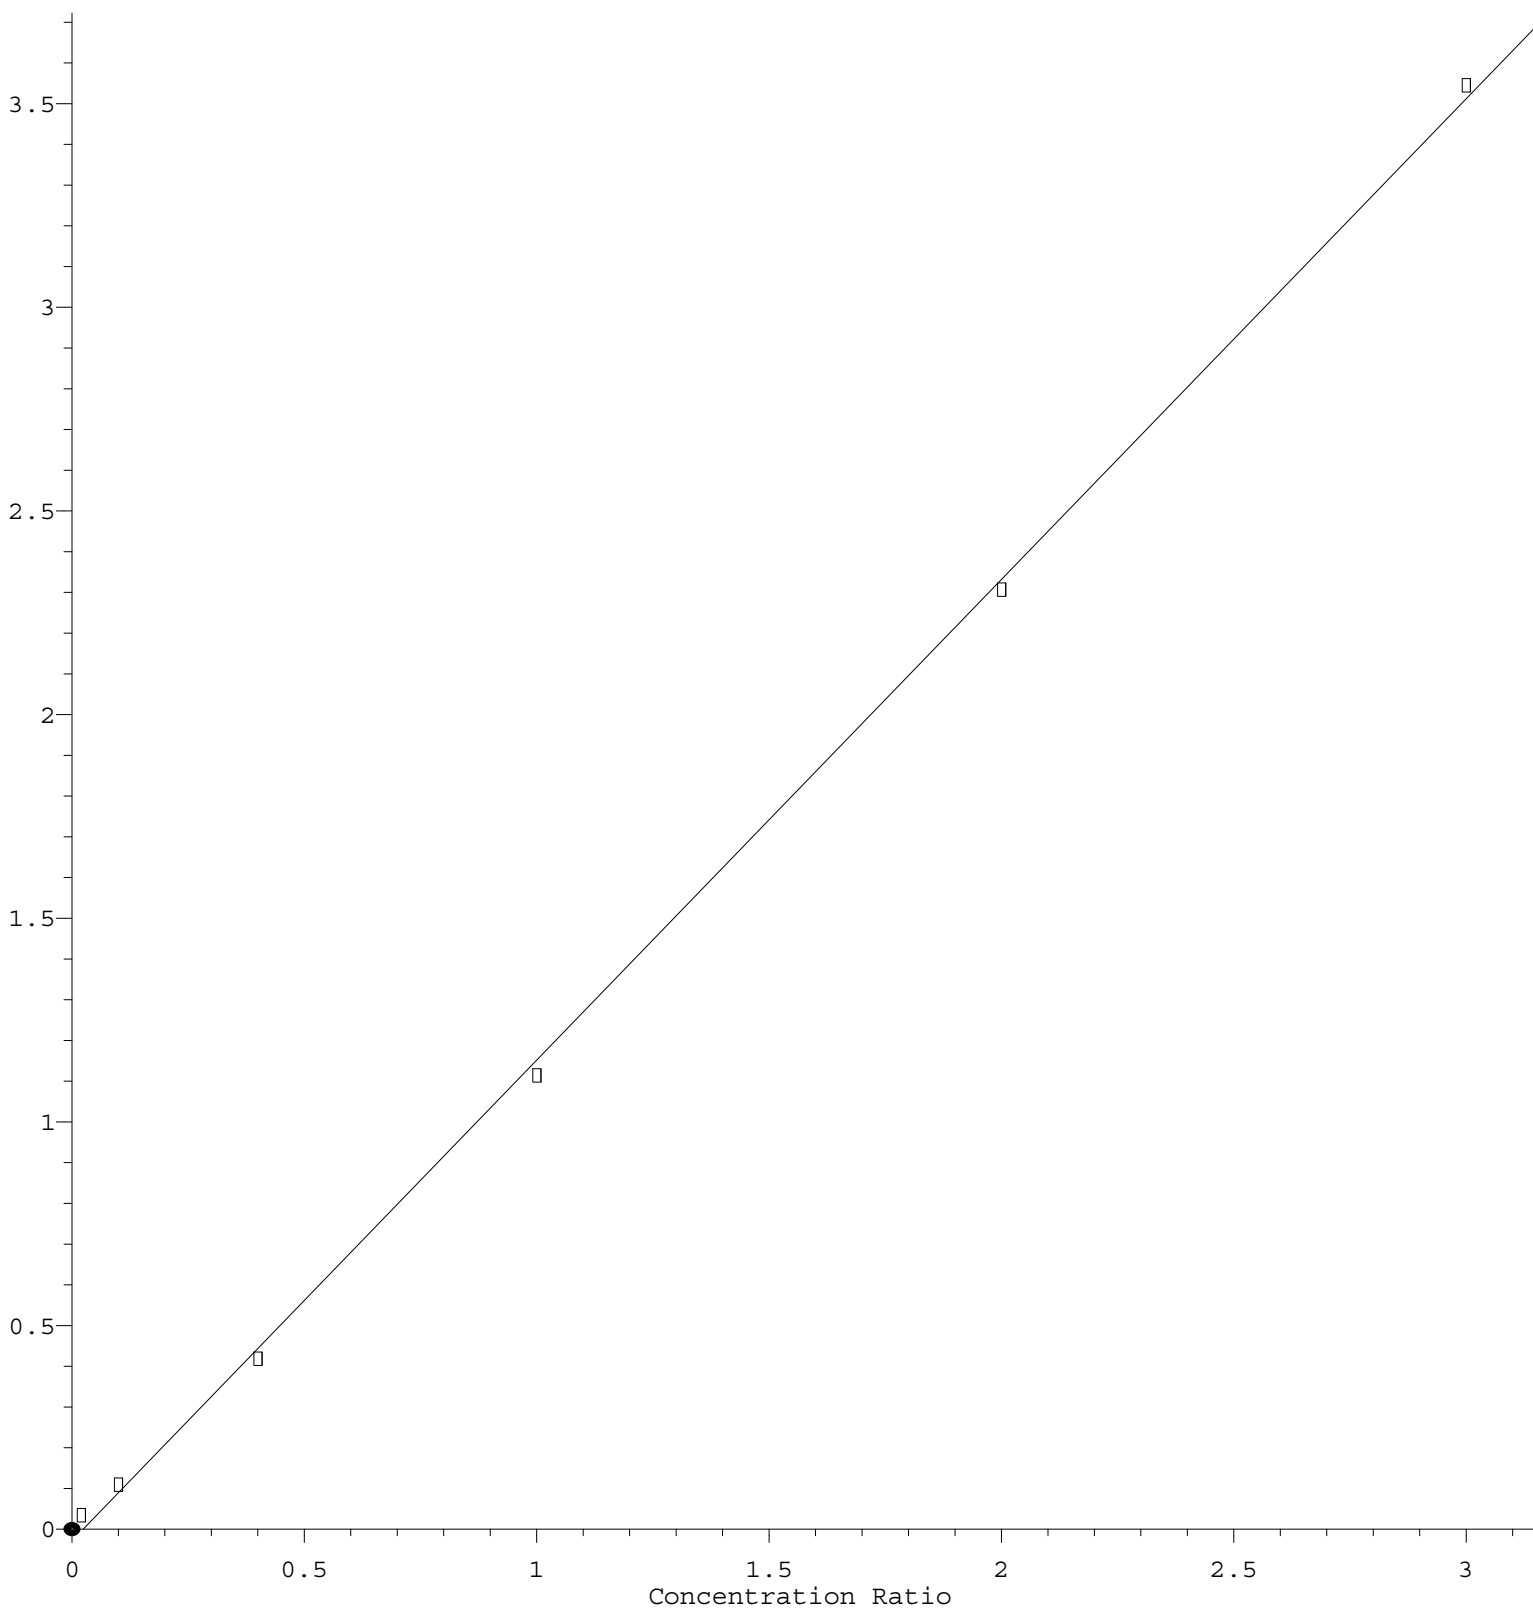

$$\text{Response} = 1.180\text{e}+000 * \text{Amt} - 2.778\text{e}-002$$

Coef of Det (r^2) = 0.999423 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA U\Method\82U062722W.M

Calibration Table Last Updated: Tue Jun 28 10:35:43 2022