

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
 Data File : VU049420.D
 Acq On : 27 Jun 2022 22:45
 Operator : SY/MD
 Sample : VU0627MBL02
 Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0627MBL02

Quant Time: Jun 28 05:29:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 28 05:14:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.372	168	295686	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.250	114	502361	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.417	117	447442	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	207041	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.700	65	190460	41.825	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	83.640%
35) Dibromofluoromethane	5.288	113	154528	43.967	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	87.940%
50) Toluene-d8	7.896	98	598045	47.707	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.420%
62) 4-Bromofluorobenzene	10.632	95	218319	45.464	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.920%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049420.D
Acq On : 27 Jun 2022 22:45
Operator : SY/MD
Sample : VU0627MBL02
Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0627MBL02

Quant Time: Jun 28 05:29:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 28 05:14:22 2022
Response via : Initial Calibration




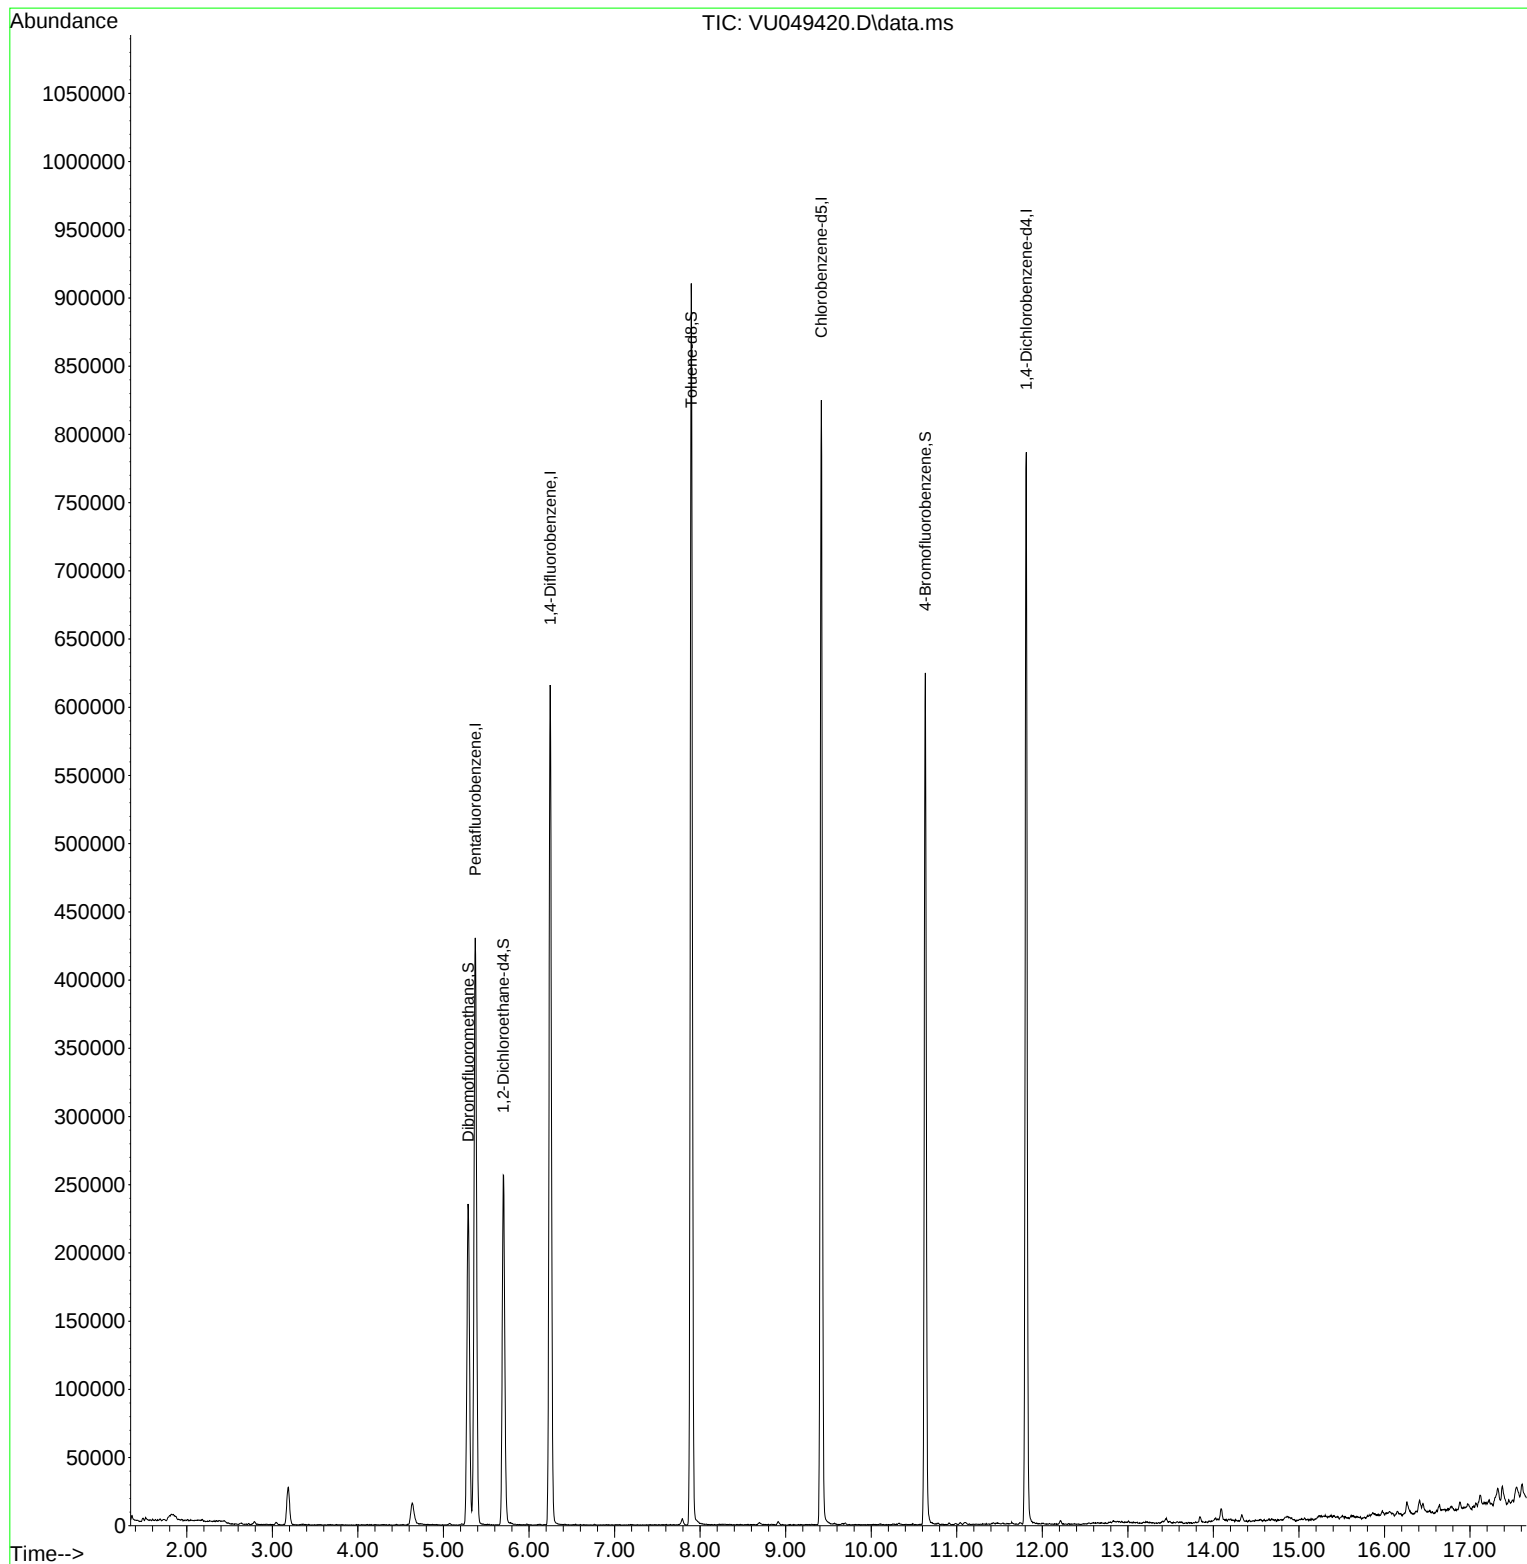


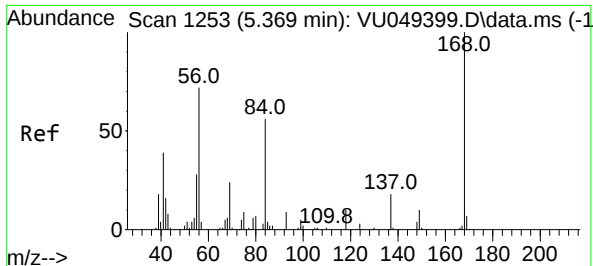

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.372 min Scan# 11
Delta R.T. 0.003 min
Lab File: VU049420.D
Acq: 27 Jun 2022 22:45




Instrument :
MSVOA_U
ClientSampleId :
VU0627MBL02


Tgt Ion:168 Resp: 295686
Ion Ratio Lower Upper
168 100
99 59.9 39.3 58.9#

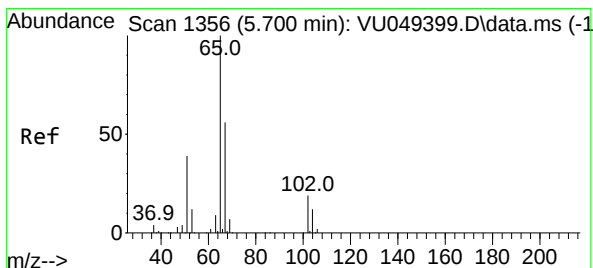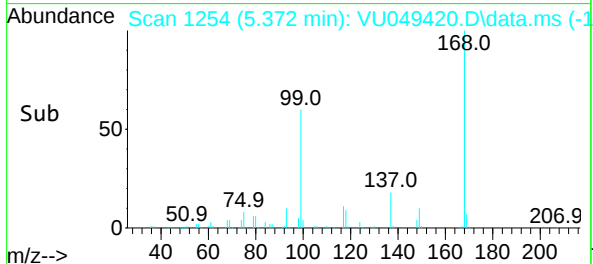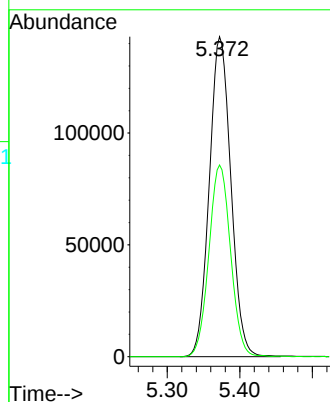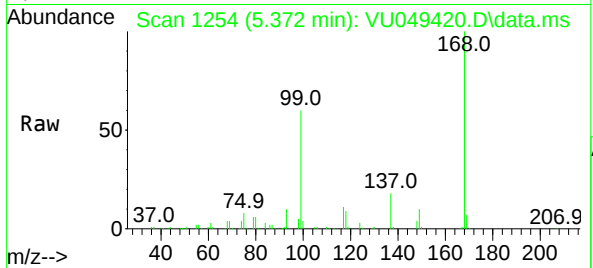

#33
1,2-Dichloroethane-d4
Concen: 41.825 ug/l
RT: 5.700 min Scan# 1356
Delta R.T. 0.000 min
Lab File: VU049420.D
Acq: 27 Jun 2022 22:45

Tgt Ion: 65 Resp: 190460
Ion Ratio Lower Upper
65 100
67 54.3 0.0 108.0

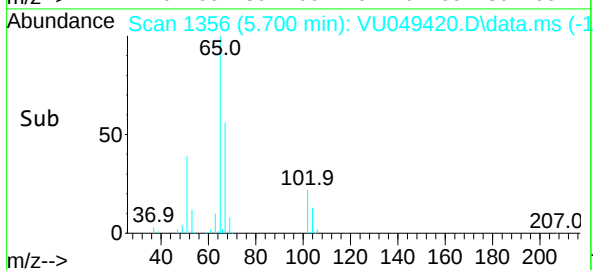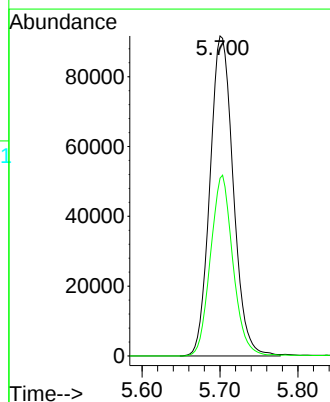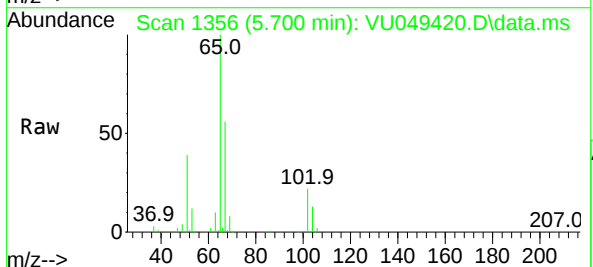

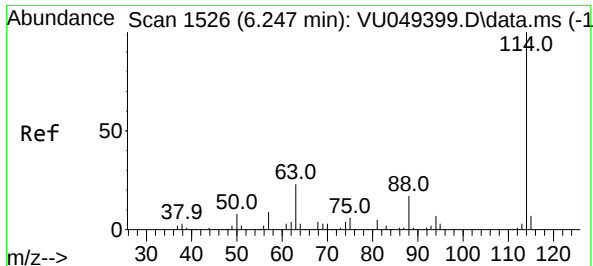

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.250 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU049420.D

Acq: 27 Jun 2022 22:45

Instrument :

MSVOA_U

ClientSampleId :

VU0627MBL02





Tgt Ion:114 Resp: 502361

Ion Ratio Lower Upper

114 100

63 22.0 0.0 37.8

88 16.0 0.0 29.2

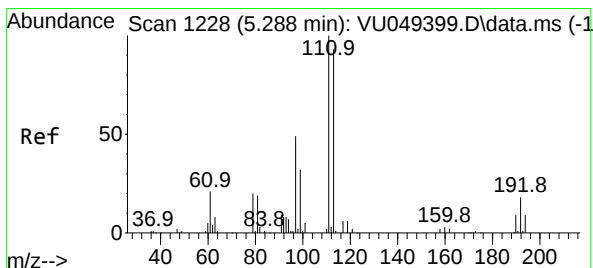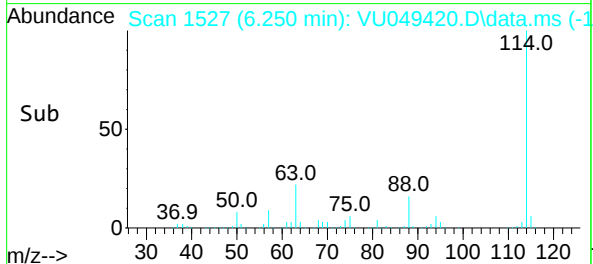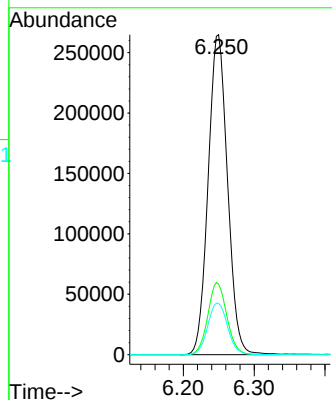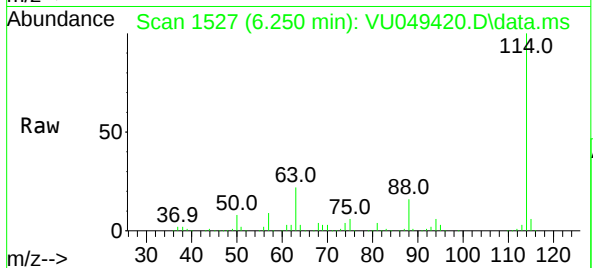

#35

Dibromofluoromethane

Concen: 43.967 ug/l

RT: 5.288 min Scan# 1228

Delta R.T. 0.000 min

Lab File: VU049420.D

Acq: 27 Jun 2022 22:45




Tgt Ion:113 Resp: 154528


Ion Ratio Lower Upper

113 100

111 103.5 82.1 123.1

192 18.6 18.0 27.0


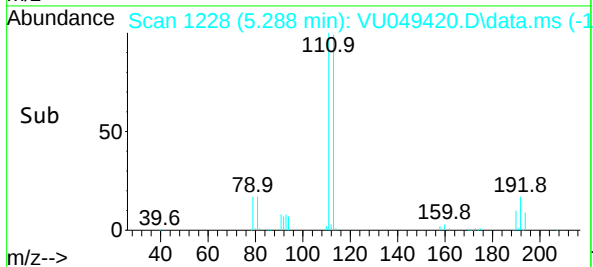
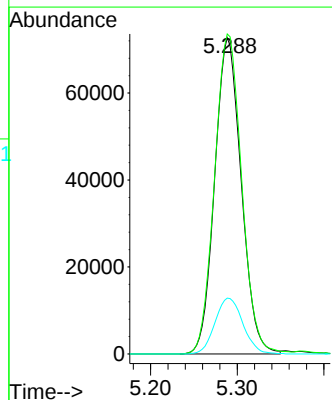
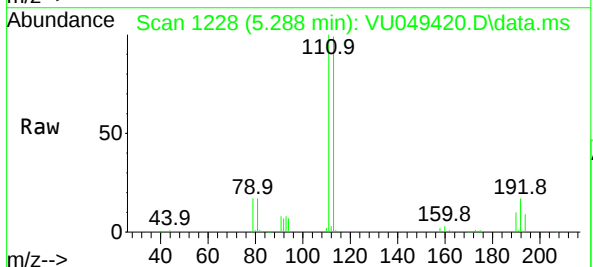


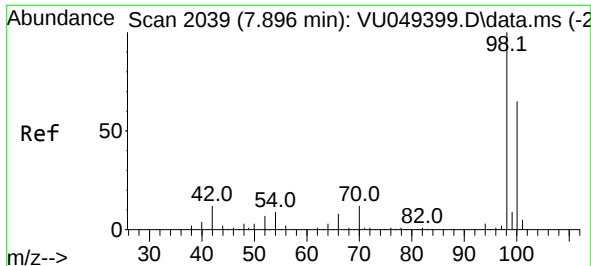

#50
Toluene-d8
Concen: 47.707 ug/l
RT: 7.896 min Scan# 2039
Delta R.T. 0.000 min
Lab File: VU049420.D
Acq: 27 Jun 2022 22:45




Instrument :
MSVOA_U
ClientSampleId :
VU0627MBL02


Tgt Ion: 98 Resp: 598045
Ion Ratio Lower Upper
98 100
100 64.6 51.7 77.5

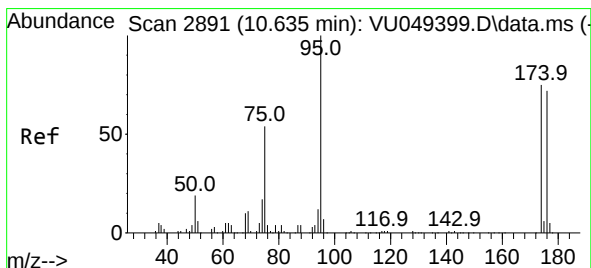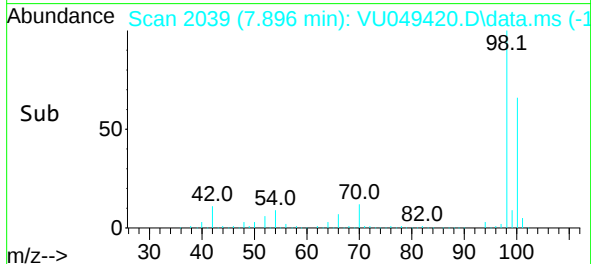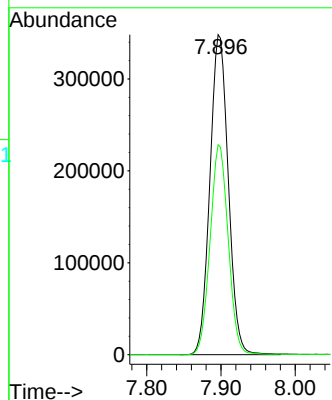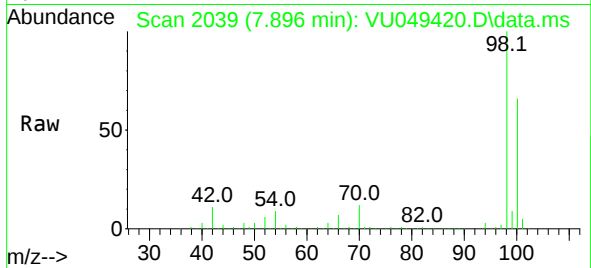

#62
4-Bromofluorobenzene
Concen: 45.464 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.003 min
Lab File: VU049420.D
Acq: 27 Jun 2022 22:45

Tgt Ion: 95 Resp: 218319
Ion Ratio Lower Upper
95 100
174 74.5 0.0 182.0
176 72.0 0.0 177.8


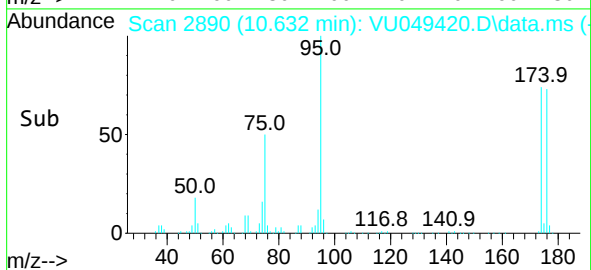
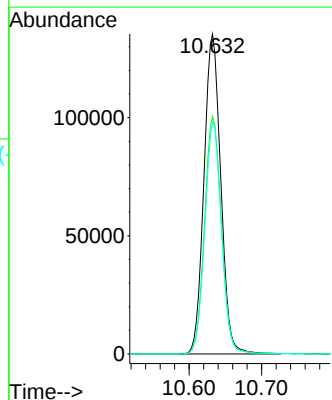
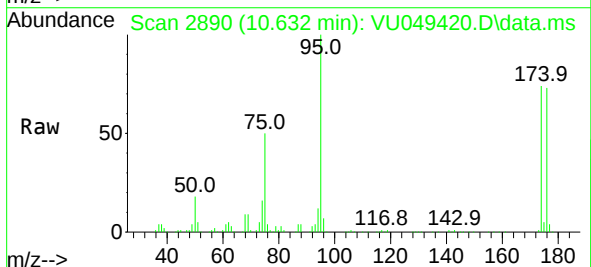


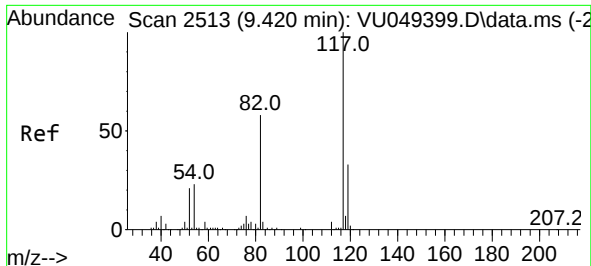

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.417 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU049420.D
Acq: 27 Jun 2022 22:45

Instrument :
MSVOA_U
ClientSampleId :
VU0627MBL02

Tgt Ion:117 Resp: 447442
Ion Ratio Lower Upper
117 100
82 59.4 41.7 62.5
119 32.3 25.7 38.5

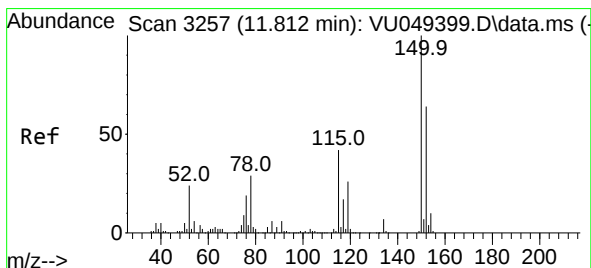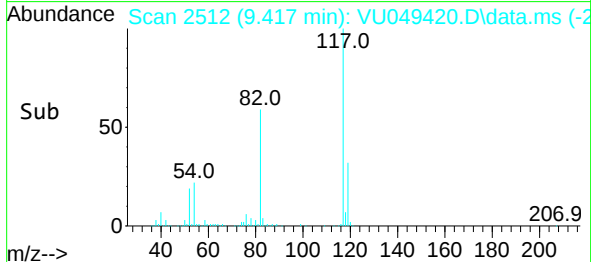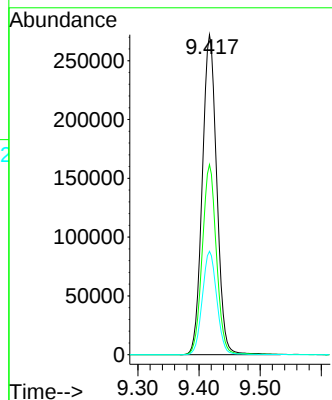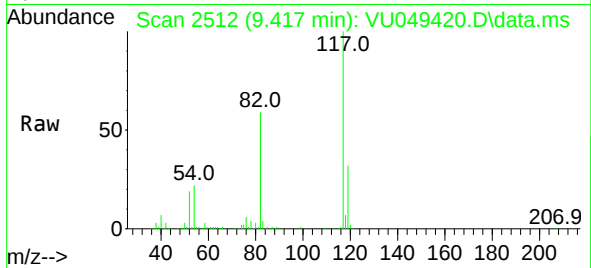

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.812 min Scan# 3257
Delta R.T. 0.000 min
Lab File: VU049420.D
Acq: 27 Jun 2022 22:45

Tgt Ion:152 Resp: 207041
Ion Ratio Lower Upper
152 100
115 62.6 37.0 110.9
150 157.6 0.0 342.2

