

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
 Data File : VU049437.D
 Acq On : 28 Jun 2022 05:26
 Operator : SY/MD
 Sample : N3482-09
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 FB062322

Quant Time: Jun 28 07:15:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 28 05:14:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.372	168	302500	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.250	114	520242	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.417	117	461942	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	209653	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.703	65	201703	43.296	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	86.600%
35) Dibromofluoromethane	5.289	113	159728	43.884	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	87.760%
50) Toluene-d8	7.896	98	612725	47.198	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.400%
62) 4-Bromofluorobenzene	10.632	95	219644	44.167	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	88.340%
Target Compounds						
16) Acetone	2.639	43	3403	1.448	ug/l	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049437.D
Acq On : 28 Jun 2022 05:26
Operator : SY/MD
Sample : N3482-09
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
FB062322

Quant Time: Jun 28 07:15:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 28 05:14:22 2022
Response via : Initial Calibration




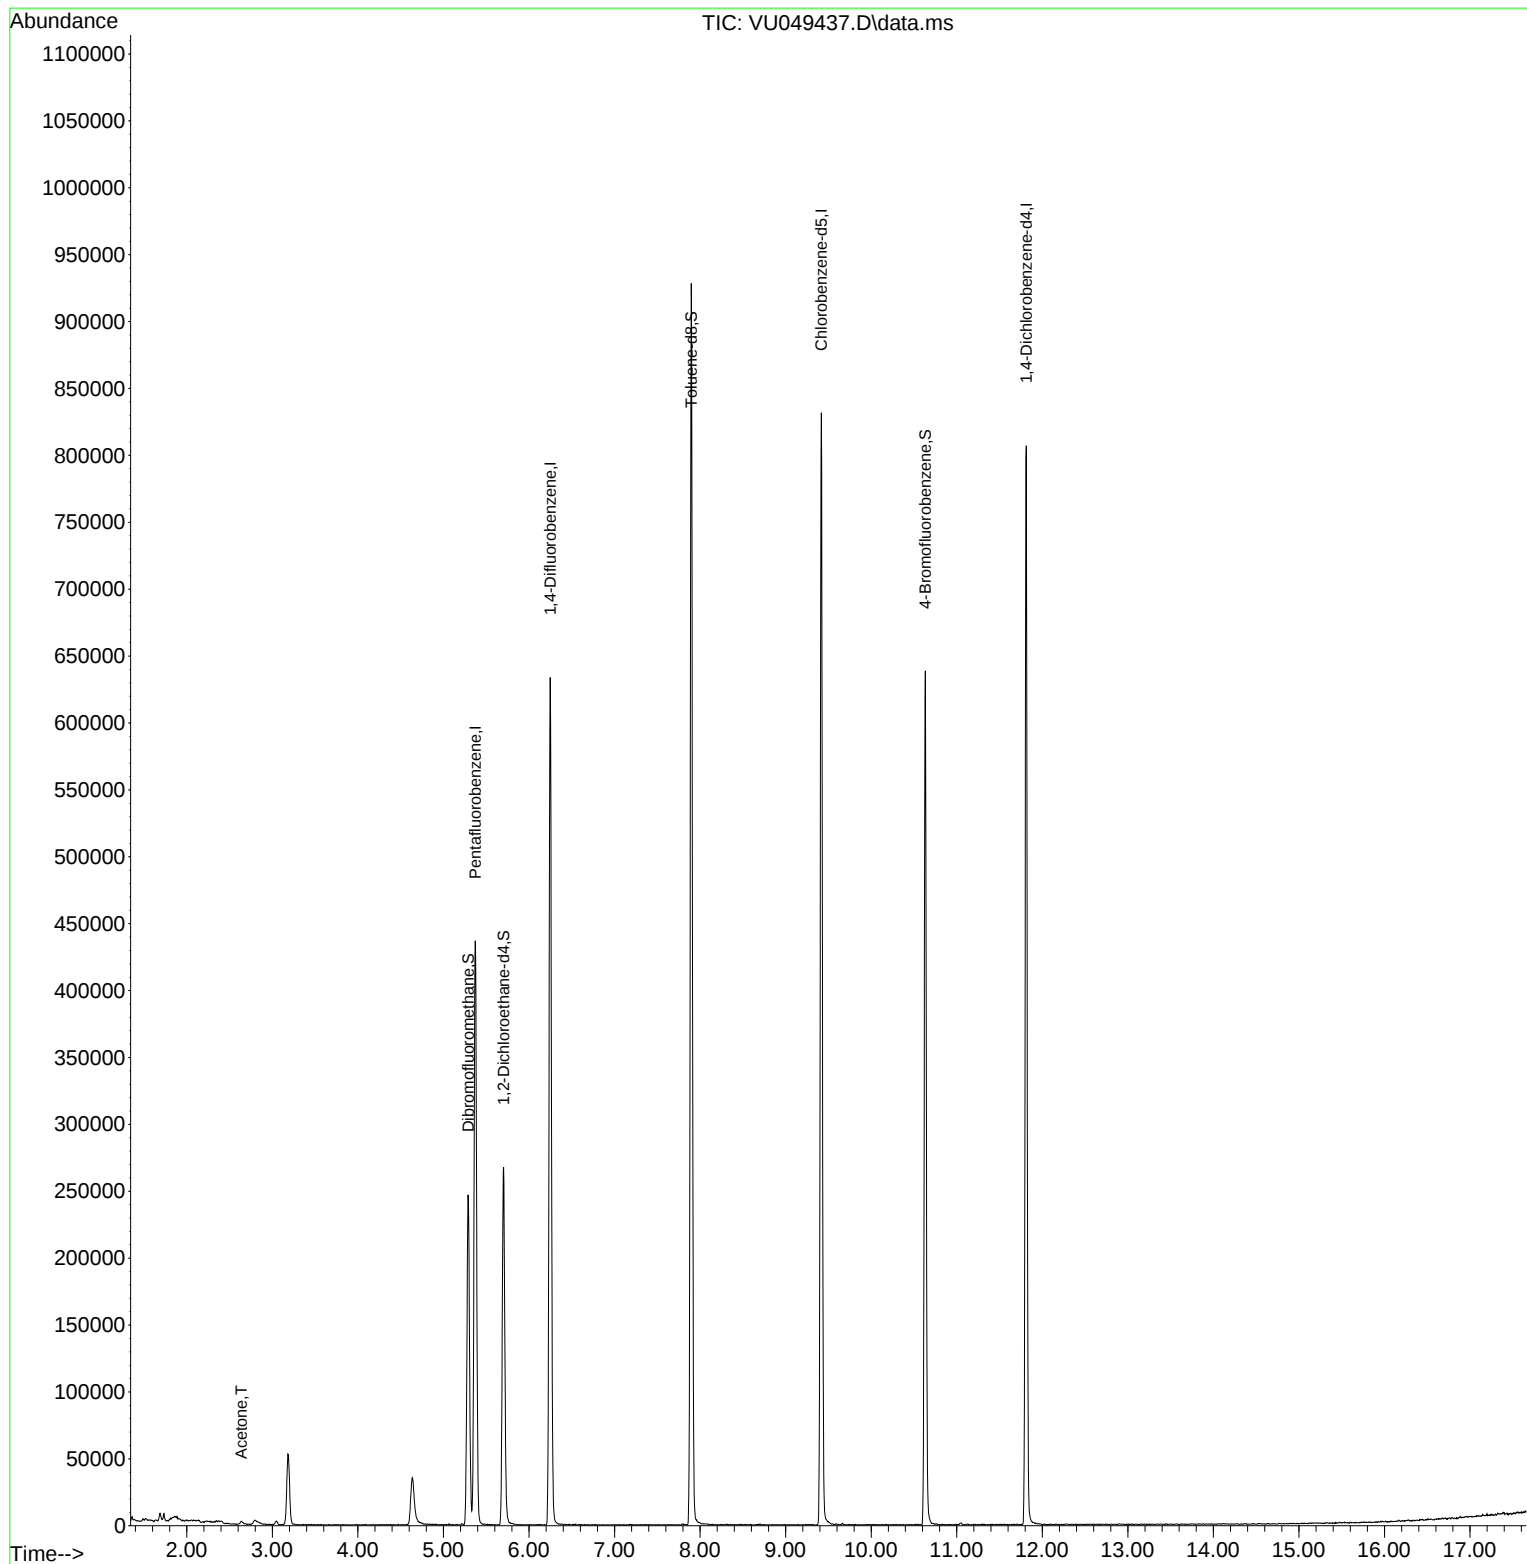


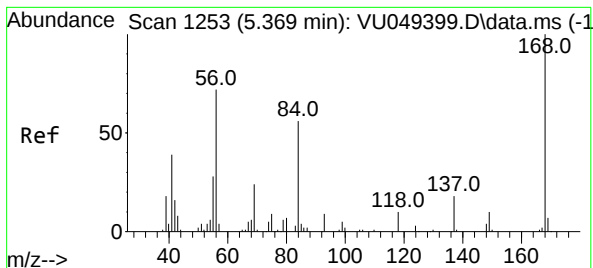

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.372 min Scan# 11
Delta R.T. 0.003 min
Lab File: VU049437.D
Acq: 28 Jun 2022 05:26




Instrument :
MSVOA_U
ClientSampleId :
FB062322


Tgt Ion:168 Resp: 302500
Ion Ratio Lower Upper
168 100
99 60.2 39.3 58.9#

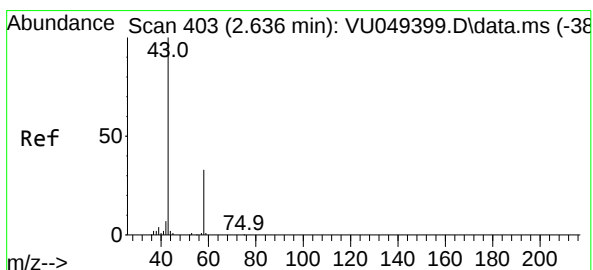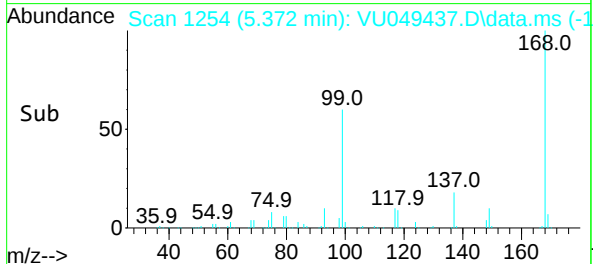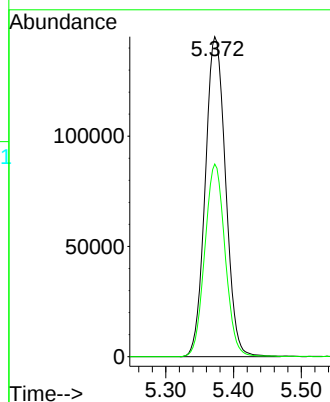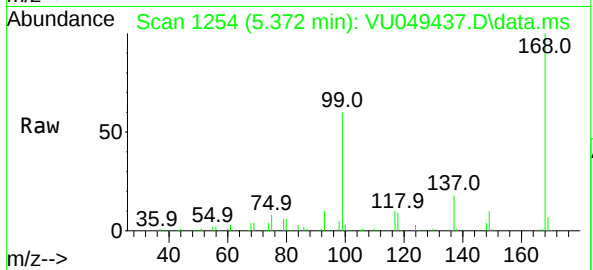

#16
Acetone
Concen: 1.448 ug/l
RT: 2.639 min Scan# 404
Delta R.T. 0.003 min
Lab File: VU049437.D
Acq: 28 Jun 2022 05:26

Tgt Ion: 43 Resp: 3403
Ion Ratio Lower Upper
43 100
58 32.1 27.5 41.3

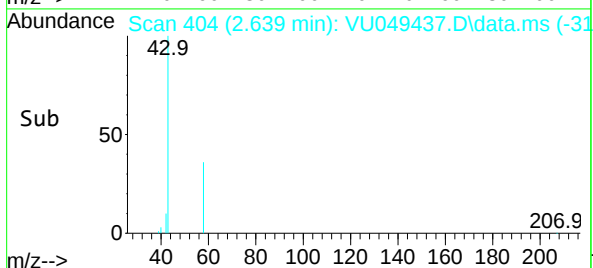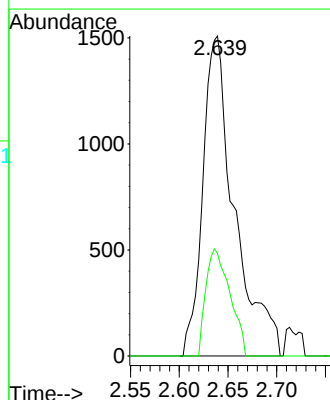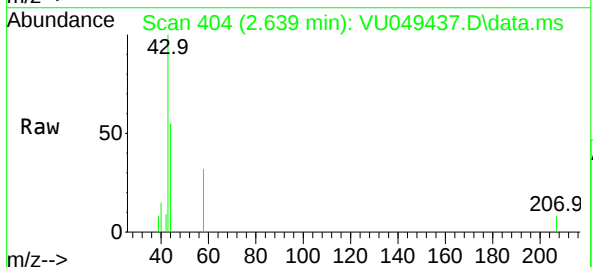

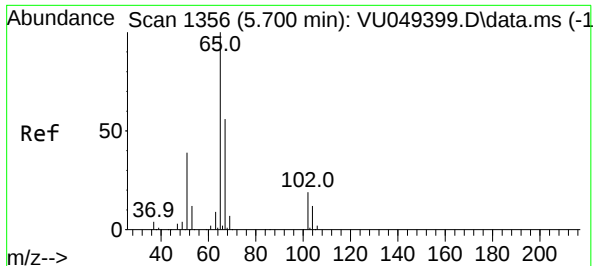

#33

1,2-Dichloroethane-d4

Concen: 43.296 ug/l

RT: 5.703 min Scan# 11

Delta R.T. 0.003 min

Lab File: VU049437.D

Acq: 28 Jun 2022 05:26

Instrument :

MSVOA_U

ClientSampleId :





FB062322

Tgt Ion: 65 Resp: 201703

Ion Ratio Lower Upper

65 100

67 54.1 0.0 108.0

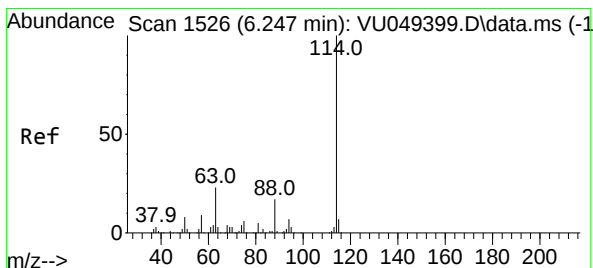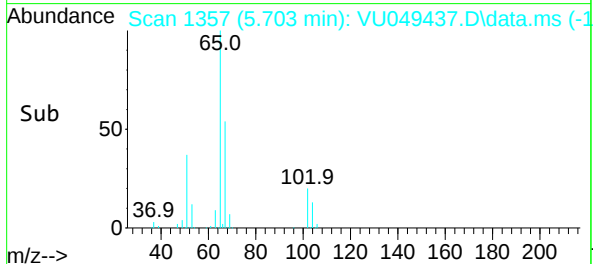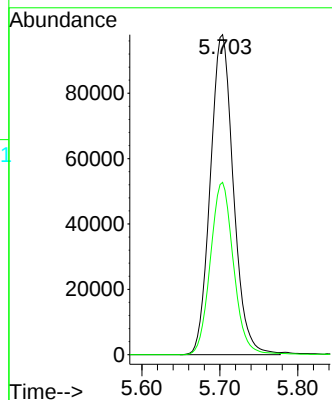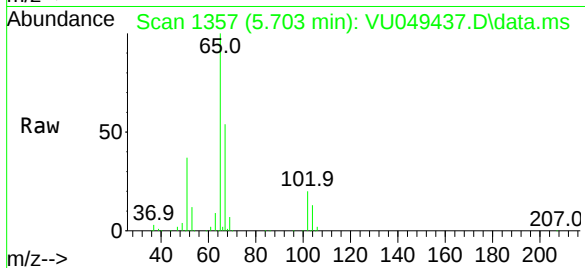

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.250 min Scan# 1527

Delta R.T. 0.003 min

Lab File: VU049437.D

Acq: 28 Jun 2022 05:26




Tgt Ion: 114 Resp: 520242


Ion Ratio Lower Upper

114 100

63 21.6 0.0 37.8

88 16.5 0.0 29.2

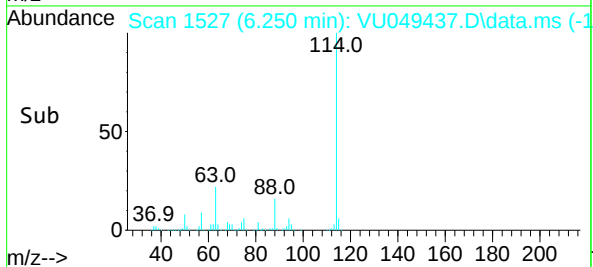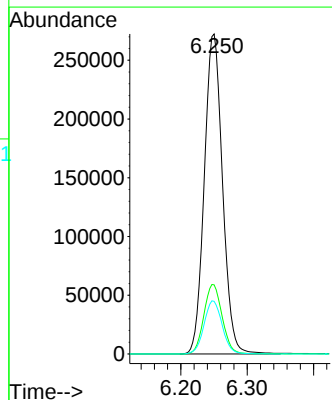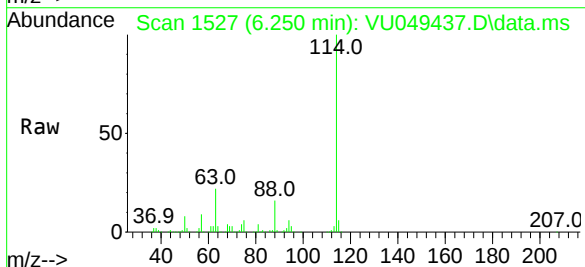

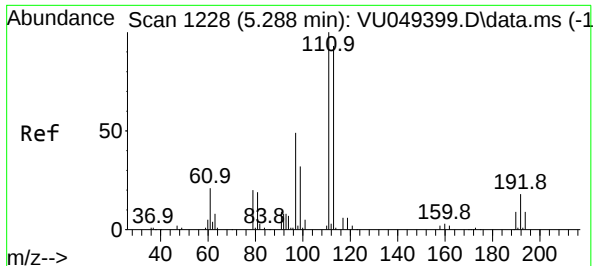

#35

Dibromofluoromethane

Concen: 43.884 ug/l

RT: 5.289 min Scan# 11

Delta R.T. 0.000 min

Lab File: VU049437.D

Acq: 28 Jun 2022 05:26

Instrument :

MSVOA_U

ClientSampleId :

FB062322





Tgt Ion:113 Resp: 159728

Ion Ratio Lower Upper

113 100

111 103.8 82.1 123.1

192 19.5 18.0 27.0

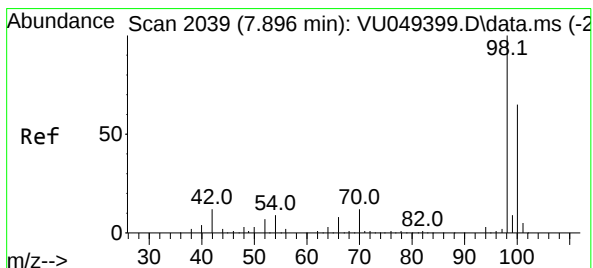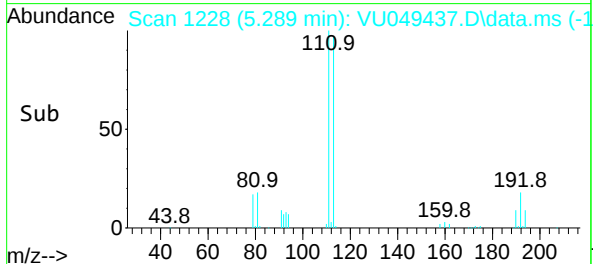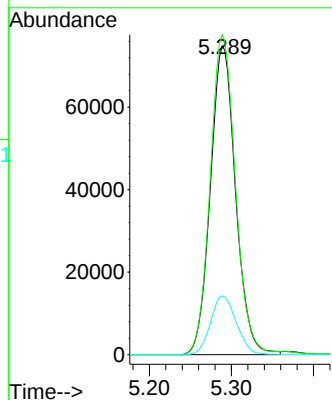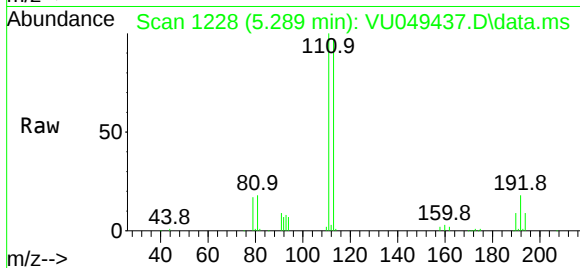

#50

Toluene-d8

Concen: 47.198 ug/l

RT: 7.896 min Scan# 2039

Delta R.T. 0.000 min

Lab File: VU049437.D




Acq: 28 Jun 2022 05:26


Tgt Ion: 98 Resp: 612725

Ion Ratio Lower Upper

98 100

100 64.9 51.7 77.5


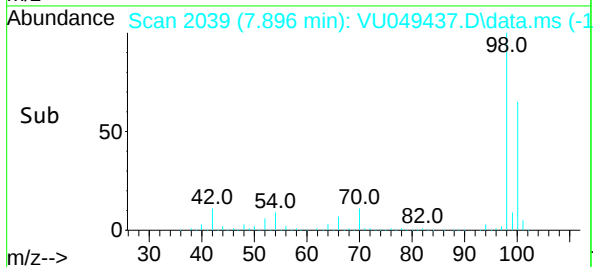
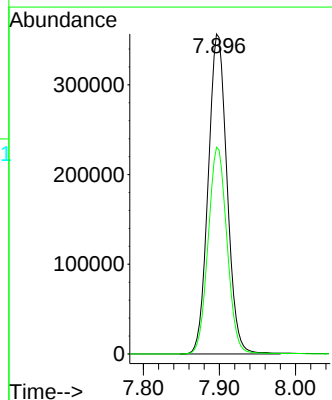
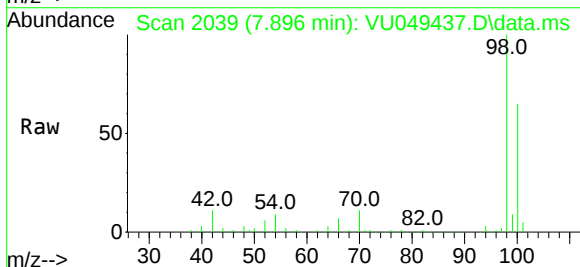


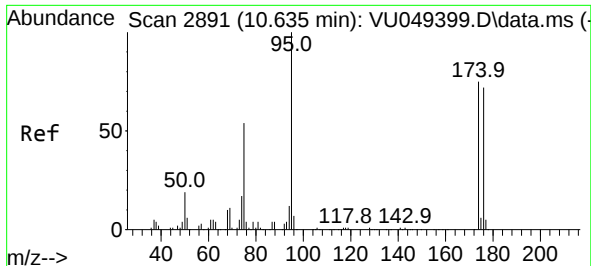

#62
4-Bromofluorobenzene
Concen: 44.167 ug/l
RT: 10.632 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU049437.D
Acq: 28 Jun 2022 05:26




Instrument :
MSVOA_U
ClientSampleId :
FB062322


Tgt Ion: 95 Resp: 219644
Ion Ratio Lower Upper
95 100
174 76.9 0.0 182.0
176 73.0 0.0 177.8

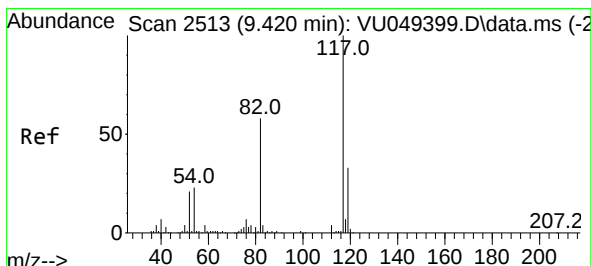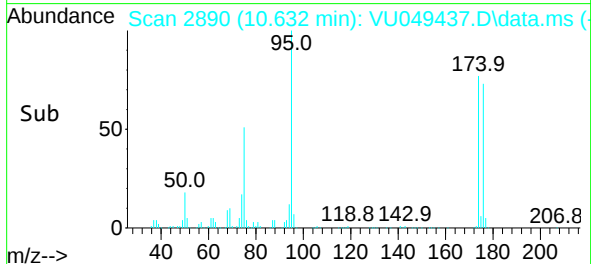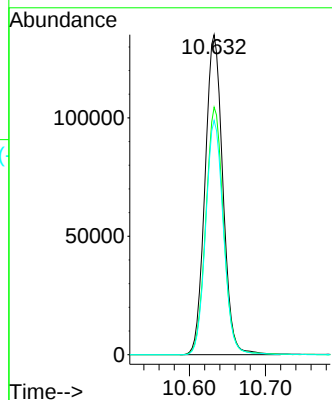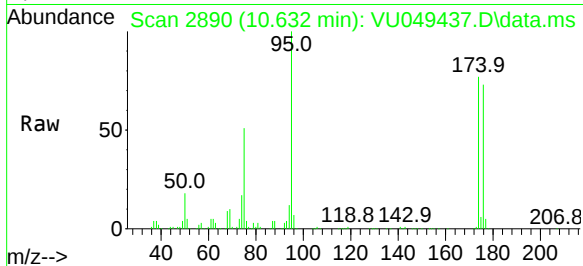

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.417 min Scan# 2512
Delta R.T. -0.003 min
Lab File: VU049437.D
Acq: 28 Jun 2022 05:26

Tgt Ion: 117 Resp: 461942
Ion Ratio Lower Upper
117 100
82 58.4 41.7 62.5
119 31.8 25.7 38.5

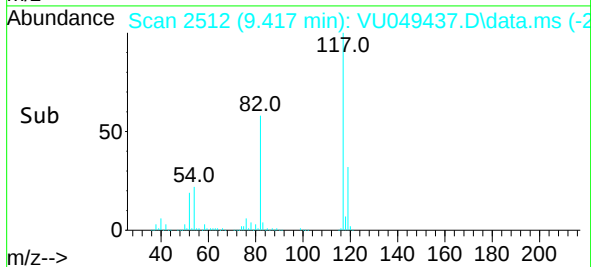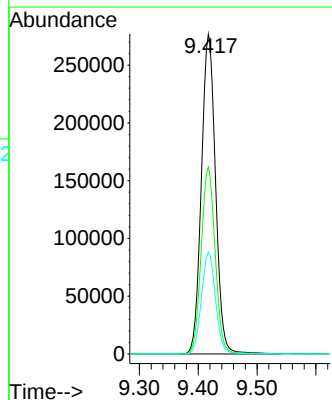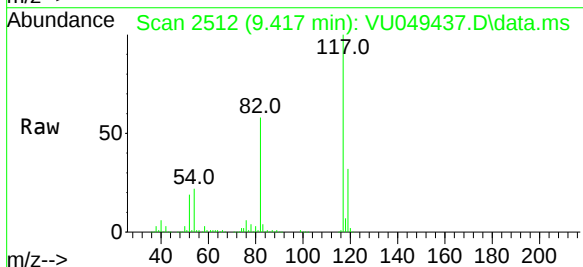

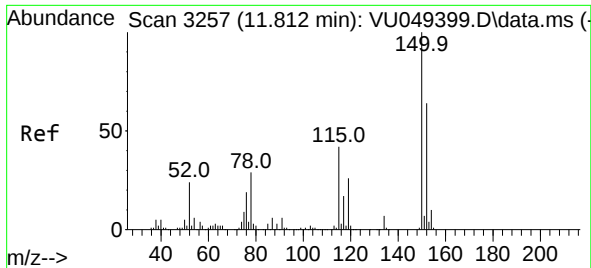

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.812 min Scan# 31

Delta R.T. 0.000 min

Lab File: VU049437.D


Acq: 28 Jun 2022 05:26

Instrument :

MSVOA_U

ClientSampleId :

FB062322

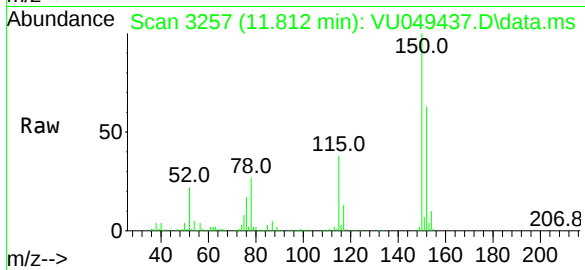

Tgt Ion:152 Resp: 209653

Ion Ratio Lower Upper

152 100

115 60.9 37.0 110.9

150 157.8 0.0 342.2

