

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
 Data File : VU049441.D
 Acq On : 28 Jun 2022 07:00
 Operator : SY/MD
 Sample : N3482-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MW-40

Quant Time: Jun 28 08:31:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 28 05:14:22 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.372	168	302399	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.250	114	520952	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.417	117	464983	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	212204	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.700	65	201777	43.326	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	86.660%
35) Dibromofluoromethane	5.289	113	160636	44.074	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	88.140%
50) Toluene-d8	7.896	98	616442	47.420	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	94.840%
62) 4-Bromofluorobenzene	10.632	95	221888	44.558	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049441.D
Acq On : 28 Jun 2022 07:00
Operator : SY/MD
Sample : N3482-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW-40

Quant Time: Jun 28 08:31:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 28 05:14:22 2022
Response via : Initial Calibration




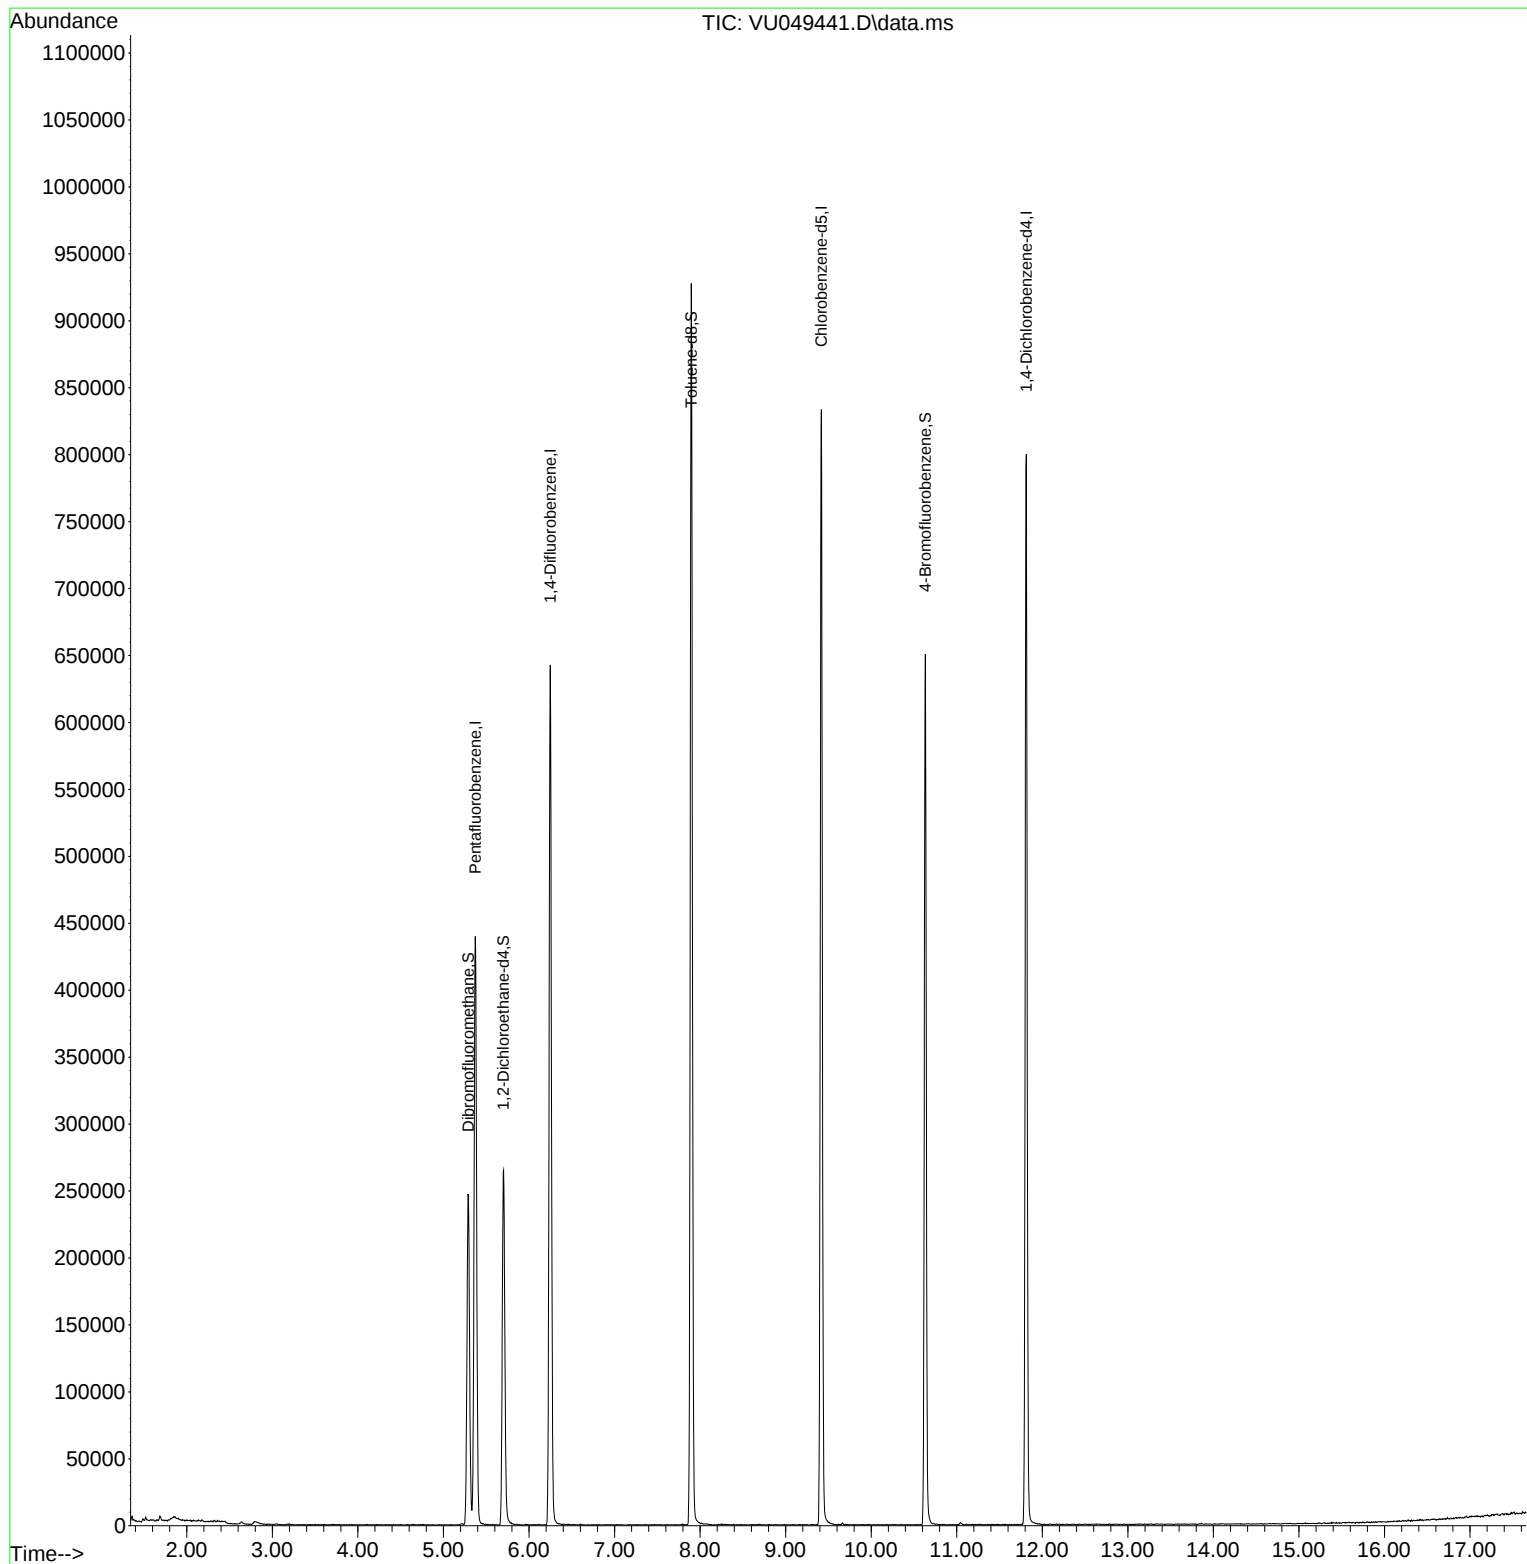


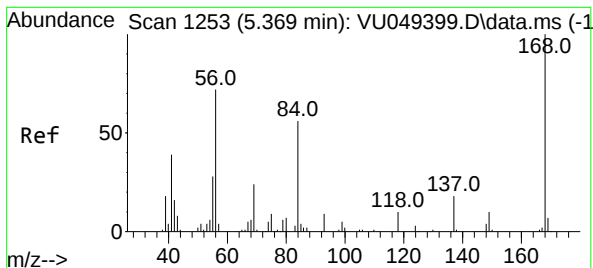

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.372 min Scan# 1254
Delta R.T. 0.003 min
Lab File: VU049441.D
Acq: 28 Jun 2022 07:00




Instrument :
MSVOA_U
ClientSampleId :
MW-40


Tgt Ion:168 Resp: 302399
Ion Ratio Lower Upper
168 100
99 59.8 39.3 58.9#

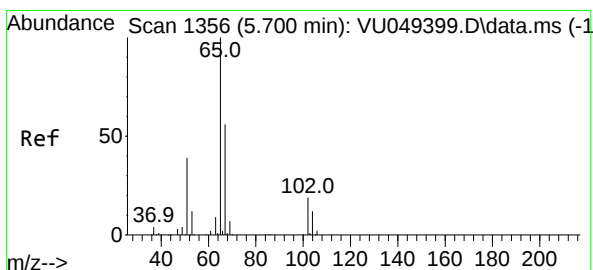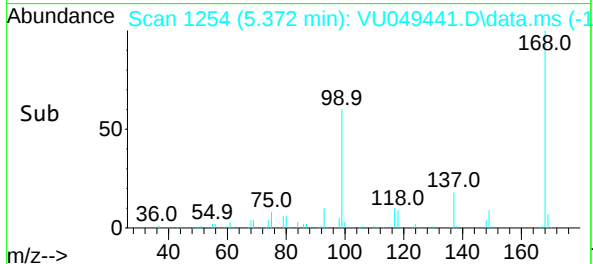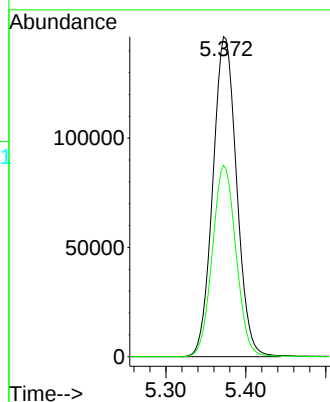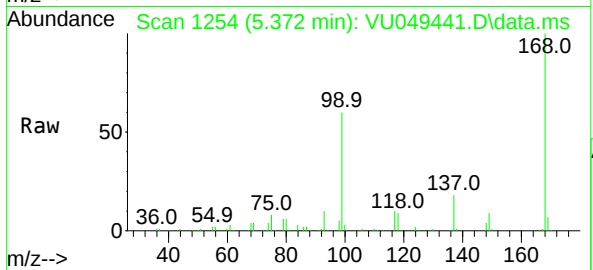

#33
1,2-Dichloroethane-d4
Concen: 43.326 ug/l
RT: 5.700 min Scan# 1356
Delta R.T. 0.000 min
Lab File: VU049441.D
Acq: 28 Jun 2022 07:00

Tgt Ion: 65 Resp: 201777
Ion Ratio Lower Upper
65 100
67 54.3 0.0 108.0


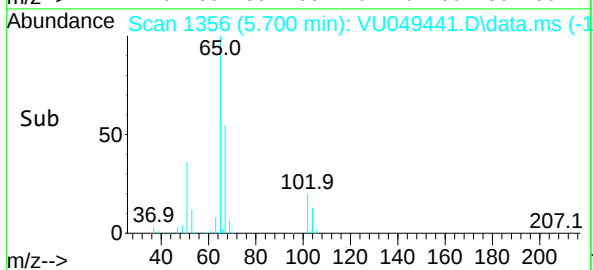
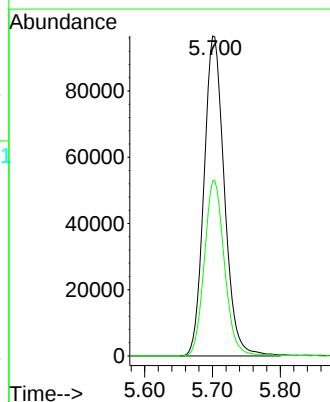
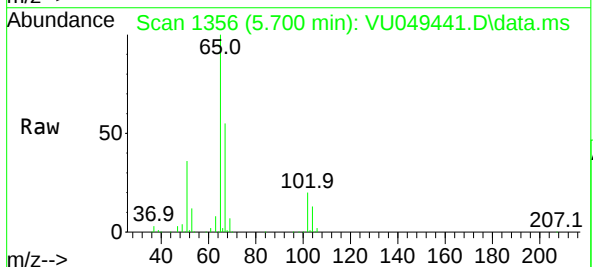


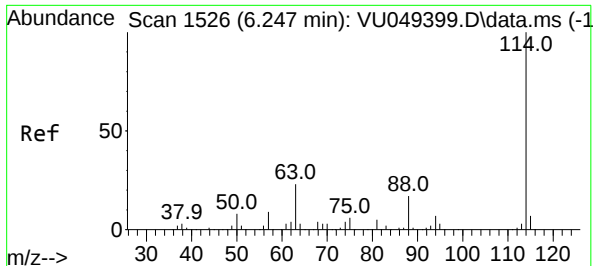

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.250 min Scan# 11
Delta R.T. 0.003 min
Lab File: VU049441.D
Acq: 28 Jun 2022 07:00




Instrument :
MSVOA_U
ClientSampleId :
MW-40


Tgt Ion:114 Resp: 520952
Ion Ratio Lower Upper
114 100
63 21.5 0.0 37.8
88 16.5 0.0 29.2

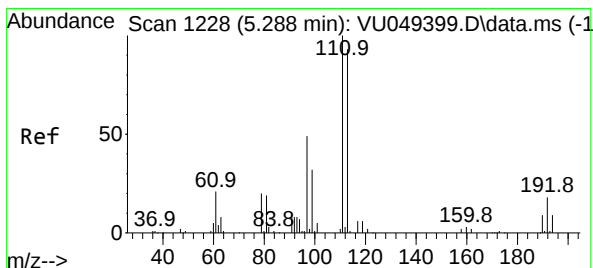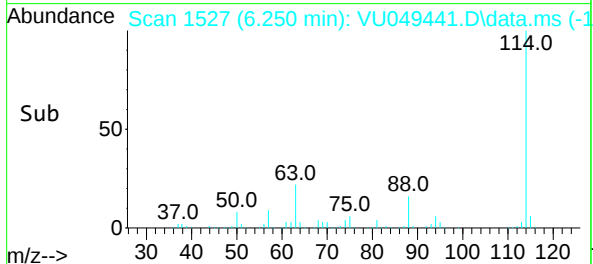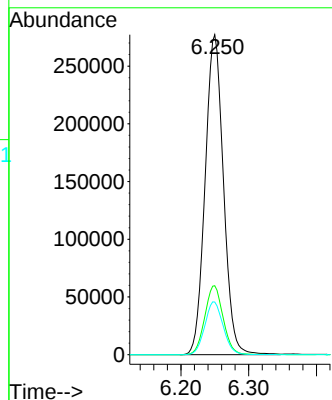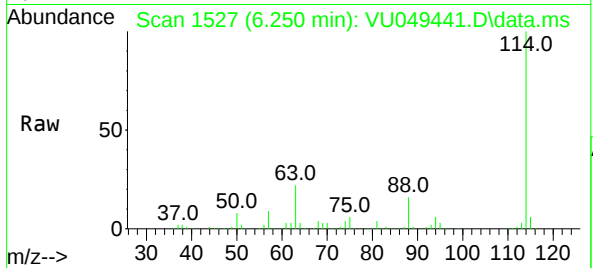

#35
Dibromofluoromethane
Concen: 44.074 ug/l
RT: 5.289 min Scan# 1228
Delta R.T. 0.000 min
Lab File: VU049441.D
Acq: 28 Jun 2022 07:00

Tgt Ion:113 Resp: 160636
Ion Ratio Lower Upper
113 100
111 104.8 82.1 123.1
192 19.2 18.0 27.0


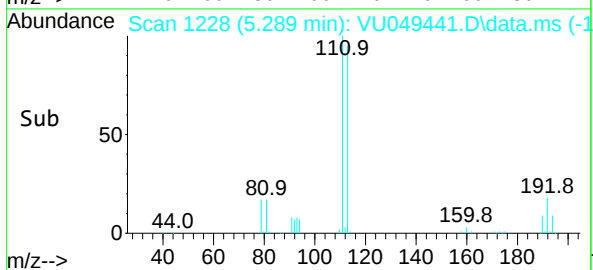
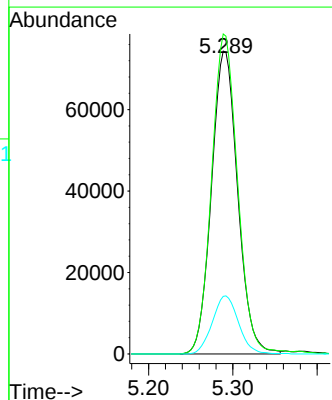
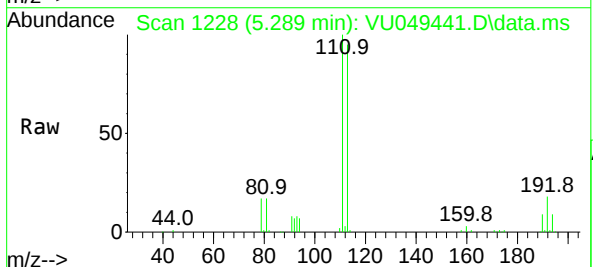


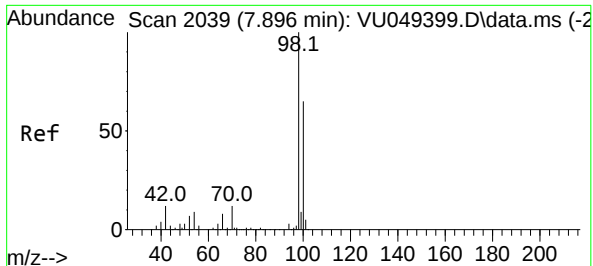

#50
Toluene-d8
Concen: 47.420 ug/l
RT: 7.896 min Scan# 2039
Delta R.T. 0.000 min
Lab File: VU049441.D
Acq: 28 Jun 2022 07:00




Instrument :
MSVOA_U
ClientSampleId :
MW-40


Tgt Ion: 98 Resp: 616442
Ion Ratio Lower Upper
98 100
100 64.6 51.7 77.5

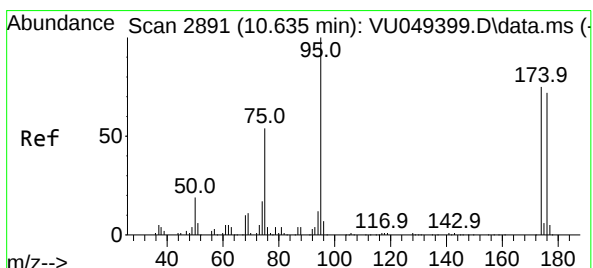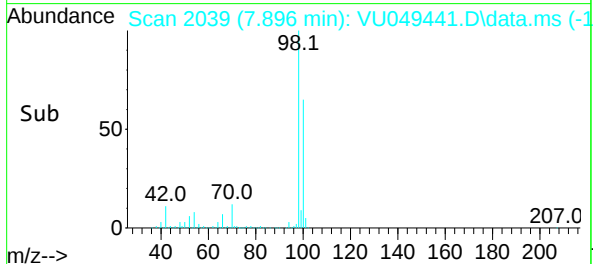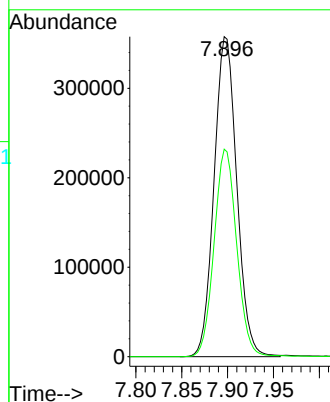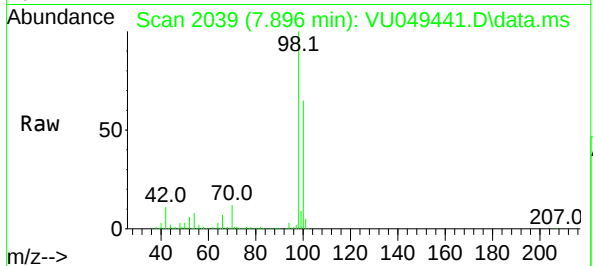

#62
4-Bromofluorobenzene
Concen: 44.558 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.003 min
Lab File: VU049441.D
Acq: 28 Jun 2022 07:00

Tgt Ion: 95 Resp: 221888
Ion Ratio Lower Upper
95 100
174 75.1 0.0 182.0
176 74.0 0.0 177.8


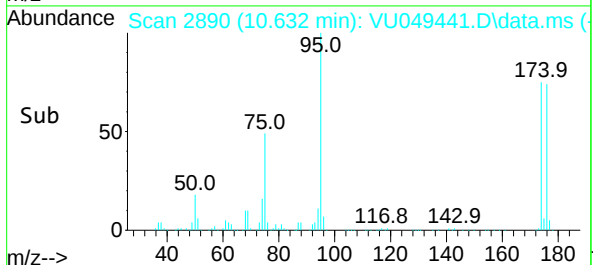
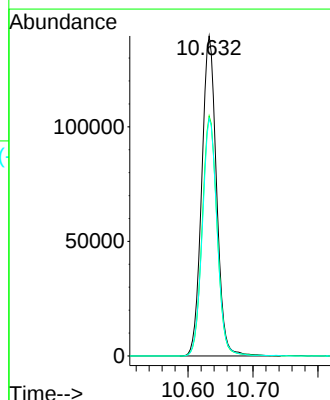
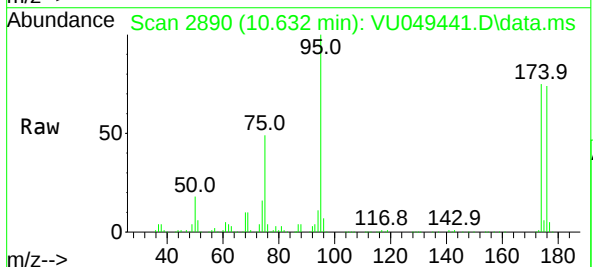


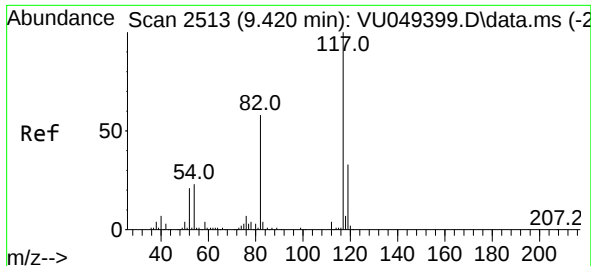

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.417 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU049441.D
Acq: 28 Jun 2022 07:00

Instrument :
MSVOA_U
ClientSampleId :
MW-40

Tgt Ion:117 Resp: 464983
Ion Ratio Lower Upper
117 100
82 58.0 41.7 62.5
119 31.5 25.7 38.5

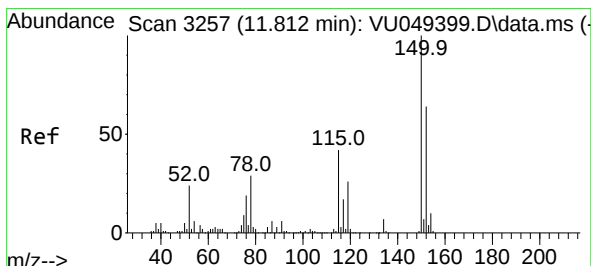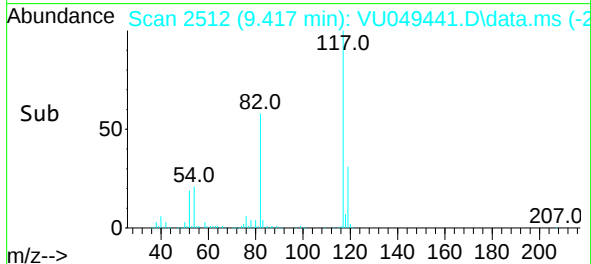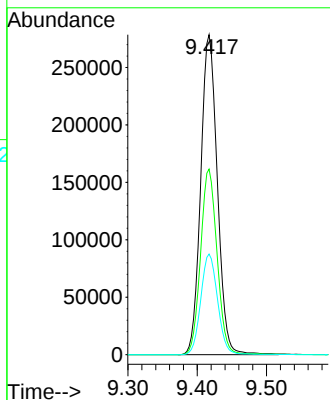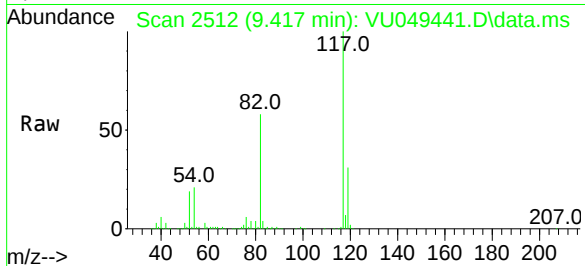

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.812 min Scan# 3257
Delta R.T. 0.000 min
Lab File: VU049441.D
Acq: 28 Jun 2022 07:00

Tgt Ion:152 Resp: 212204
Ion Ratio Lower Upper
152 100
115 61.1 37.0 110.9
150 157.6 0.0 342.2

