

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
 Data File : VU049421.D
 Acq On : 27 Jun 2022 23:08
 Operator : SY/MD
 Sample : VU0627WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0627WBL02

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M

Title : SW846 8260

Signal : TIC: VU049421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.186	555	574	595	rVB2	27238	64108	4.00%	0.748%
2	4.633	1008	1024	1047	rBV2	18596	54519	3.40%	0.636%
3	5.288	1212	1228	1241	rBV	242143	516653	32.22%	6.027%
4	5.372	1241	1254	1273	rVB	438629	899502	56.10%	10.492%
5	5.700	1342	1356	1381	rBV	263853	542818	33.85%	6.332%
6	6.247	1511	1526	1553	rBV	630249	1200064	74.84%	13.998%
7	7.896	2025	2039	2061	rBV	931778	1603421	100.00%	18.703%
8	9.417	2498	2512	2535	rBV	836213	1371120	85.51%	15.994%
9	10.632	2877	2890	2920	rBV	643987	1022424	63.77%	11.926%
10	11.809	3243	3256	3280	rBV	799314	1281341	79.91%	14.947%
11	16.269	4630	4643	4652	rBV4	8023	16876	1.05%	0.197%




Sum of corrected areas: 8572846

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049421.D
Acq On : 27 Jun 2022 23:08
Operator : SY/MD
Sample : VU0627WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0627WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

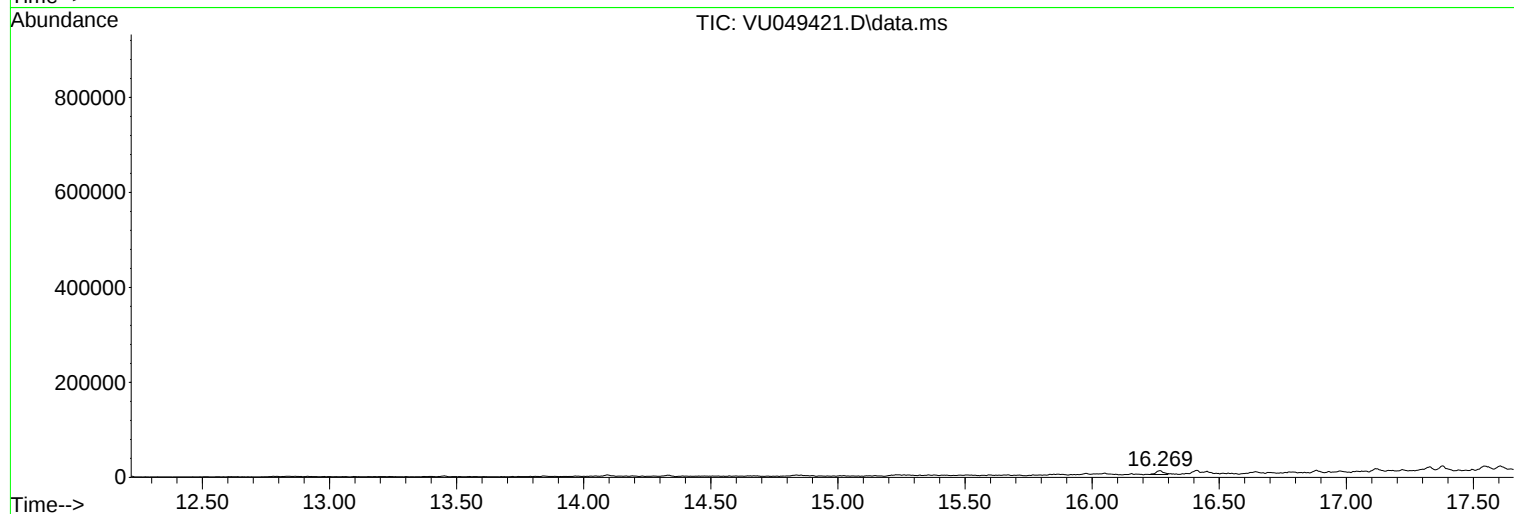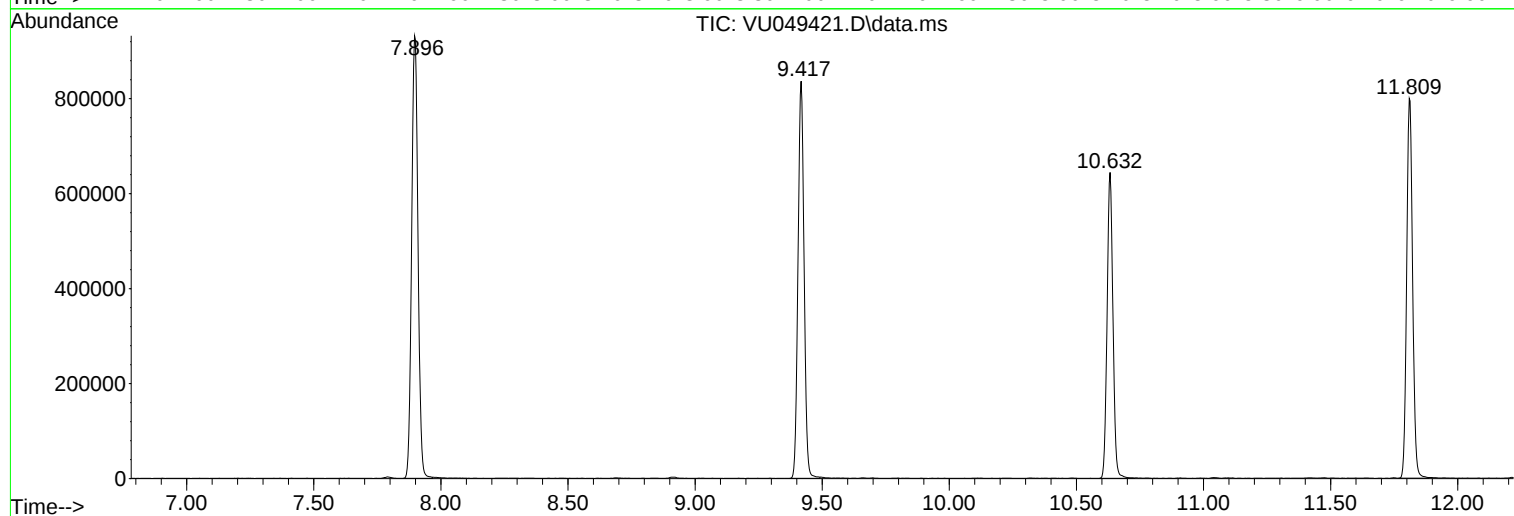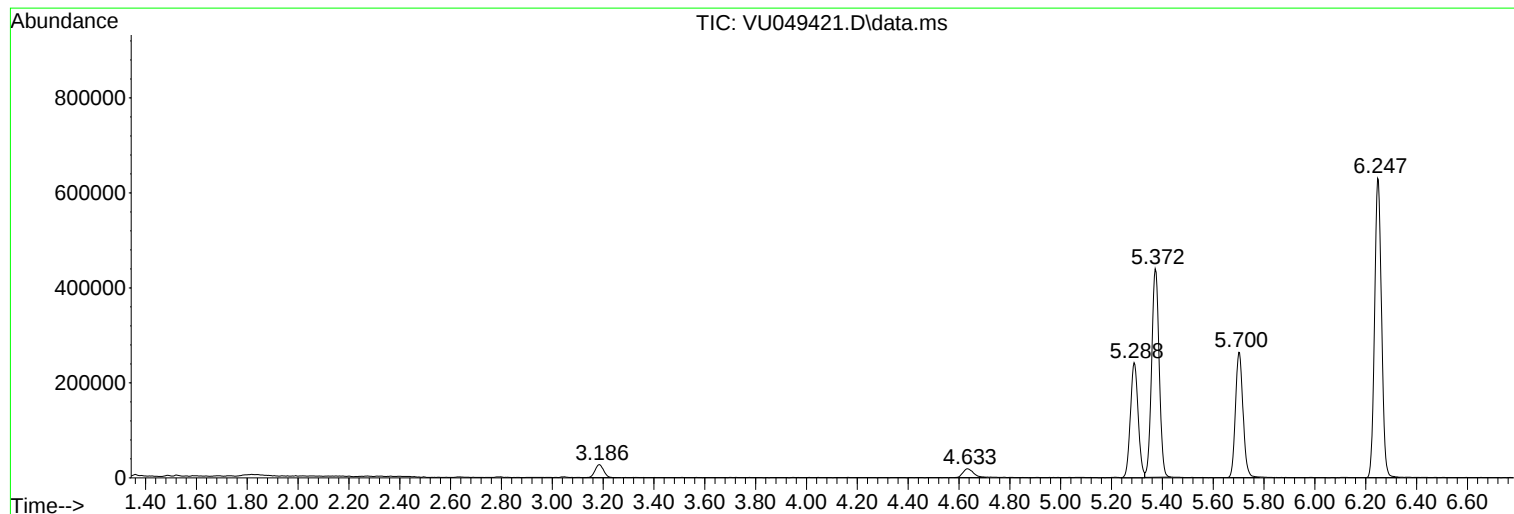

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049421.D
Acq On : 27 Jun 2022 23:08
Operator : SY/MD
Sample : VU0627WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0627WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049421.D
Acq On : 27 Jun 2022 23:08
Operator : SY/MD
Sample : VU0627WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0627WBL02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc