

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
 Data File : VU049426.D
 Acq On : 28 Jun 2022 01:06
 Operator : SY/MD
 Sample : N3482-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB062322

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M

Title : SW846 8260

Signal : TIC: VU049426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.787	434	450	483	rBV2	16036	61752	3.80%	0.697%
2	3.186	558	574	595	rVB	28841	66494	4.09%	0.751%
3	4.636	1009	1025	1047	rBV2	17330	52230	3.21%	0.590%
4	5.289	1212	1228	1241	rBV	248845	526043	32.34%	5.939%
5	5.372	1241	1254	1277	rVB	444254	921731	56.67%	10.407%
6	5.700	1342	1356	1382	rBV	267489	549973	33.81%	6.210%
7	6.247	1510	1526	1555	rBV	647814	1225972	75.37%	13.842%
8	6.543	1607	1618	1630	rBV2	18358	32920	2.02%	0.372%
9	7.896	2024	2039	2058	rBV	943836	1626618	100.00%	18.366%
10	9.417	2499	2512	2535	rBV	851969	1406098	86.44%	15.876%
11	10.632	2877	2890	2912	rBV	661712	1057763	65.03%	11.943%
12	11.812	3242	3257	3279	rBV	841746	1329212	81.72%	15.008%




Sum of corrected areas: 8856806

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049426.D
Acq On : 28 Jun 2022 01:06
Operator : SY/MD
Sample : N3482-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB062322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

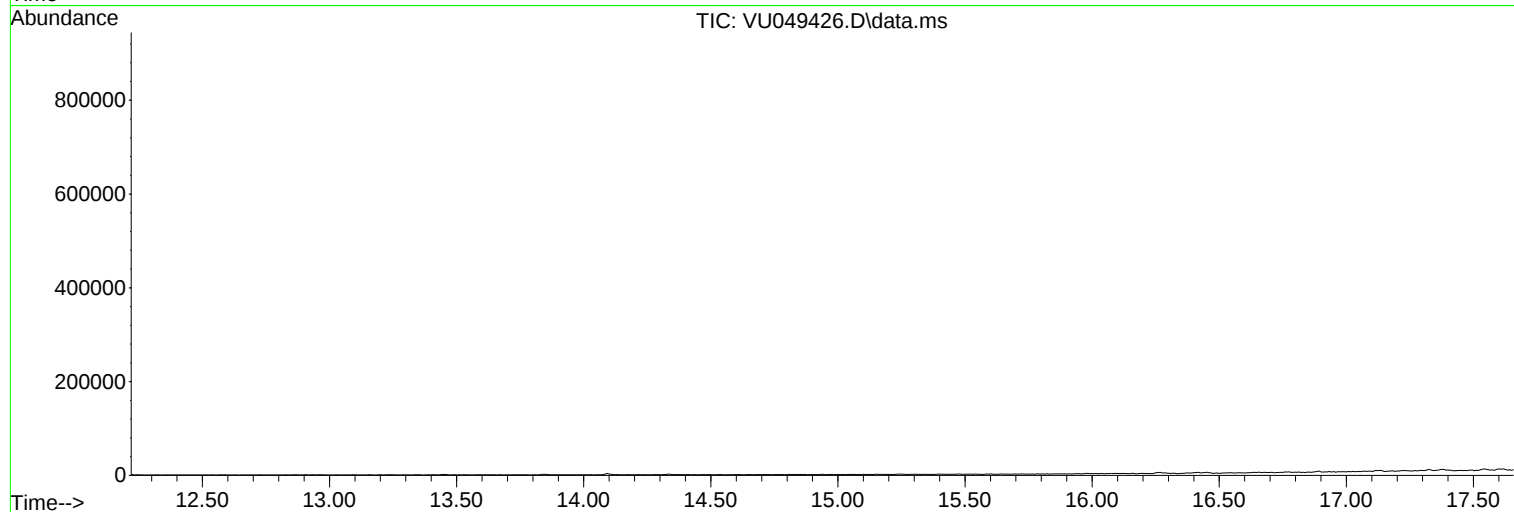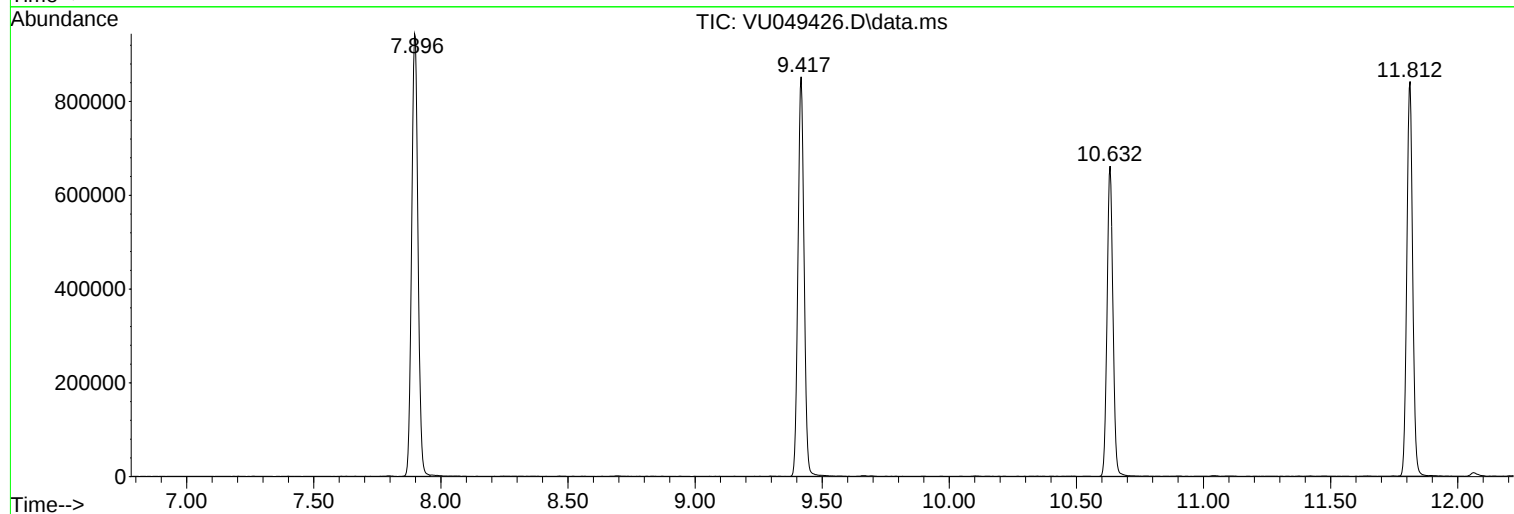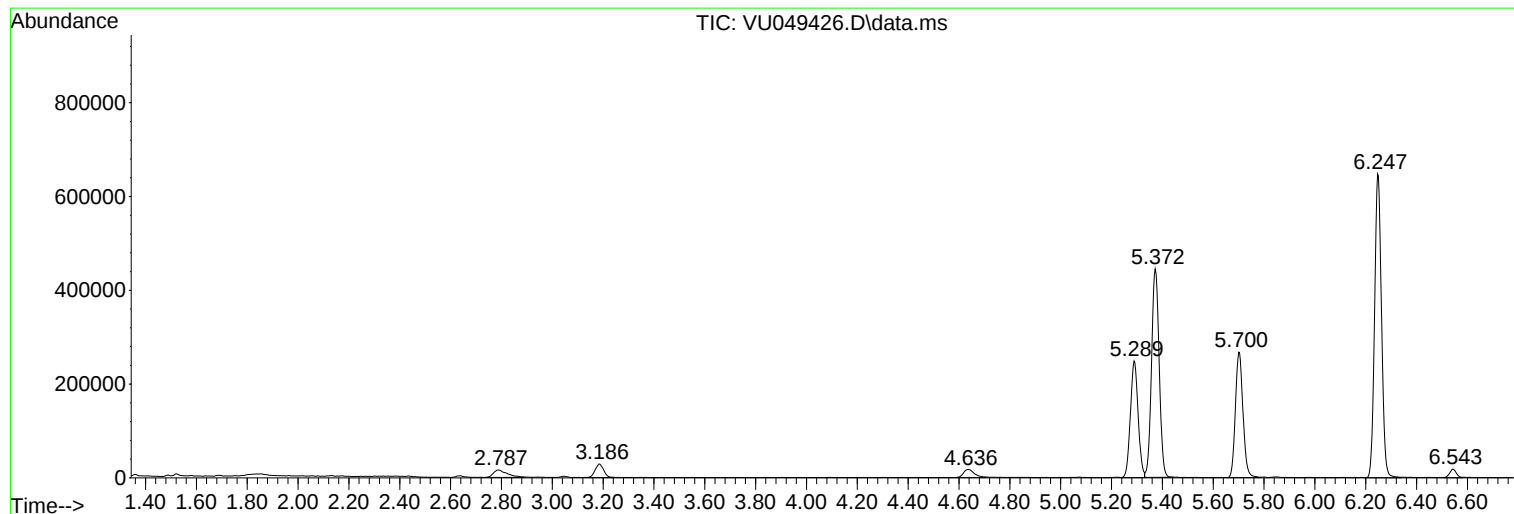

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049426.D
Acq On : 28 Jun 2022 01:06
Operator : SY/MD
Sample : N3482-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB062322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049426.D
Acq On : 28 Jun 2022 01:06
Operator : SY/MD
Sample : N3482-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB062322

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc