

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
 Data File : VU049427.D
 Acq On : 28 Jun 2022 01:30
 Operator : SY/MD
 Sample : N3386-01RE 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 RE105D2-20220613RE

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M

Title : SW846 8260

Signal : TIC: VU049427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.186	554	574	598	rBV	30465	69929	4.28%	0.701%
2	4.639	1008	1026	1048	rBV	17579	52841	3.23%	0.530%
3	5.288	1212	1228	1241	rBV	250233	527760	32.27%	5.292%
4	5.372	1241	1254	1281	rVB	445768	923764	56.48%	9.263%
5	5.700	1342	1356	1377	rBV	271630	556936	34.05%	5.585%
6	6.250	1513	1527	1556	rBV	649668	1230987	75.27%	12.344%
7	6.542	1601	1618	1644	rBV	636268	1189901	72.76%	11.932%
8	7.896	2025	2039	2063	rBV	945300	1635479	100.00%	16.400%
9	9.417	2498	2512	2548	rBV	861583	1411615	86.31%	14.155%
10	10.632	2876	2890	2914	rBV	654639	1050604	64.24%	10.535%
11	11.812	3243	3257	3280	rBV	822052	1322514	80.86%	13.262%




Sum of corrected areas: 9972330

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049427.D
Acq On : 28 Jun 2022 01:30
Operator : SY/MD
Sample : N3386-01RE 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE105D2-20220613RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

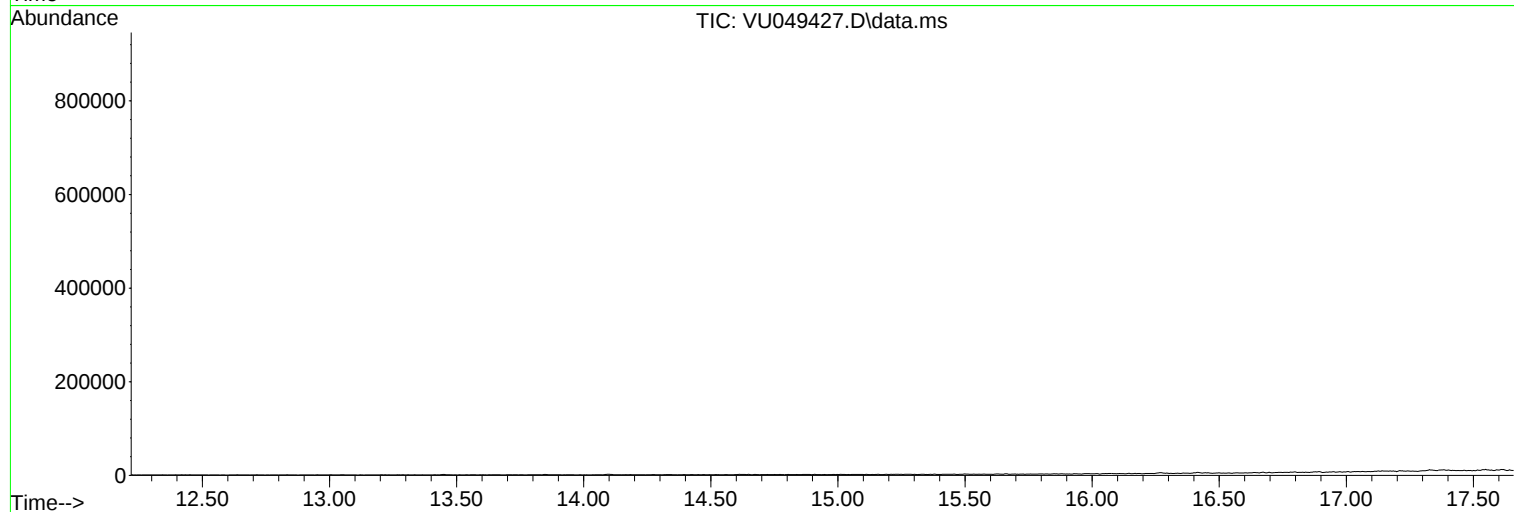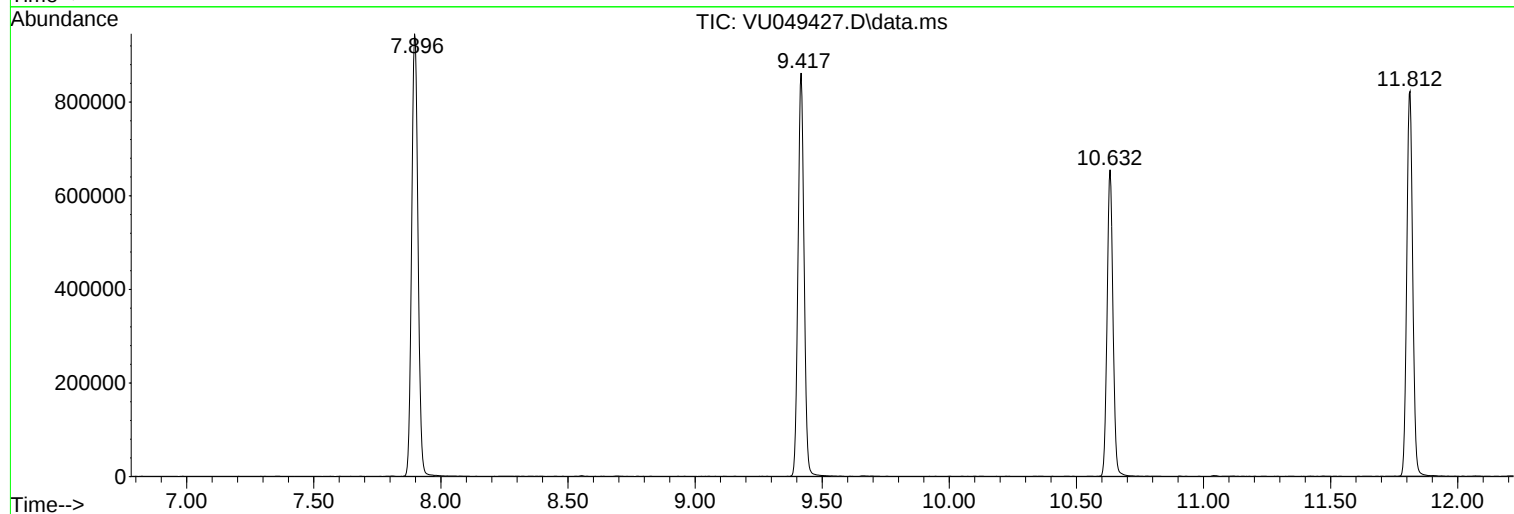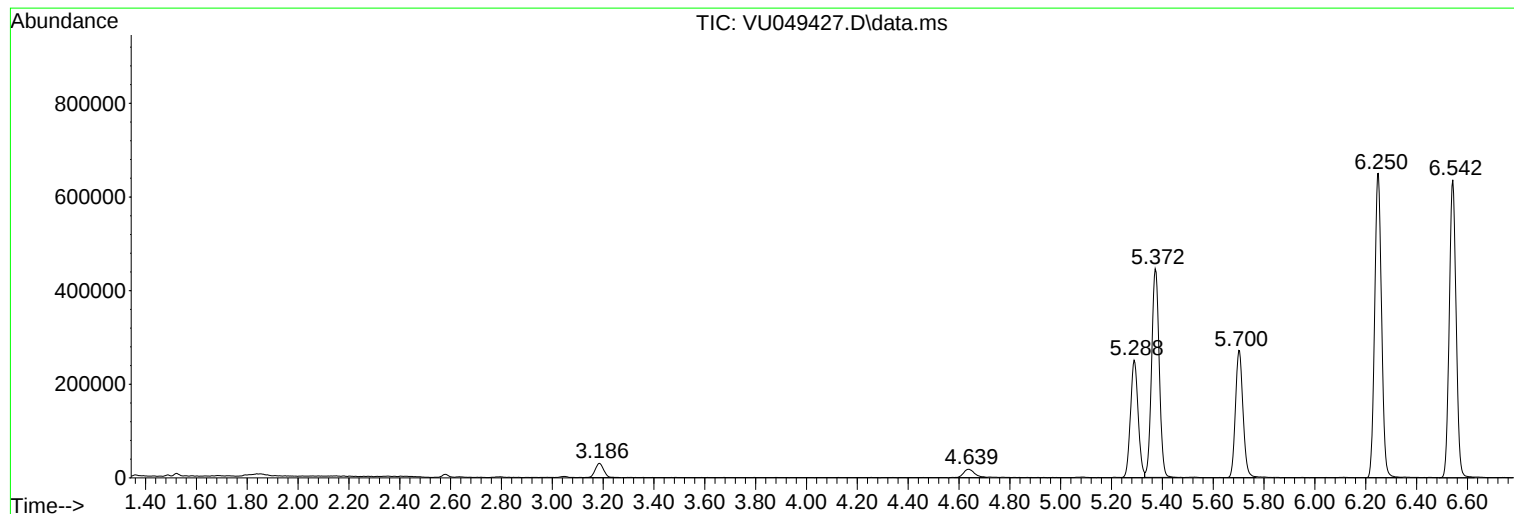

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049427.D
Acq On : 28 Jun 2022 01:30
Operator : SY/MD
Sample : N3386-01RE 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE105D2-20220613RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049427.D
Acq On : 28 Jun 2022 01:30
Operator : SY/MD
Sample : N3386-01RE 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE105D2-20220613RE

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc