

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062722\  
 Data File : VU049438.D  
 Acq On : 28 Jun 2022 05:49  
 Operator : SY/MD  
 Sample : N3482-01  
 Misc : 5.0mL/MSVOA\_U/WATER  
 ALS Vial : 45 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 MW-35

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U062722W.M  
 Title : SW846 8260

Signal : TIC: VU049438.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.199       | 557           | 578         | 613          | rBV2     | 79703          | 254651        | 15.70%          | 2.851%        |
| 2         | 3.363       | 613           | 629         | 652          | rVB2     | 36159          | 87440         | 5.39%           | 0.979%        |
| 3         | 3.993       | 806           | 825         | 840          | rBV2     | 7063           | 18888         | 1.16%           | 0.211%        |
| 4         | 5.089       | 1152          | 1166        | 1187         | rBV3     | 11067          | 25458         | 1.57%           | 0.285%        |
| 5         | 5.289       | 1212          | 1228        | 1241         | rBV2     | 244810         | 523496        | 32.27%          | 5.862%        |
| 6         | 5.372       | 1241          | 1254        | 1284         | rVB      | 439756         | 906656        | 55.88%          | 10.152%       |
| 7         | 5.703       | 1342          | 1357        | 1377         | rBV      | 266836         | 553862        | 34.14%          | 6.202%        |
| 8         | 5.838       | 1390          | 1399        | 1424         | rVB5     | 8397           | 21813         | 1.34%           | 0.244%        |
| 9         | 6.247       | 1512          | 1526        | 1551         | rBV      | 640908         | 1218916       | 75.13%          | 13.648%       |
| 10        | 7.896       | 2025          | 2039        | 2063         | rBV      | 937352         | 1622423       | 100.00%         | 18.166%       |
| 11        | 9.417       | 2498          | 2512        | 2538         | rBV      | 834760         | 1393969       | 85.92%          | 15.608%       |
| 12        | 10.632      | 2877          | 2890        | 2920         | rBV      | 643817         | 1033475       | 63.70%          | 11.572%       |
| 13        | 11.813      | 3243          | 3257        | 3284         | rBV      | 791215         | 1270020       | 78.28%          | 14.220%       |




Sum of corrected areas: 8931067

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062722\  
Data File : VU049438.D  
Acq On : 28 Jun 2022 05:49  
Operator : SY/MD  
Sample : N3482-01  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
MW-35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U062722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

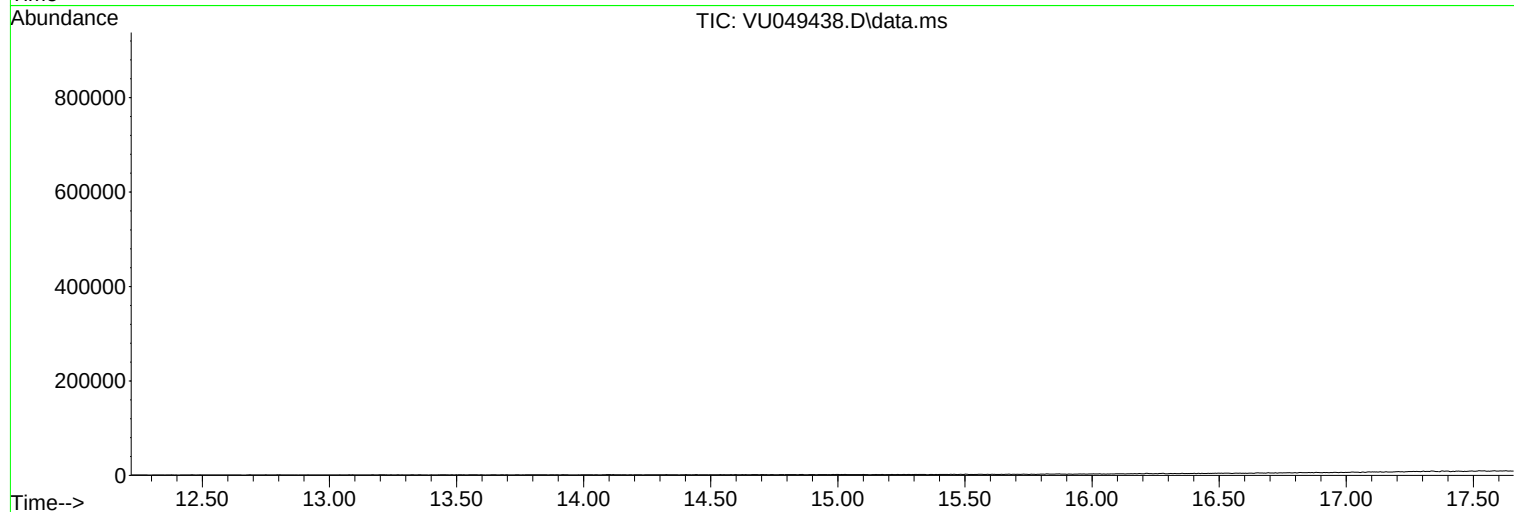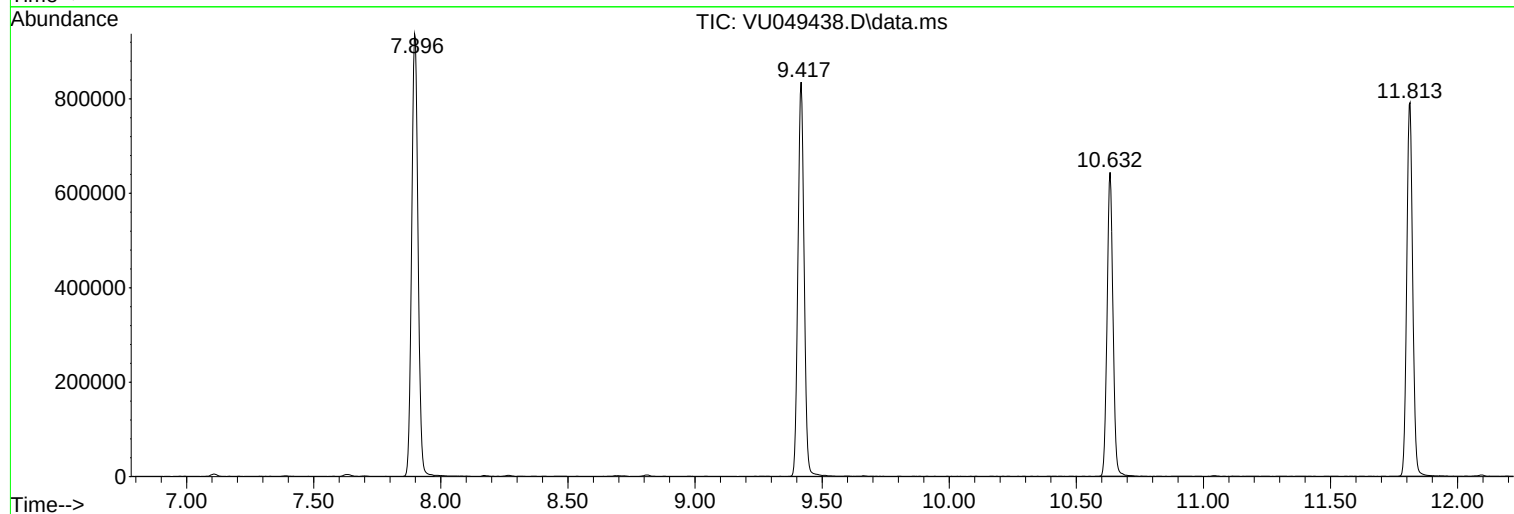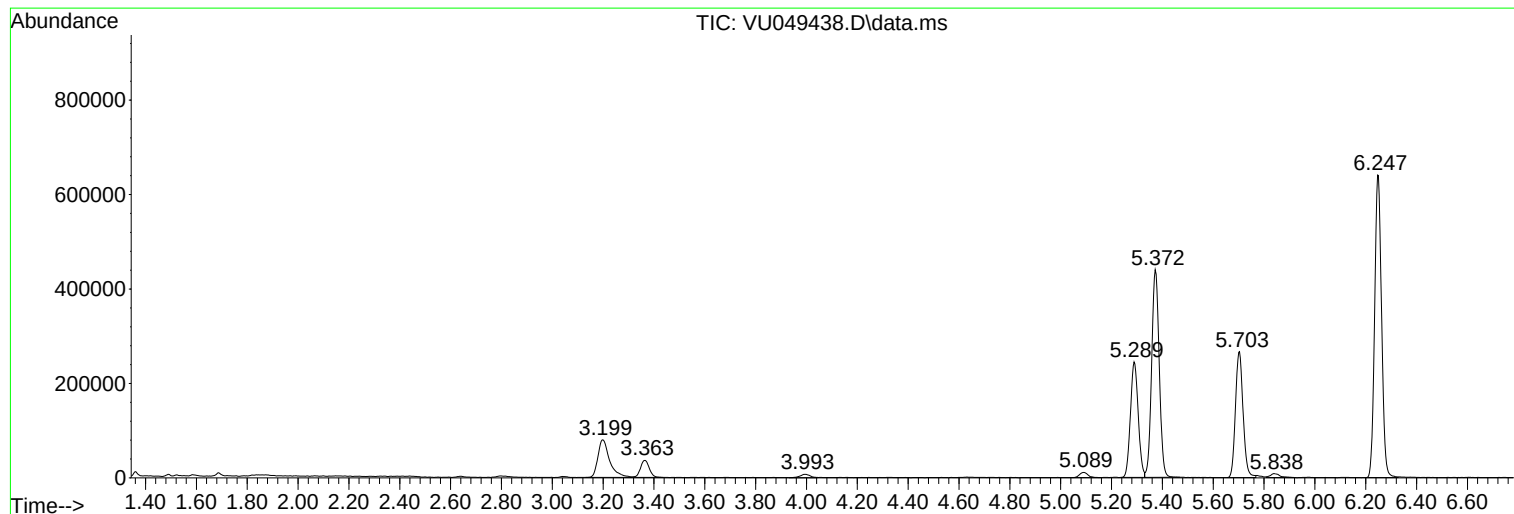

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062722\  
Data File : VU049438.D  
Acq On : 28 Jun 2022 05:49  
Operator : SY/MD  
Sample : N3482-01  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
MW-35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U062722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062722\  
Data File : VU049438.D  
Acq On : 28 Jun 2022 05:49  
Operator : SY/MD  
Sample : N3482-01  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 45 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
MW-35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U062722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|