


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062722\
Data File : VU049418.D
Acq On : 27 Jun 2022 21:34
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Title : SW846 8260
Last Update : Tue Jun 28 10:35:43 2022

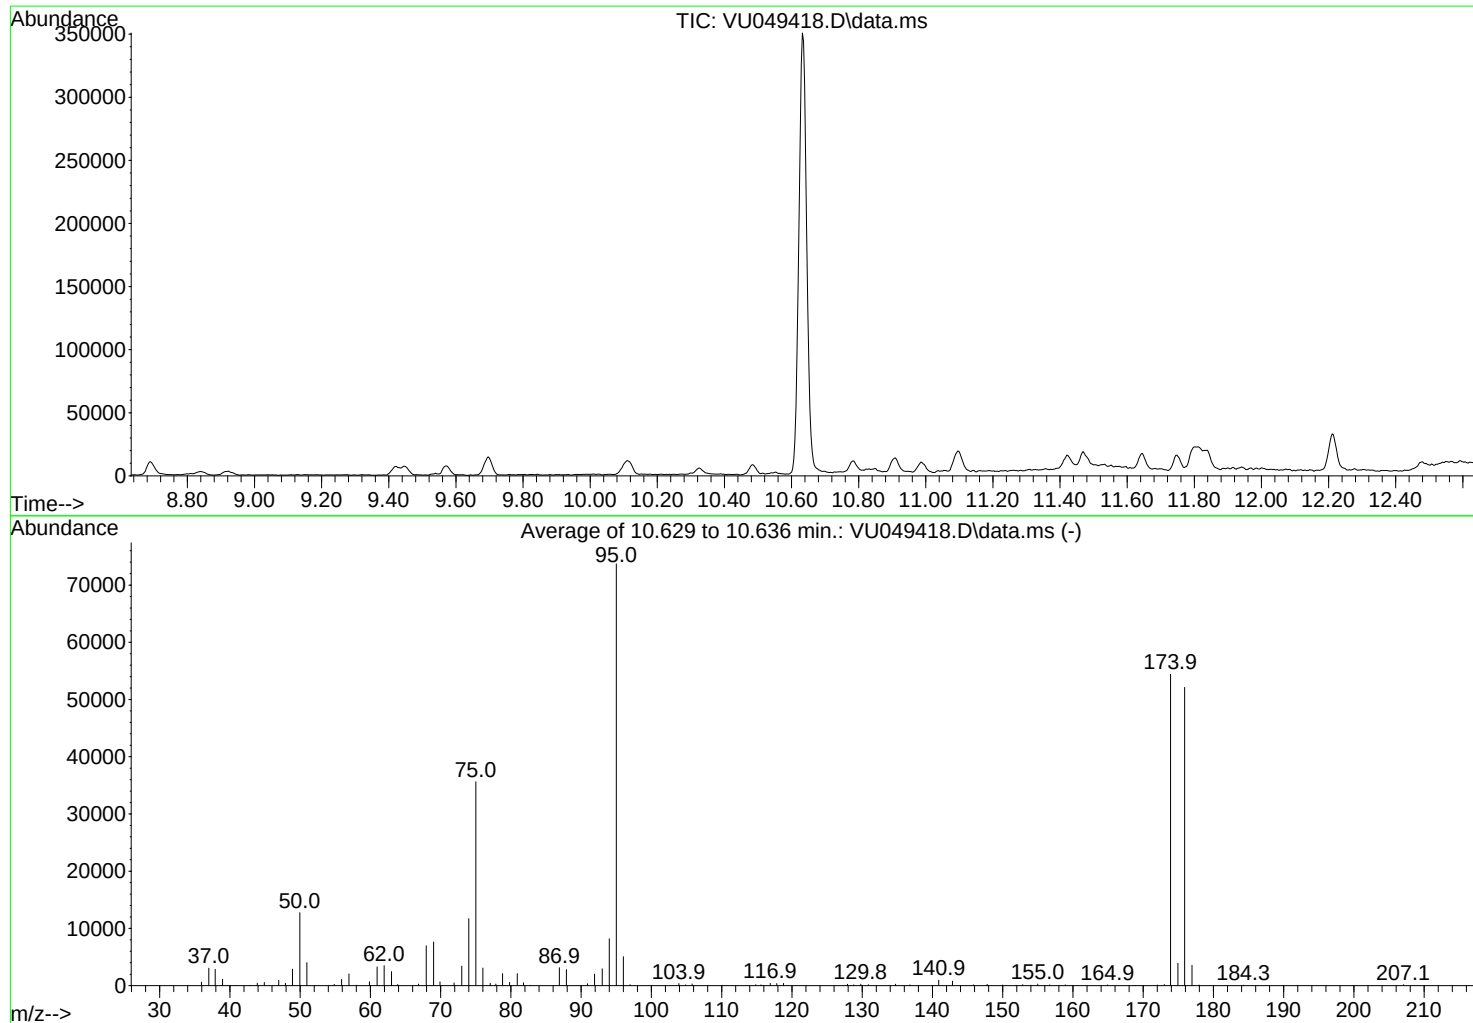

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.3	12753	PASS
75	95	30	60	48.3	35624	PASS
95	95	100	100	100.0	73712	PASS
96	95	5	9	6.9	5068	PASS
173	174	0.00	2	0.4	194	PASS
174	95	50	100	73.8	54411	PASS
175	174	5	9	7.2	3905	PASS
176	174	95	101	95.8	52112	PASS
177	176	5	9	6.8	3554	PASS