


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062818\
 Data File : VU025007.D
 Acq On : 28 Jun 2018 09:19
 Operator : MD/SY
 Sample : BFB
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
 Title : SW846 8260
 Last Update : Wed Jun 13 13:55:26 2018

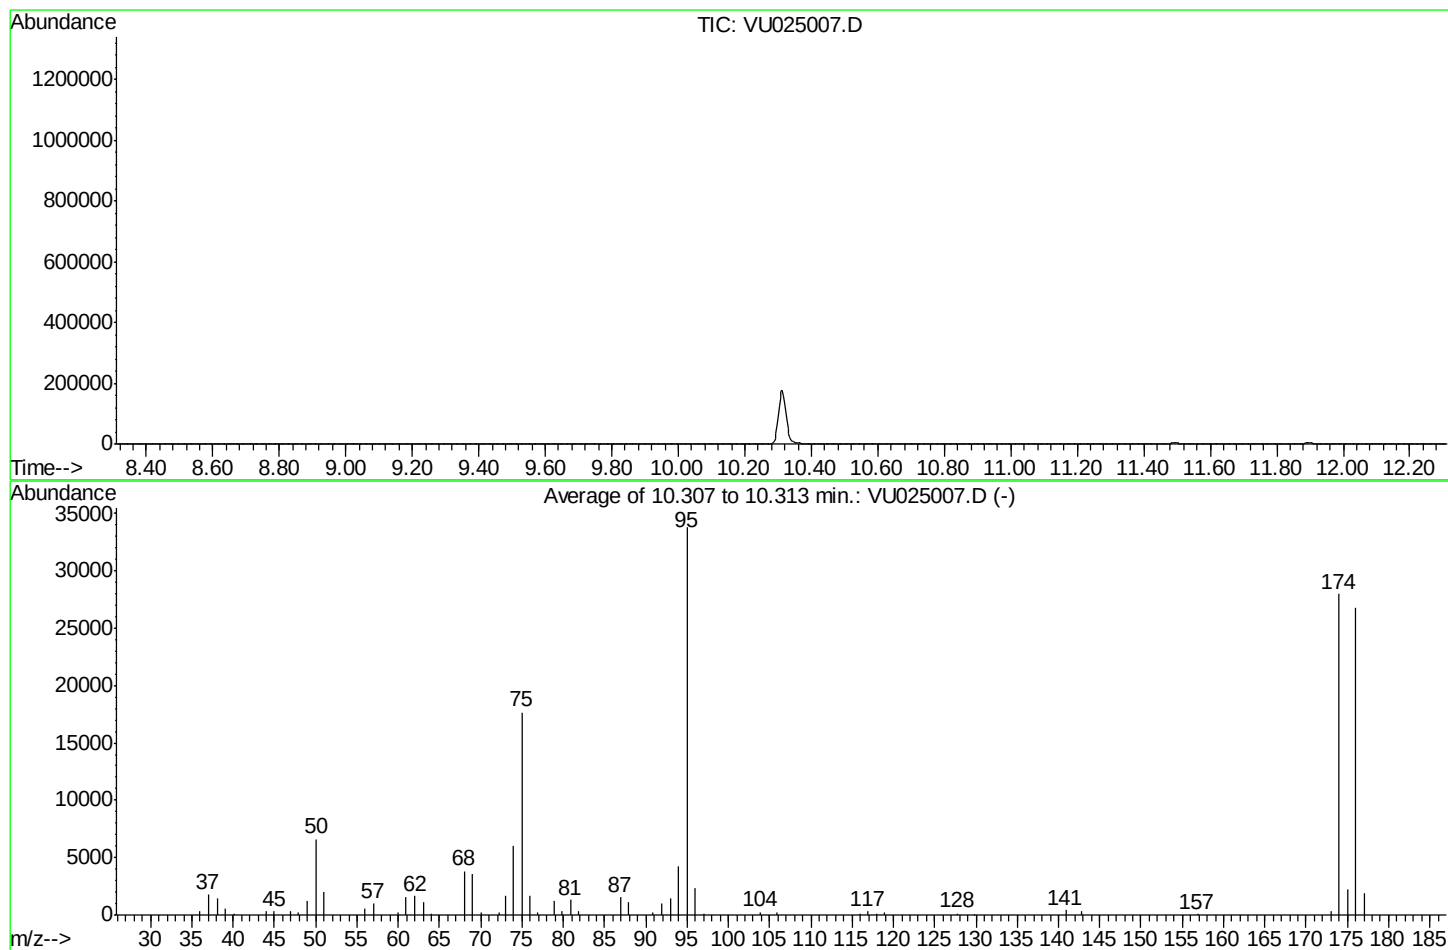

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	6611	PASS
75	95	30	60	52.3	17668	PASS
95	95	100	100	100.0	33781	PASS
96	95	5	9	6.9	2321	PASS
173	174	0.00	2	1.4	386	PASS
174	95	50	100	82.8	27957	PASS
175	174	5	9	8.0	2242	PASS
176	174	95	101	95.8	26789	PASS
177	176	5	9	6.9	1847	PASS