


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062818\
Data File : VU025035.D
Acq On : 28 Jun 2018 21:32
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U061318W.M
Title : SW846 8260
Last Update : Wed Jun 13 13:55:26 2018

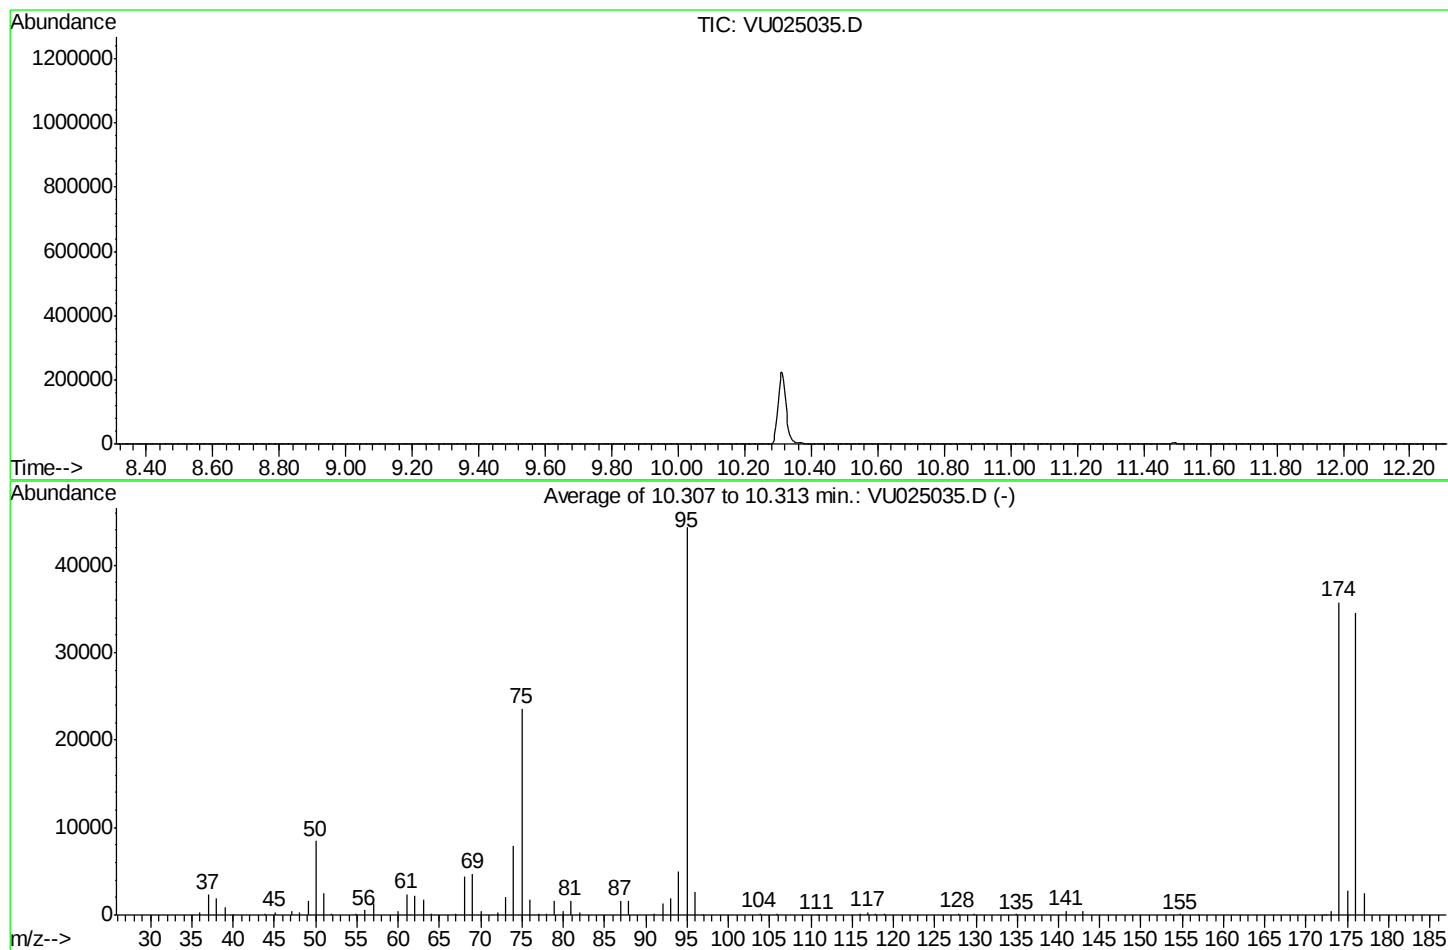

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3010

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	8431	PASS
75	95	30	60	53.3	23629	PASS
95	95	100	100	100.0	44336	PASS
96	95	5	9	6.1	2695	PASS
173	174	0.00	2	1.3	447	PASS
174	95	50	100	80.6	35746	PASS
175	174	5	9	7.7	2760	PASS
176	174	95	101	96.5	34485	PASS
177	176	5	9	7.2	2486	PASS