


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU062819\
Data File : VU033059.D
Acq On : 27 Jun 2019 12:07
Operator : JC/SP
Sample : BFB31
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB31

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM061719WMA.M
Title : VOC Analysis
Last Update : Tue Jul 02 04:16:18 2019

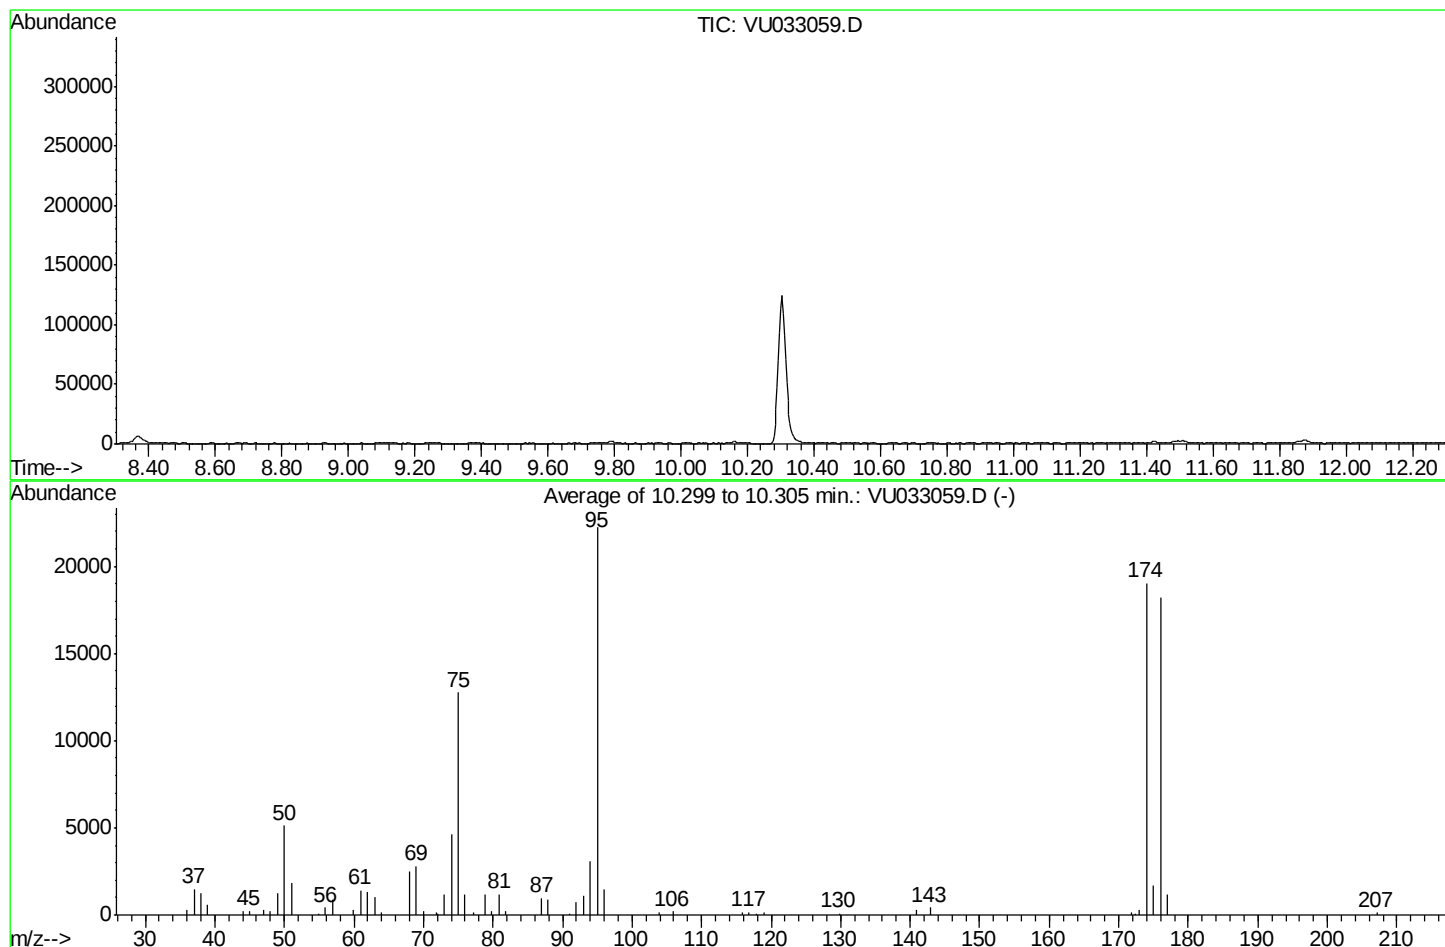

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.1	5139	PASS
75	95	30	80	57.4	12761	PASS
95	95	100	100	100.0	22237	PASS
96	95	5	9	6.6	1460	PASS
173	174	0.00	2	1.6	304	PASS
174	95	50	120	85.6	19032	PASS
175	174	5	9	8.9	1694	PASS
176	174	95	101	95.9	18245	PASS
177	176	5	9	6.6	1209	PASS

Scan 2854 (10.267 min): VU033059.D
BFB31

m/z	Abundance
39.90	168.0
44.00	315.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
35.90	263.0
37.00	1447.0
38.00	1263.0
39.00	506.0
39.90	134.0
44.00	500.0
45.00	219.0
47.10	293.0
47.90	192.0
49.00	1218.0
50.00	4925.0
51.00	1848.0
55.00	116.0
55.90	444.0
57.00	845.0
59.90	223.0
61.00	1323.0
62.00	1210.0
63.00	992.0
64.00	180.0
68.00	2501.0
69.00	2765.0
70.00	278.0
71.80	115.0
73.00	1025.0
74.00	4468.0
75.00	12227.0
76.00	1119.0
77.10	168.0
78.90	1110.0
79.80	192.0
80.90	1156.0
81.80	190.0
87.00	832.0
87.80	816.0
90.90	110.0
91.90	735.0
93.00	1074.0
94.00	2931.0
95.00	21088.0
96.00	1415.0
103.80	156.0
105.90	195.0
115.80	113.0
116.80	177.0
117.90	101.0
118.90	140.0
129.90	102.0
140.90	278.0
142.90	357.0
171.90	154.0
172.90	293.0
174.00	17376.0
175.00	1622.0
176.00	17136.0
176.90	1080.0
207.10	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
35.90	341.0
37.00	1558.0
38.00	1322.0
39.00	615.0
39.90	145.0
44.00	504.0
44.90	227.0
47.10	279.0
47.90	253.0
49.00	1283.0
50.00	5312.0
51.00	1932.0
55.00	106.0
55.90	460.0
57.00	916.0
59.90	268.0
61.00	1500.0
62.00	1355.0
63.00	1077.0
64.00	147.0
68.00	2575.0
69.00	2920.0
70.00	264.0
71.80	138.0
72.10	128.0
73.00	1184.0
74.00	4799.0
75.00	13284.0
76.00	1224.0
77.20	168.0
78.90	1183.0
79.80	225.0
80.90	1247.0
81.80	209.0
87.00	1012.0
87.90	921.0
91.00	110.0
91.90	711.0
93.00	1123.0
94.00	3210.0
95.00	22984.0
96.00	1497.0
103.80	155.0
105.90	232.0
115.80	119.0
116.90	165.0
117.90	100.0
118.90	129.0
129.80	122.0
140.90	298.0
142.90	428.0
171.90	163.0
172.90	303.0
174.00	19656.0
175.00	1785.0
176.00	18848.0
176.90	1240.0
207.10	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
35.90	337.0
37.00	1491.0
38.00	1239.0
39.00	644.0
39.90	149.0
44.00	531.0
44.90	227.0
47.00	256.0
47.90	256.0
49.00	1146.0
50.00	5181.0
51.00	1764.0
55.90	417.0
57.00	919.0
59.90	292.0
61.00	1442.0
62.00	1305.0
63.00	1081.0
63.90	118.0
68.00	2468.0
69.00	2760.0
70.00	216.0
71.90	172.0
73.00	1275.0
74.00	4660.0
75.00	12772.0
76.00	1189.0
77.20	132.0
78.90	1173.0
79.80	263.0
80.90	1227.0
81.80	220.0
87.00	1038.0
87.90	958.0
91.00	107.0
91.90	669.0
93.00	1076.0
94.00	3182.0
95.00	22640.0
96.00	1469.0
103.90	137.0
105.90	213.0
115.80	134.0
116.90	155.0
119.00	106.0
129.80	113.0
140.90	319.0
142.90	439.0
171.90	166.0
172.30	179.0
173.00	317.0
174.00	20064.0
175.00	1676.0
176.00	18752.0
177.00	1307.0
207.10	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31