

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
 Data File : VU049464.D
 Acq On : 28 Jun 2022 17:31
 Operator : SY/MD
 Sample : N3480-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 30985

Quant Time: Jun 28 17:56:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 28 10:35:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.372	168	306794	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.250	114	533963	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.417	117	479710	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	231039	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.700	65	201406	42.627	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	85.260%		
35) Dibromofluoromethane	5.288	113	164711	44.091	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	88.180%		
50) Toluene-d8	7.896	98	633151	47.518	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	95.040%		
62) 4-Bromofluorobenzene	10.632	95	237499	46.531	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	93.060%		
Target Compounds						
						Qvalue
3) Chloromethane	1.520	50	1923	Below Cal		91
6) Chloroethane	1.948	64	69	1.944 ug/l	#	44
11) Tert butyl alcohol	3.192	59	3732	3.375 ug/l	#	41
16) Acetone	2.626	43	109292	45.869 ug/l		99
17) Carbon Disulfide	2.793	76	3772	0.363 ug/l		97
20) Methylene Chloride	3.047	84	409	Below Cal	#	81
25) 2-Butanone	4.713	43	17741	4.968 ug/l	#	86
31) Cyclohexane	5.372	56	7257	1.023 ug/l	#	11
36) 1,1-Dichloropropene	5.372	75	24124	4.454 ug/l	#	49
38) Carbon Tetrachloride	5.372	117	31303	5.510 ug/l	#	16
39) Methylcyclohexane	6.764	83	2988	0.460 ug/l		95
51) 4-Methyl-2-Pentanone	7.793	43	3603	0.496 ug/l		91
52) Toluene	7.970	92	8741	0.899 ug/l		92
55) 1,1,2-Trichloroethane	8.369	97	1231	0.306 ug/l	#	14
59) 2-Hexanone	8.690	43	3218	0.564 ug/l		98
67) Ethyl Benzene	9.571	91	5351	0.297 ug/l		98
68) m/p-Xylenes	9.693	106	6269	0.941 ug/l		90
69) o-Xylene	10.102	106	5972	0.903 ug/l		92
74) N-amyl acetate	10.388	43	5106	0.586 ug/l	#	44
76) 1,2,3-Trichloropropane	10.632	75	117471	14.999 ug/l	#	46
78) n-propylbenzene	10.905	91	5513	0.276 ug/l		92
80) 1,3,5-Trimethylbenzene	11.086	105	7505	0.522 ug/l		97
81) trans-1,4-Dichloro-2-b...	10.632	75	117471	55.389 ug/l	#	15
84) 1,2,4-Trimethylbenzene	11.468	105	20436	1.448 ug/l		93
85) sec-Butylbenzene	11.645	105	3817	0.215 ug/l		84
86) p-Isopropyltoluene	11.793	119	3583	0.249 ug/l	#	66
89) n-Butylbenzene	12.192	91	4600	0.346 ug/l	#	32
90) Hexachloroethane	12.497	117	750	0.262 ug/l	#	5
95) Naphthalene	14.085	128	11288	2.338 ug/l	#	91
96) 1,2,3-Trichlorobenzene	14.346	180	285	1.229 ug/l	#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049464.D
Acq On : 28 Jun 2022 17:31
Operator : SY/MD
Sample : N3480-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
30985

Quant Time: Jun 28 17:56:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 28 10:35:43 2022
Response via : Initial Calibration




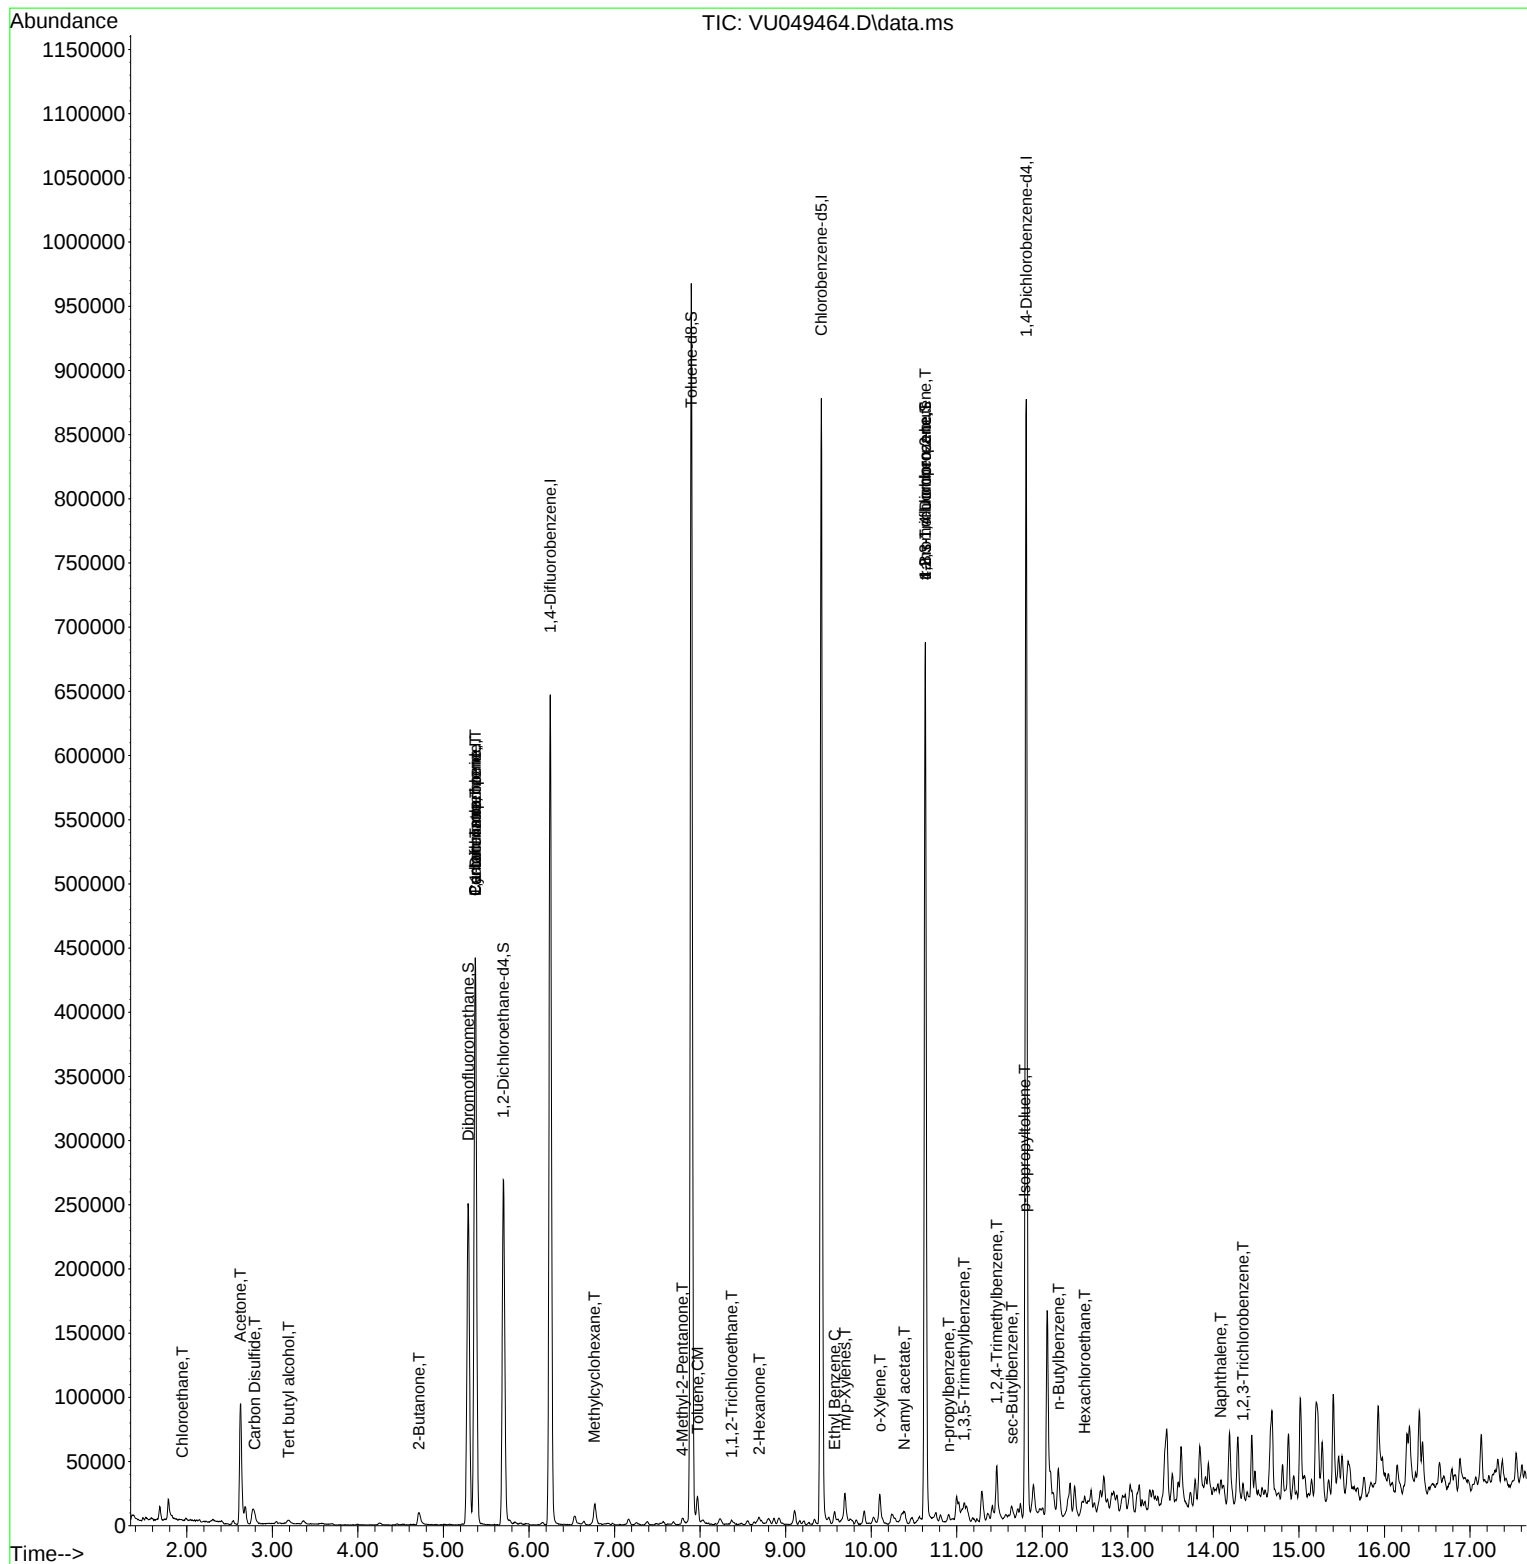




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.372 min Scan# 11
Delta R.T. 0.003 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31




Instrument :
MSVOA_U
ClientSampleId :
30985

Tgt Ion:168 Resp: 306794
Ion Ratio Lower Upper
168 100
99 59.6 39.3 58.9#

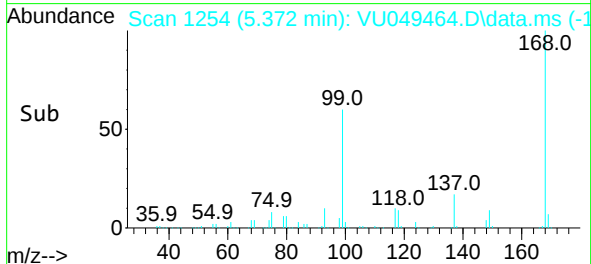

#3
Chloromethane
Concen: Below Cal
RT: 1.520 min Scan# 56
Delta R.T. -0.000 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31

Tgt Ion: 50 Resp: 1923
Ion Ratio Lower Upper
50 100
52 39.2 27.4 41.2


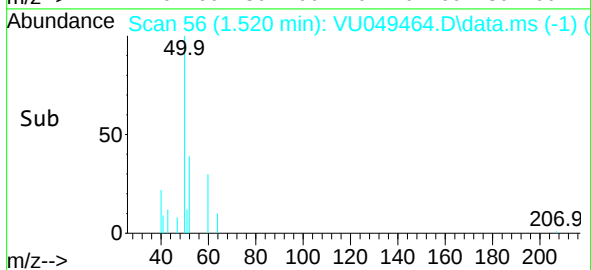

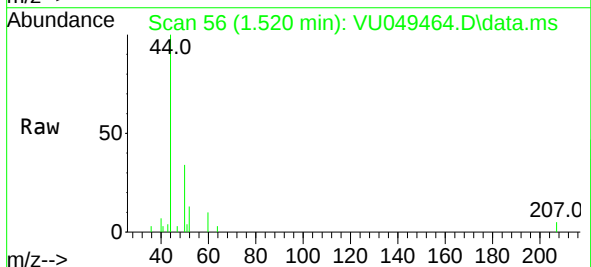




#6
Chloroethane
Concen: 1.944 ug/l
RT: 1.948 min Scan# 11
Delta R.T. 0.039 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31




Instrument :
MSVOA_U
ClientSampleId :
30985


Tgt Ion: 64 Resp: 69
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#

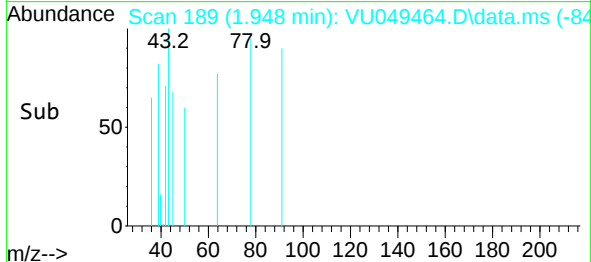

#11
Tert butyl alcohol
Concen: 3.375 ug/l
RT: 3.192 min Scan# 576
Delta R.T. -0.119 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31

Tgt Ion: 59 Resp: 3732
Ion Ratio Lower Upper
59 100
57 2.6 30.6 45.8#


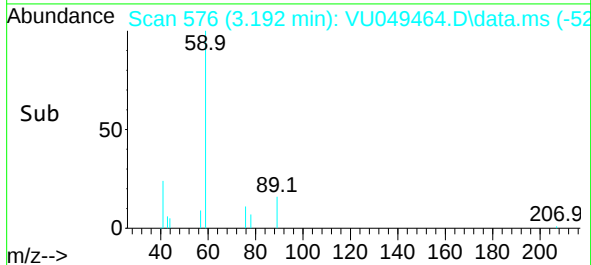

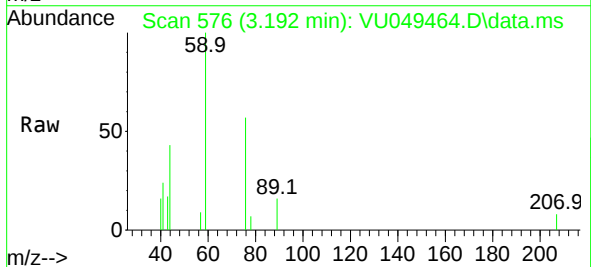




#16
Acetone
Concen: 45.869 ug/l
RT: 2.626 min Scan# 403
Delta R.T. -0.010 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31




Instrument :
MSVOA_U
ClientSampleId :
30985


Tgt Ion: 43 Resp: 109292
Ion Ratio Lower Upper
43 100
58 33.6 27.5 41.3

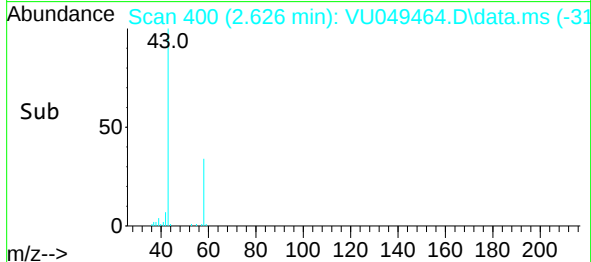

#17
Carbon Disulfide
Concen: 0.363 ug/l
RT: 2.793 min Scan# 452
Delta R.T. 0.016 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31

Tgt Ion: 76 Resp: 3772
Ion Ratio Lower Upper
76 100
78 10.2 7.3 10.9

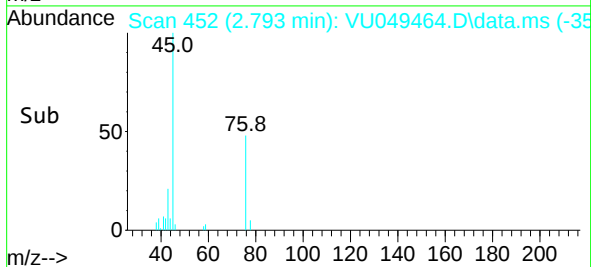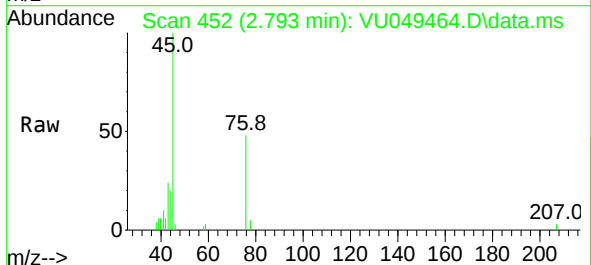



#20

Methylene Chloride

Concen: Below Cal

RT: 3.047 min Scan# 51

Delta R.T. 0.010 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31

Instrument :

MSVOA_U

ClientSampleId :

30985

Tgt Ion: 84 Resp: 409





Ion Ratio Lower Upper

84 100

49 124.3 86.6 129.8

51 68.6 26.6 40.0#

86 65.7 50.6 75.8

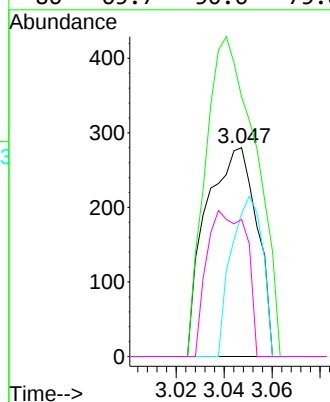

#25

2-Butanone

Concen: 4.968 ug/l

RT: 4.713 min Scan# 1049

Delta R.T. 0.003 min

Lab File: VU049464.D




Acq: 28 Jun 2022 17:31


Tgt Ion: 43 Resp: 17741

Ion Ratio Lower Upper

43 100

72 22.4 23.8 35.6#

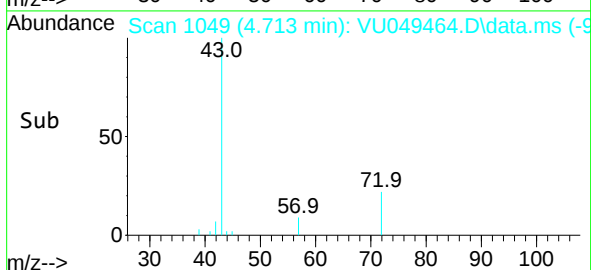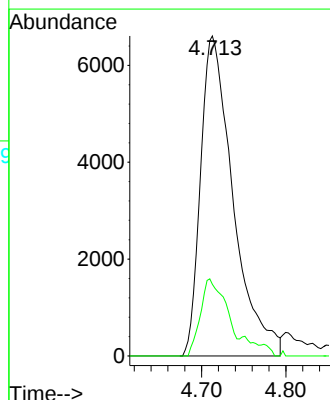

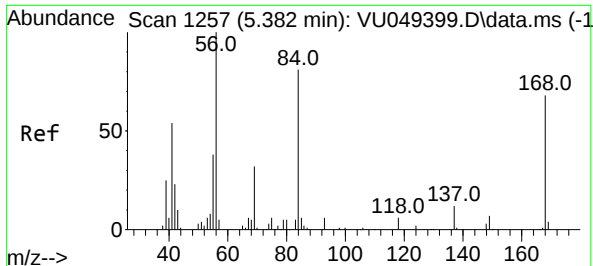

#31

Cyclohexane

Concen: 1.023 ug/l

RT: 5.372 min Scan# 1257

Delta R.T. -0.010 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31

Instrument :

MSVOA_U

ClientSampleId :

30985





Tgt Ion: 56 Resp: 7257

Ion Ratio Lower Upper

56 100

69 161.8 27.8 41.8#

84 131.3 74.2 111.4#

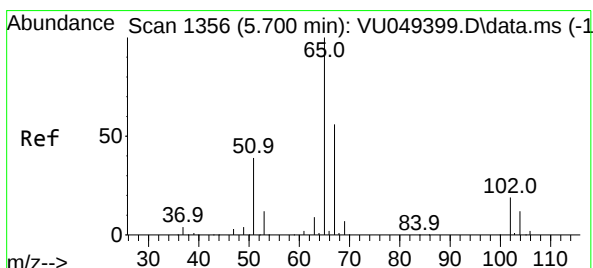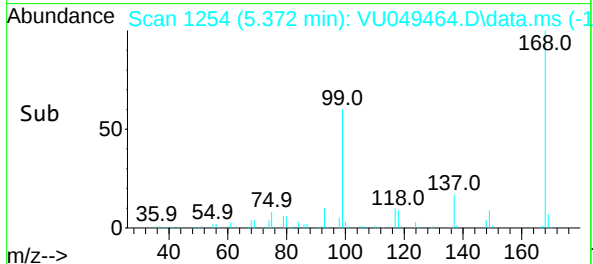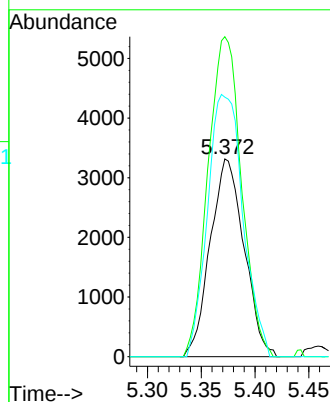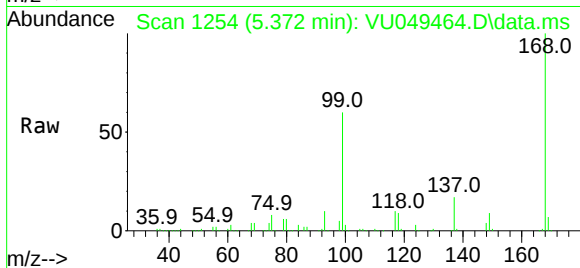

#33

1,2-Dichloroethane-d4

Concen: 42.627 ug/l

RT: 5.700 min Scan# 1356

Delta R.T. -0.000 min

Lab File: VU049464.D




Acq: 28 Jun 2022 17:31


Tgt Ion: 65 Resp: 201406

Ion Ratio Lower Upper

65 100

67 54.6 0.0 108.0

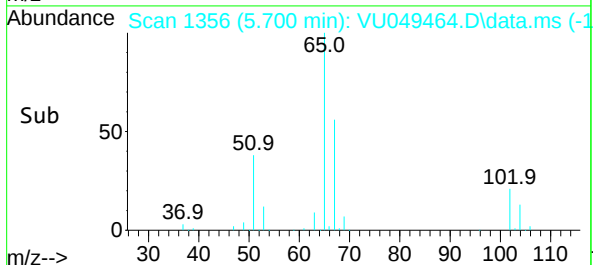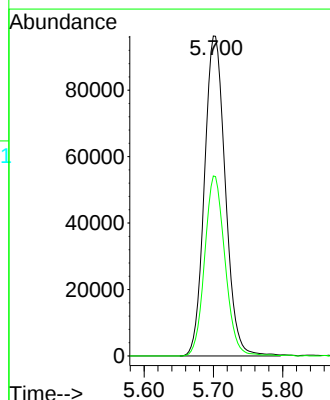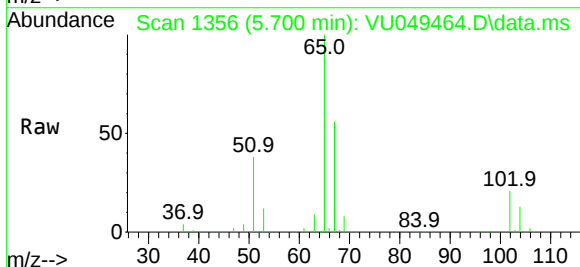

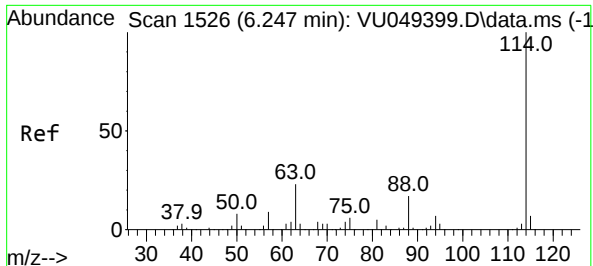

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.250 min Scan# 11

Delta R.T. 0.003 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31

Instrument :

MSVOA_U

ClientSampleId :

30985





Tgt Ion:114 Resp: 533963

Ion Ratio Lower Upper

114 100

63 21.5 0.0 37.8

88 16.5 0.0 29.2

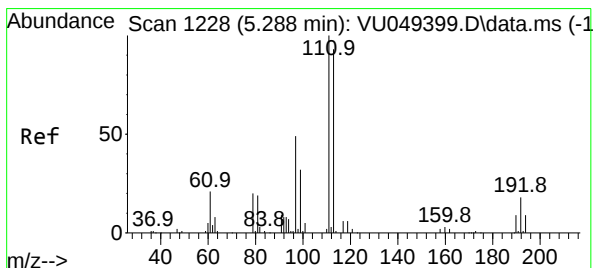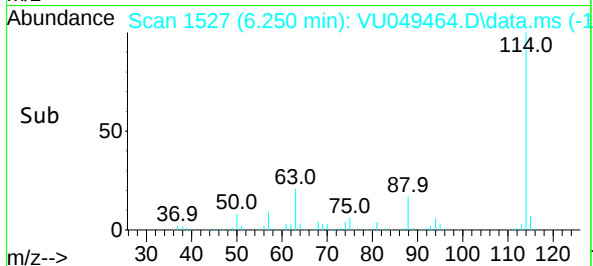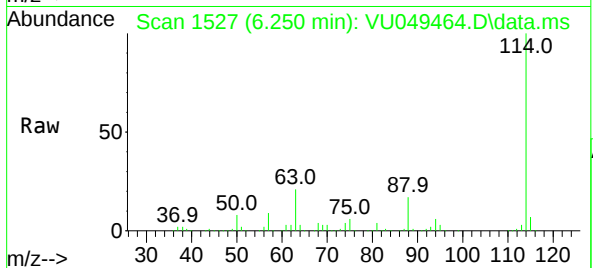

#35

Dibromofluoromethane

Concen: 44.091 ug/l

RT: 5.288 min Scan# 1228

Delta R.T. -0.000 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31




Tgt Ion:113 Resp: 164711


Ion Ratio Lower Upper

113 100

111 102.4 82.1 123.1

192 18.7 18.0 27.0

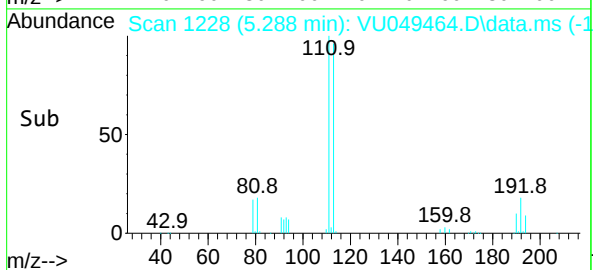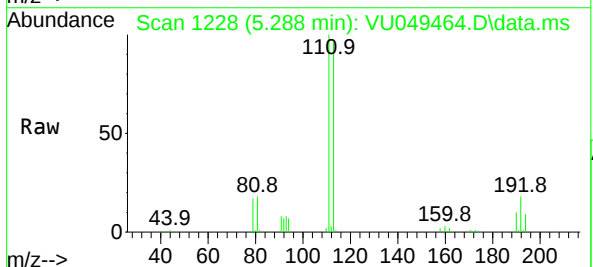

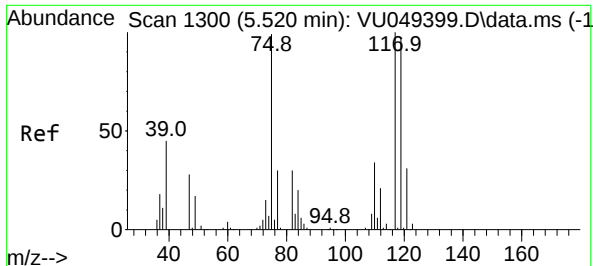

#36

1,1-Dichloropropene

Concen: 4.454 ug/l

RT: 5.372 min Scan# 11

Delta R.T. -0.148 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31

Instrument :

MSVOA_U

ClientSampleId :

30985





Tgt Ion: 75 Resp: 24124

Ion Ratio Lower Upper

75 100

110 8.9 18.4 55.2#

77 0.0 25.1 37.7#

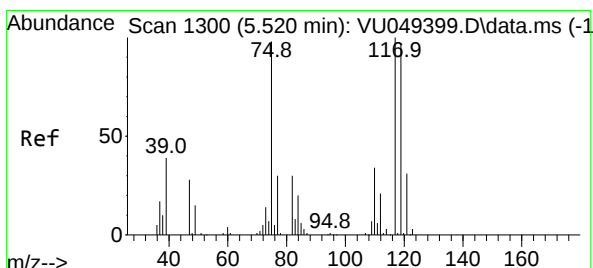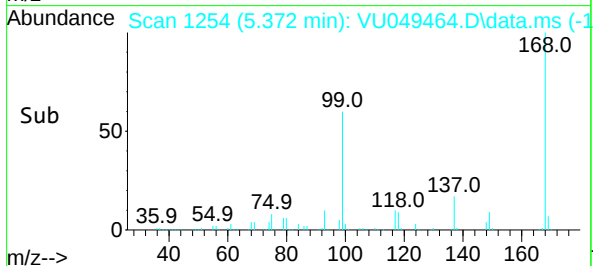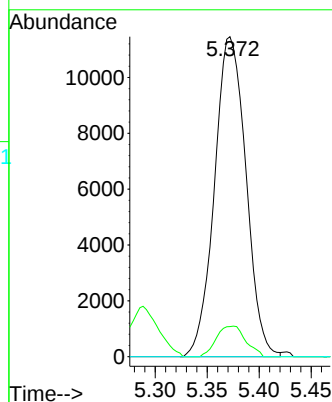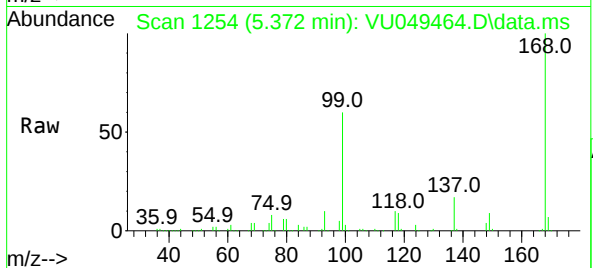

#38

Carbon Tetrachloride

Concen: 5.510 ug/l

RT: 5.372 min Scan# 1254

Delta R.T. -0.148 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31




Tgt Ion: 117 Resp: 31303


Ion Ratio Lower Upper

117 100

119 5.5 76.8 115.2#

121 0.0 24.7 37.1#

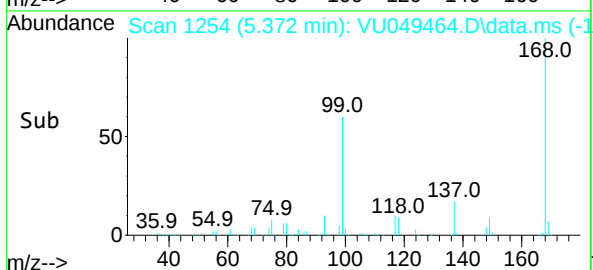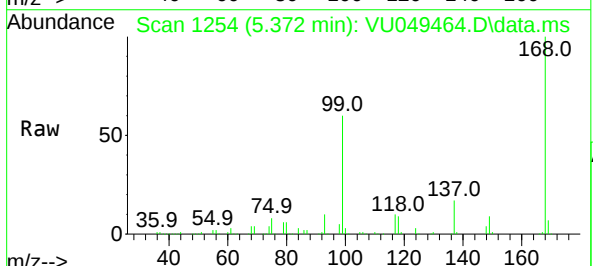

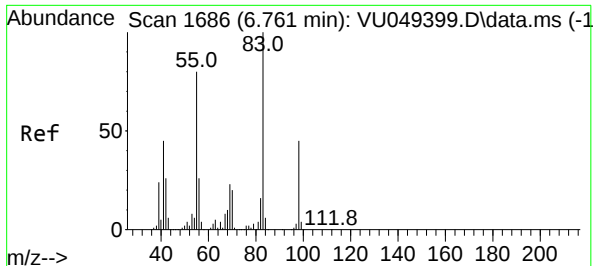

#39

Methylcyclohexane

Concen: 0.460 ug/l

RT: 6.764 min Scan# 1

Delta R.T. 0.003 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31

Instrument :

MSVOA_U

ClientSampleId :

30985





Tgt Ion: 83 Resp: 2988

Ion Ratio Lower Upper

83 100

55 61.8 55.3 82.9

98 46.5 37.3 55.9

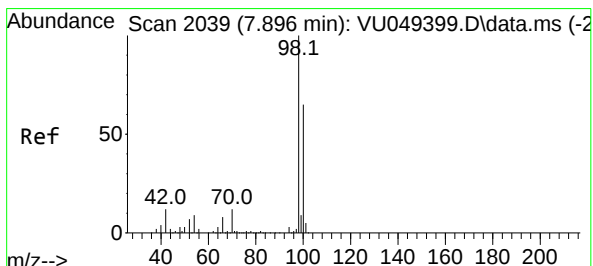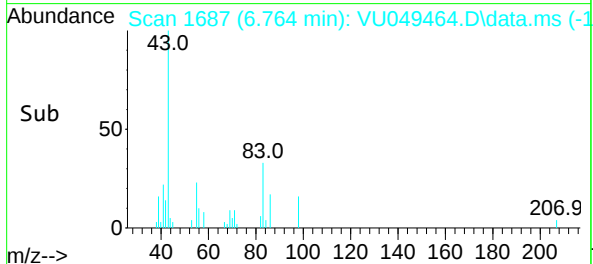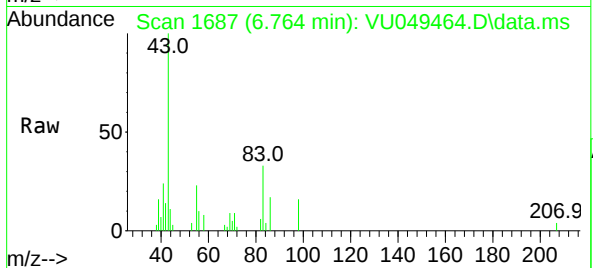

#50

Toluene-d8

Concen: 47.518 ug/l

RT: 7.896 min Scan# 2039

Delta R.T. -0.000 min

Lab File: VU049464.D




Acq: 28 Jun 2022 17:31


Tgt Ion: 98 Resp: 633151

Ion Ratio Lower Upper

98 100

100 65.1 51.7 77.5

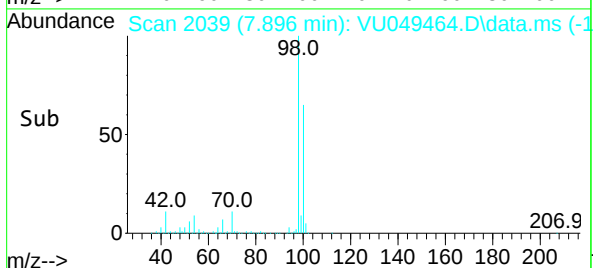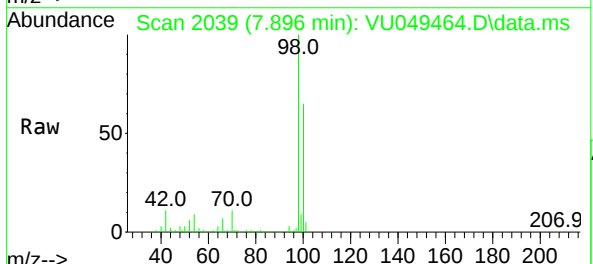

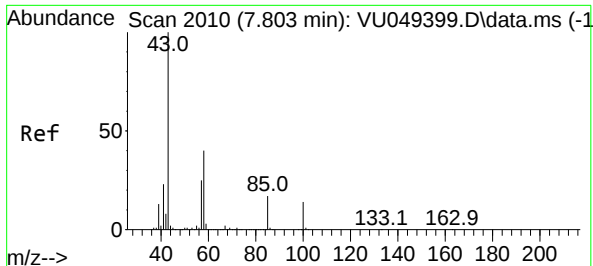

#51

4-Methyl-2-Pentanone

Concen: 0.496 ug/l

RT: 7.793 min Scan# 20

Delta R.T. -0.010 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31

Instrument :

MSVOA_U

ClientSampleId :





30985

Tgt Ion: 43 Resp: 3603

Ion Ratio Lower Upper

43 100

58 37.6 34.7 52.1

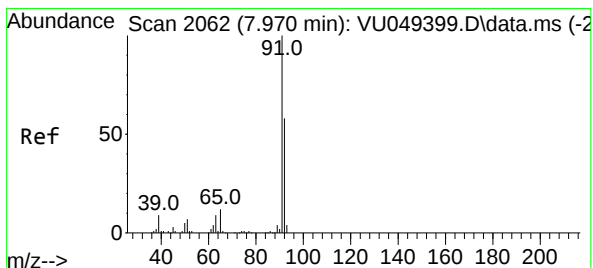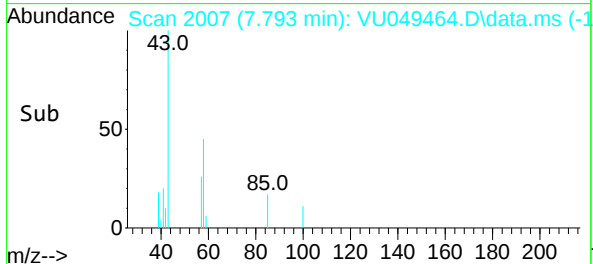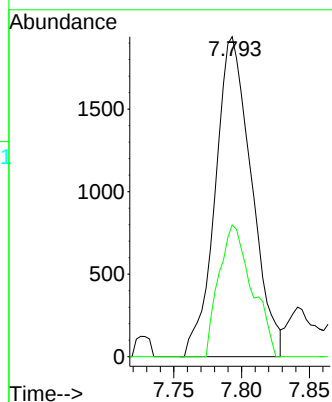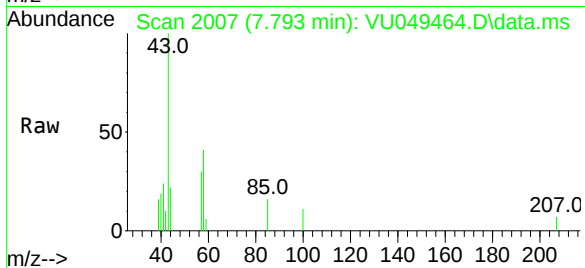

#52

Toluene

Concen: 0.899 ug/l

RT: 7.970 min Scan# 2062

Delta R.T. -0.000 min

Lab File: VU049464.D




Acq: 28 Jun 2022 17:31


Tgt Ion: 92 Resp: 8741

Ion Ratio Lower Upper

92 100


91 161.1 138.2 207.4

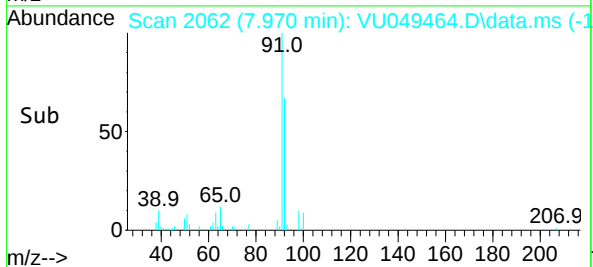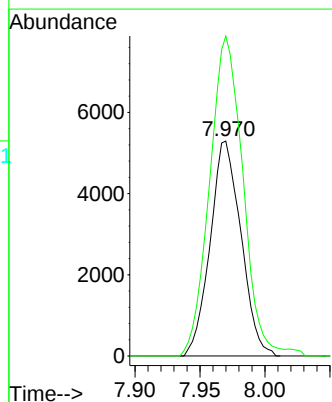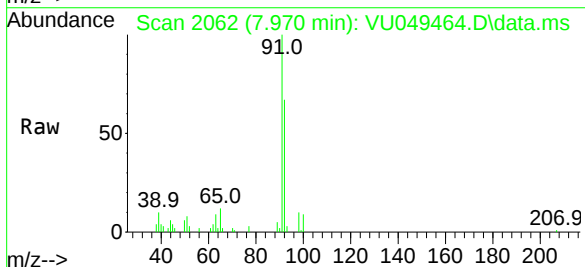






#55
 1,1,2-Trichloroethane
 Concen: 0.306 ug/l
 RT: 8.369 min Scan# 2197
 Delta R.T. -0.035 min
 Lab File: VU049464.D
 Acq: 28 Jun 2022 17:31

Instrument :
 MSVOA_U
 ClientSampleId :
 30985



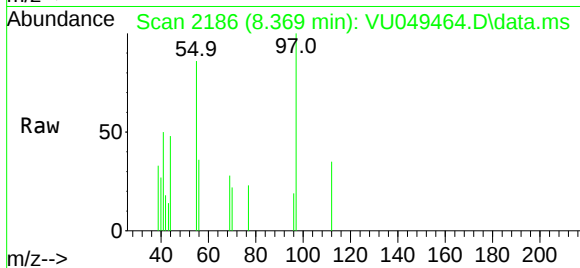



Tgt Ion: 97 Resp: 1231
 Ion Ratio Lower Upper
 97 100
 83 0.0 70.2 105.4#
 85 0.0 44.6 66.8#
 99 0.0 51.0 76.6#

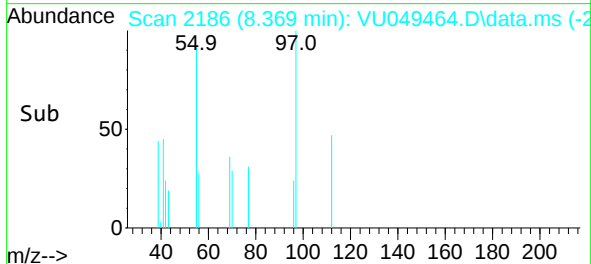

#59
 2-Hexanone
 Concen: 0.564 ug/l
 RT: 8.690 min Scan# 2286
 Delta R.T. -0.006 min
 Lab File: VU049464.D
 Acq: 28 Jun 2022 17:31

Tgt Ion: 43 Resp: 3218
 Ion Ratio Lower Upper
 43 100
 58 58.8 30.3 90.8




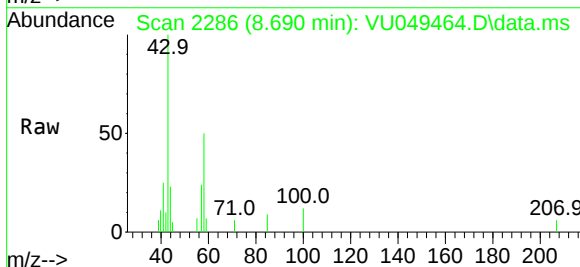




#62
4-Bromofluorobenzene
Concen: 46.531 ug/l
RT: 10.632 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31




Instrument :
MSVOA_U
ClientSampleId :
30985


Tgt Ion: 95 Resp: 237499
Ion Ratio Lower Upper
95 100
174 75.3 0.0 182.0
176 72.4 0.0 177.8

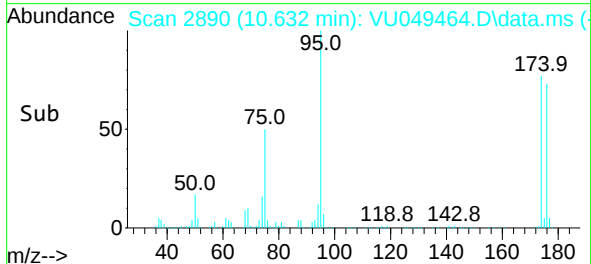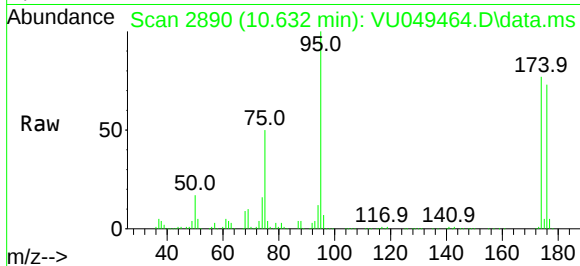

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.417 min Scan# 2512
Delta R.T. -0.003 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31

Tgt Ion: 117 Resp: 479710
Ion Ratio Lower Upper
117 100
82 58.4 41.7 62.5
119 32.3 25.7 38.5

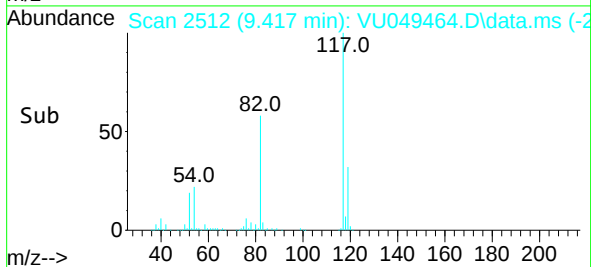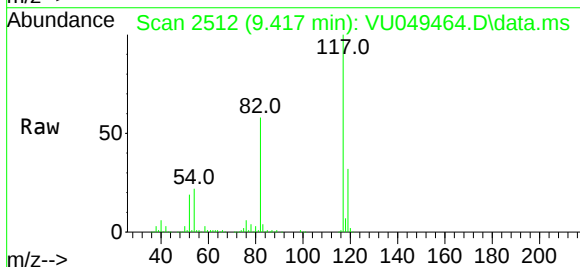



#67

Ethyl Benzene

Concen: 0.297 ug/l

RT: 9.571 min Scan# 2560

Delta R.T. -0.000 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31

Instrument :

MSVOA_U

ClientSampleId :





30985

Tgt Ion: 91 Resp: 5351

Ion Ratio Lower Upper

91 100

106 31.0 25.6 38.4

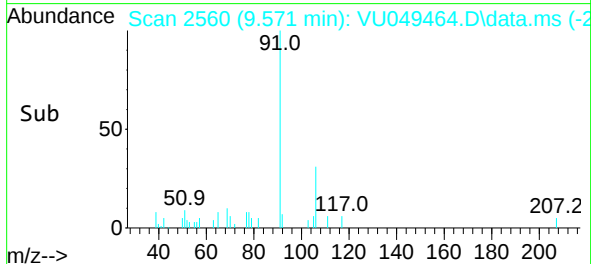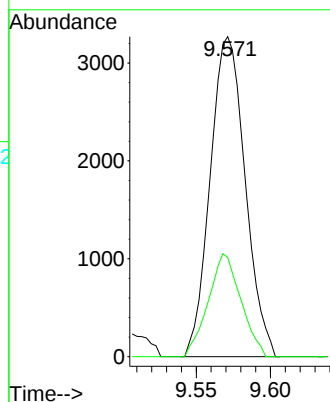

#68

m/p-Xylenes

Concen: 0.941 ug/l

RT: 9.693 min Scan# 2598

Delta R.T. -0.000 min

Lab File: VU049464.D




Acq: 28 Jun 2022 17:31


Tgt Ion: 106 Resp: 6269

Ion Ratio Lower Upper

106 100

91 211.5 157.2 235.8

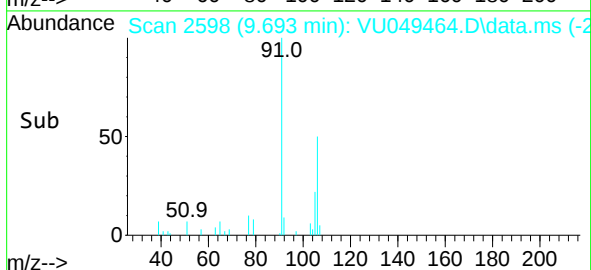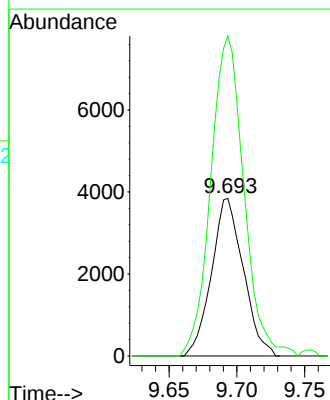



#69

o-Xylene

Concen: 0.903 ug/l

RT: 10.102 min Scan# 21

Delta R.T. -0.000 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31

Instrument :

MSVOA_U

ClientSampleId :





30985

Tgt Ion:106 Resp: 5972

Ion Ratio Lower Upper

106 100

91 218.8 103.5 310.5

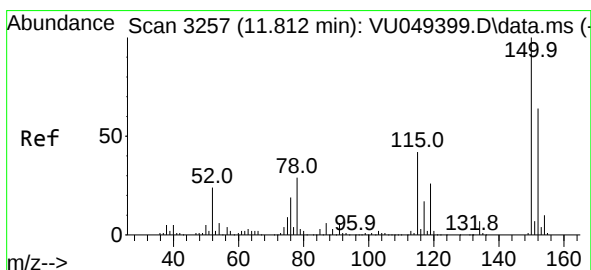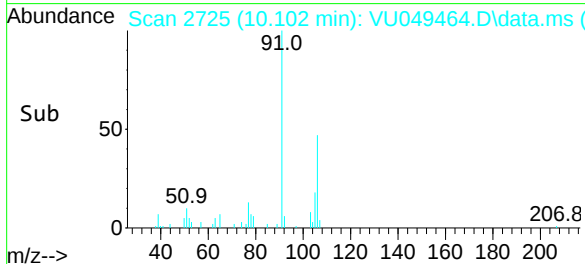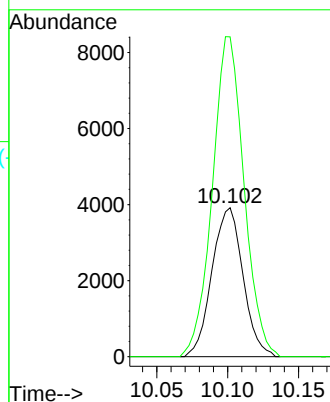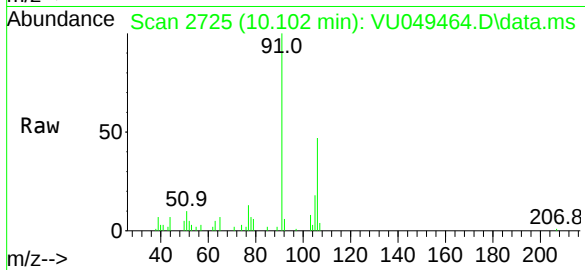

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 11.812 min Scan# 3257

Delta R.T. -0.000 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31




Tgt Ion:152 Resp: 231039


Ion Ratio Lower Upper

152 100

115 61.5 37.0 110.9


150 156.6 0.0 342.2

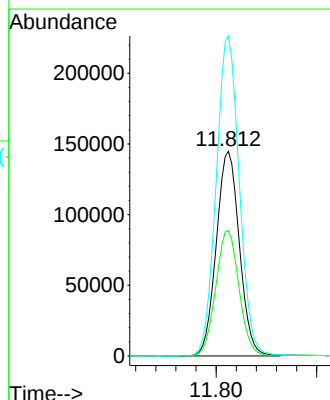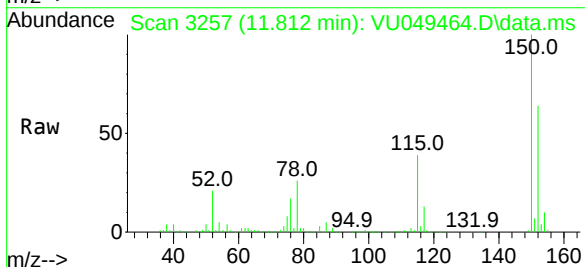






#74
N-amy1 acetate
Concen: 0.586 ug/l
RT: 10.388 min Scan# 2814
Delta R.T. 0.064 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31

Instrument :
MSVOA_U
ClientSampleId :
30985







Tgt Ion: 43 Resp: 5106
Ion Ratio Lower Upper
43 100
70 7.4 38.7 58.1#
55 0.0 21.8 32.8#
61 0.0 21.9 32.9#

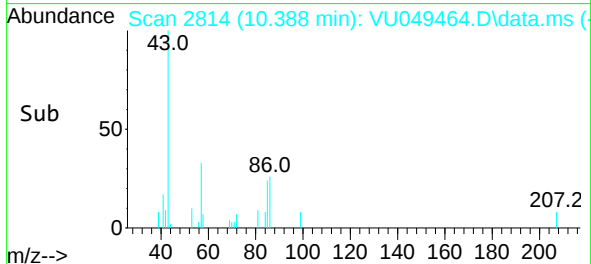

#76
1,2,3-Trichloropropane
Concen: 14.999 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.196 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31

Tgt Ion: 75 Resp: 117471
Ion Ratio Lower Upper
75 100
77 1.3 15.8 47.3#

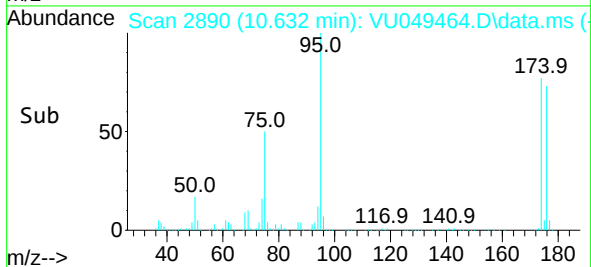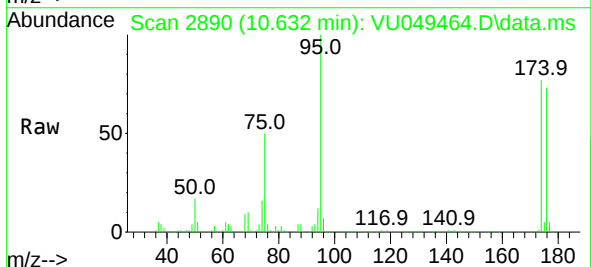



#78

n-propylbenzene

Concen: 0.276 ug/l

RT: 10.905 min Scan# 2975

Delta R.T. -0.000 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31

Instrument :

MSVOA_U

ClientSampleId :





30985

Tgt Ion: 91 Resp: 5513

Ion Ratio Lower Upper

91 100

120 19.6 11.9 35.5

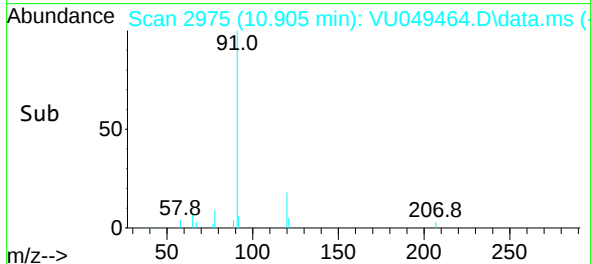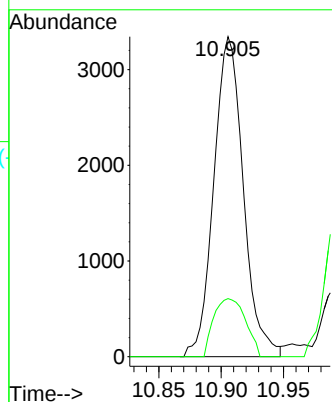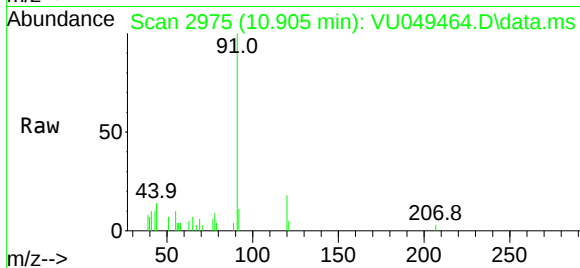

#80

1,3,5-Trimethylbenzene

Concen: 0.522 ug/l

RT: 11.086 min Scan# 3031

Delta R.T. -0.003 min

Lab File: VU049464.D




Acq: 28 Jun 2022 17:31


Tgt Ion: 105 Resp: 7505

Ion Ratio Lower Upper

105 100

120 48.5 25.3 75.9


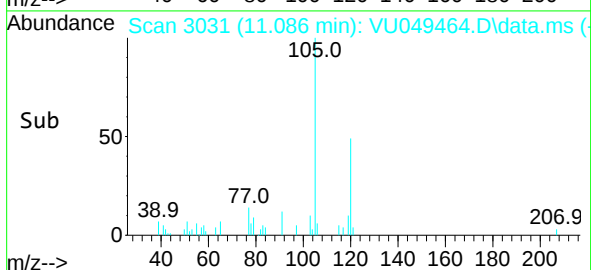

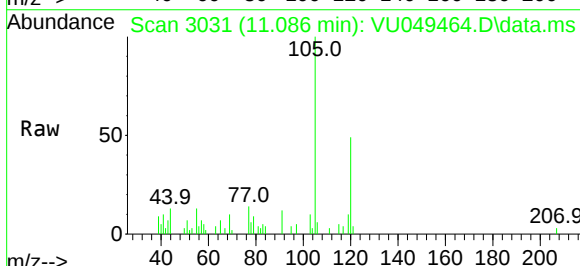




#81
trans-1,4-Dichloro-2-butene
Concen: 55.389 ug/l
RT: 10.632 min Scan# 21
Delta R.T. 0.084 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31




Instrument :
MSVOA_U
ClientSampleId :
30985


Tgt Ion: 75 Resp: 117471
Ion Ratio Lower Upper
75 100
53 0.1 69.2 103.8#
89 0.0 37.0 55.6#

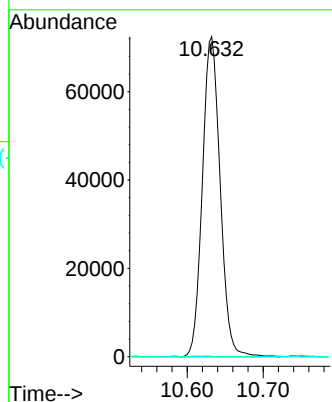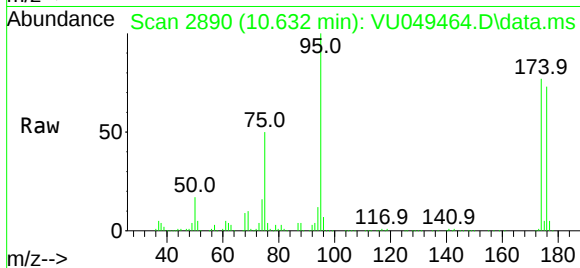

#84
1,2,4-Trimethylbenzene
Concen: 1.448 ug/l
RT: 11.468 min Scan# 3150
Delta R.T. -0.000 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31

Tgt Ion:105 Resp: 20436
Ion Ratio Lower Upper
105 100
120 42.5 23.4 70.3


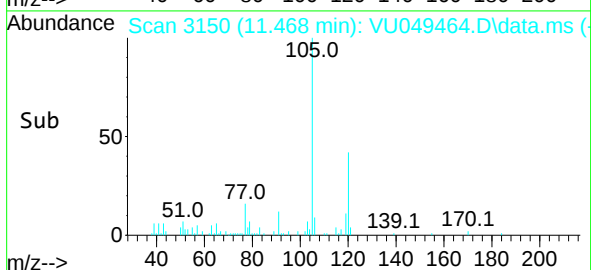

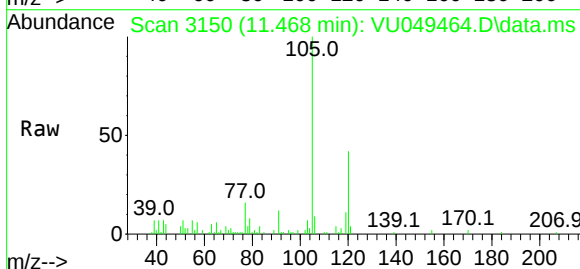


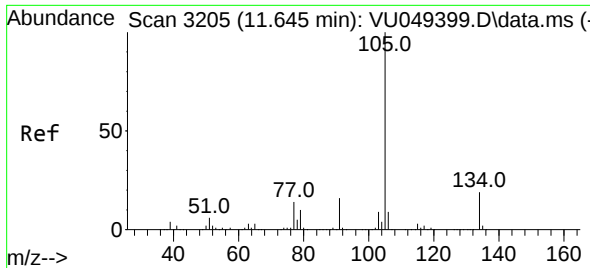

#85
 sec-Butylbenzene
 Concen: 0.215 ug/l
 RT: 11.645 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VU049464.D
 Acq: 28 Jun 2022 17:31




Instrument :
 MSVOA_U
 ClientSampleId :
 30985


Tgt Ion:105 Resp: 3817
 Ion Ratio Lower Upper
 105 100
 134 13.2 10.4 31.1

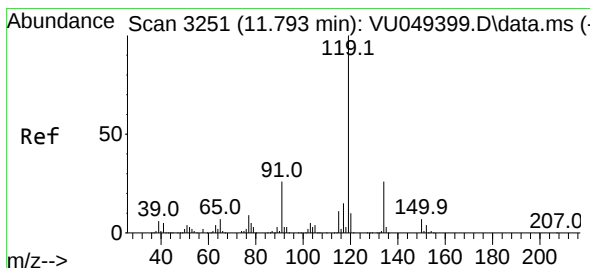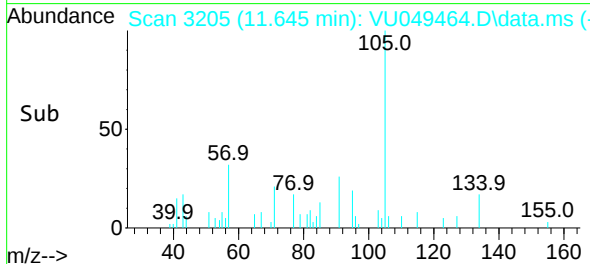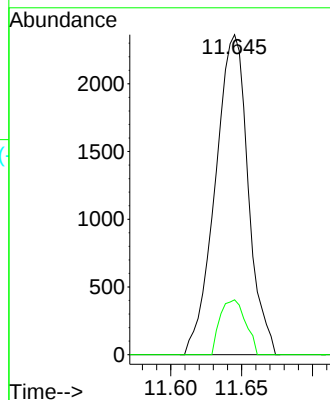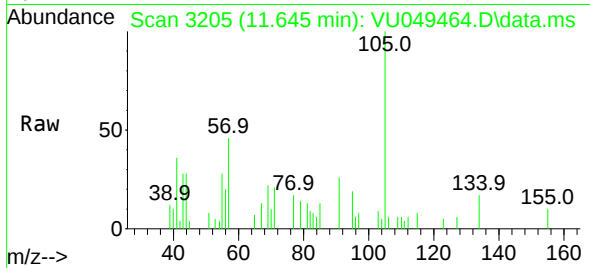

#86
 p-Isopropyltoluene
 Concen: 0.249 ug/l
 RT: 11.793 min Scan# 3251
 Delta R.T. -0.000 min
 Lab File: VU049464.D
 Acq: 28 Jun 2022 17:31

Tgt Ion:119 Resp: 3583
 Ion Ratio Lower Upper
 119 100
 134 31.8 13.5 40.4
 91 53.0 11.2 33.5#

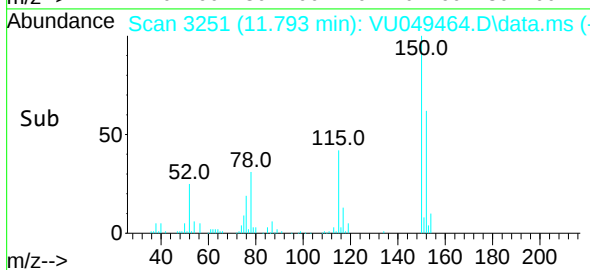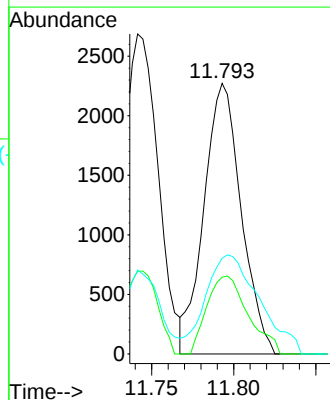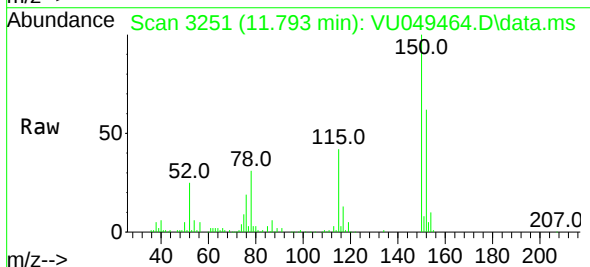



#89

n-Butylbenzene

Concen: 0.346 ug/l

RT: 12.192 min Scan# 31

Delta R.T. -0.016 min

Lab File: VU049464.D

Acq: 28 Jun 2022 17:31

Instrument :

MSVOA_U

ClientSampleId :

30985





Tgt Ion: 91 Resp: 4600

Ion Ratio Lower Upper

91 100

92 34.3 26.2 78.6

134 104.2 13.5 40.4#

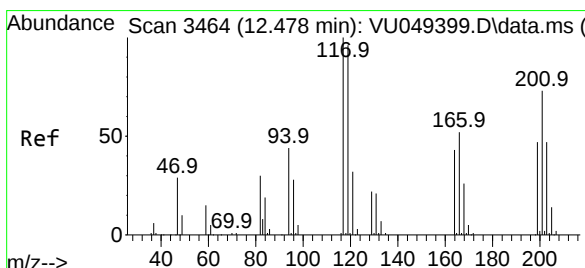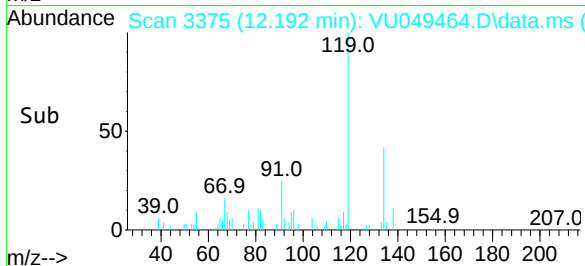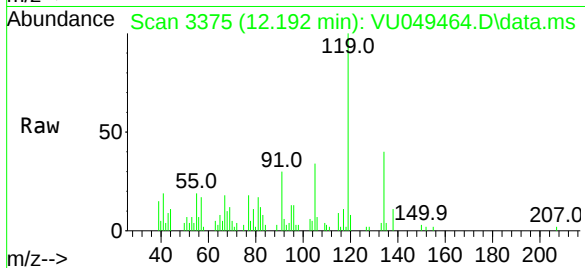

#90

Hexachloroethane

Concen: 0.262 ug/l

RT: 12.497 min Scan# 3470

Delta R.T. 0.019 min

Lab File: VU049464.D




Acq: 28 Jun 2022 17:31


Tgt Ion: 117 Resp: 750

Ion Ratio Lower Upper

117 100

201 0.0 44.6 134.0#


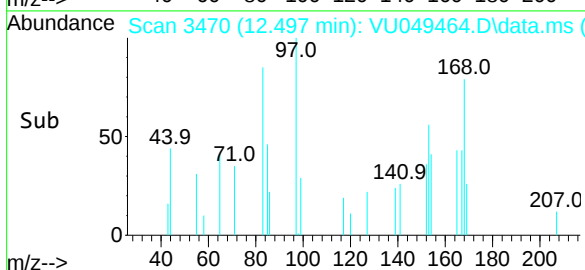

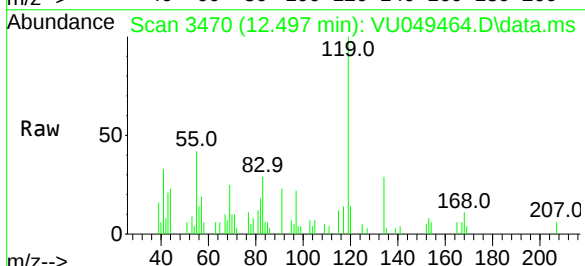


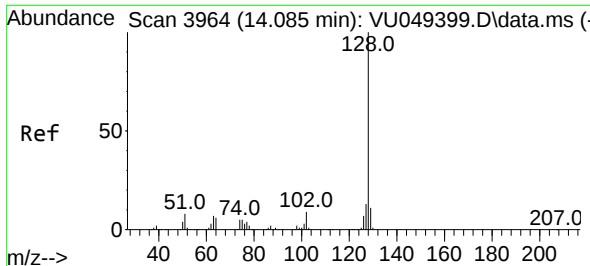

#95
Naphthalene
Concen: 2.338 ug/l
RT: 14.085 min Scan# 3964
Delta R.T. -0.000 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31

Instrument :
MSVOA_U
ClientSampleId :
30985

Tgt Ion:128 Resp: 11288
Ion Ratio Lower Upper
128 100
127 16.5 10.3 15.5#
129 7.1 8.6 13.0#

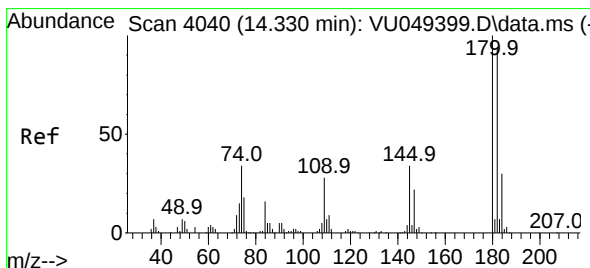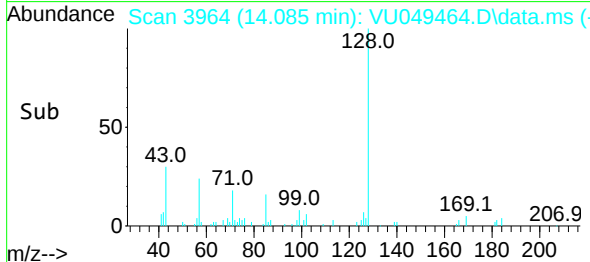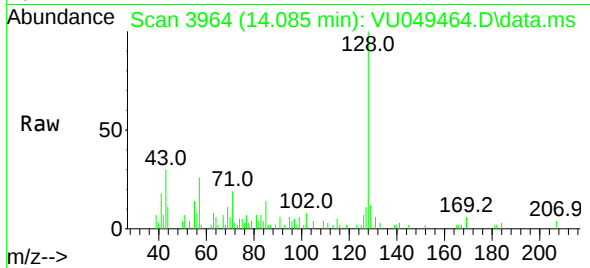

#96
1,2,3-Trichlorobenzene
Concen: 1.229 ug/l
RT: 14.346 min Scan# 4045
Delta R.T. 0.016 min
Lab File: VU049464.D
Acq: 28 Jun 2022 17:31

Tgt Ion:180 Resp: 285
Ion Ratio Lower Upper
180 100
182 48.1 48.4 145.0#
145 1171.2 14.8 44.4#

