

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
 Data File : VU049460.D
 Acq On : 28 Jun 2022 15:57
 Operator : SY/MD
 Sample : N3458-10DL 10X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 RE120D2-20220622DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
 Title : SW846 8260

Signal : TIC: VU049460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.578	375	385	396	rBV3	14986	26266	1.56%	0.253%
2	3.186	559	574	595	rVB	35956	82149	4.87%	0.792%
3	4.636	1007	1025	1051	rBV2	24197	73879	4.38%	0.712%
4	5.289	1213	1228	1241	rBV	254651	540582	32.07%	5.209%
5	5.372	1241	1254	1276	rVB	449811	923127	54.77%	8.895%
6	5.700	1342	1356	1380	rBV	273619	566478	33.61%	5.458%
7	6.250	1509	1527	1547	rBV	657881	1247033	73.99%	12.016%
8	6.542	1603	1618	1636	rBV	566006	1053480	62.51%	10.151%
9	7.896	2024	2039	2069	rBV	982533	1685426	100.00%	16.240%
10	9.417	2497	2512	2537	rBV	889951	1447515	85.88%	13.948%
11	10.632	2876	2890	2917	rBV	676940	1096079	65.03%	10.561%
12	11.812	3243	3257	3274	rBV	856284	1371241	81.36%	13.213%
13	16.262	4633	4641	4652	rBV3	21794	34771	2.06%	0.335%
14	16.407	4679	4686	4692	rBV4	17477	26856	1.59%	0.259%
15	16.446	4694	4698	4708	rVB6	15749	22047	1.31%	0.212%
16	17.114	4900	4906	4917	rBV	16116	24177	1.43%	0.233%
17	17.327	4957	4972	4980	rBV4	24279	48369	2.87%	0.466%
18	17.378	4980	4988	5004	rVB3	23733	45789	2.72%	0.441%
19	17.539	5032	5038	5049	rVB4	20397	28889	1.71%	0.278%
20	17.606	5052	5059	5068	rVV3	20310	34086	2.02%	0.328%




Sum of corrected areas: 10378239

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049460.D
Acq On : 28 Jun 2022 15:57
Operator : SY/MD
Sample : N3458-10DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE120D2-20220622DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

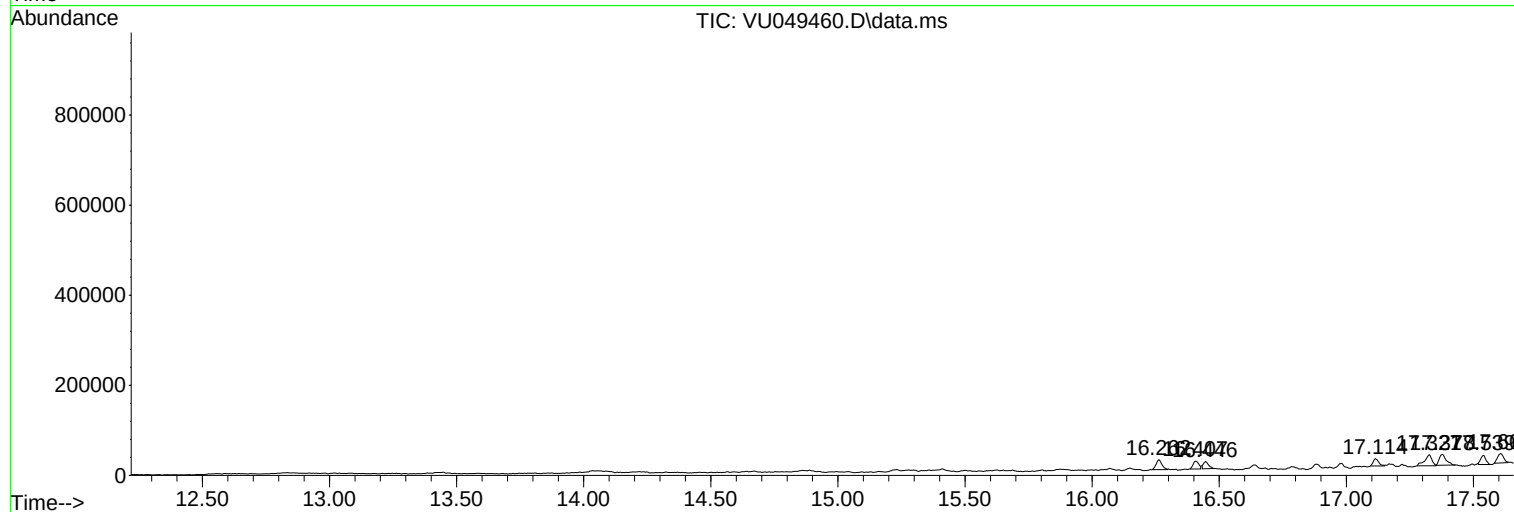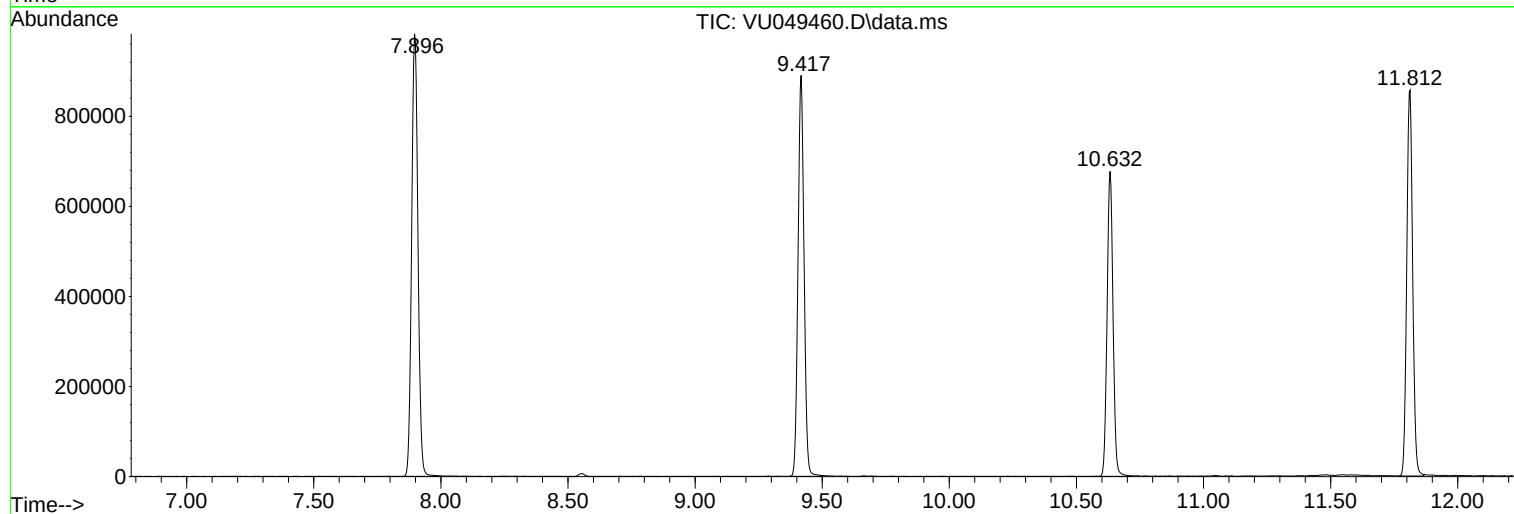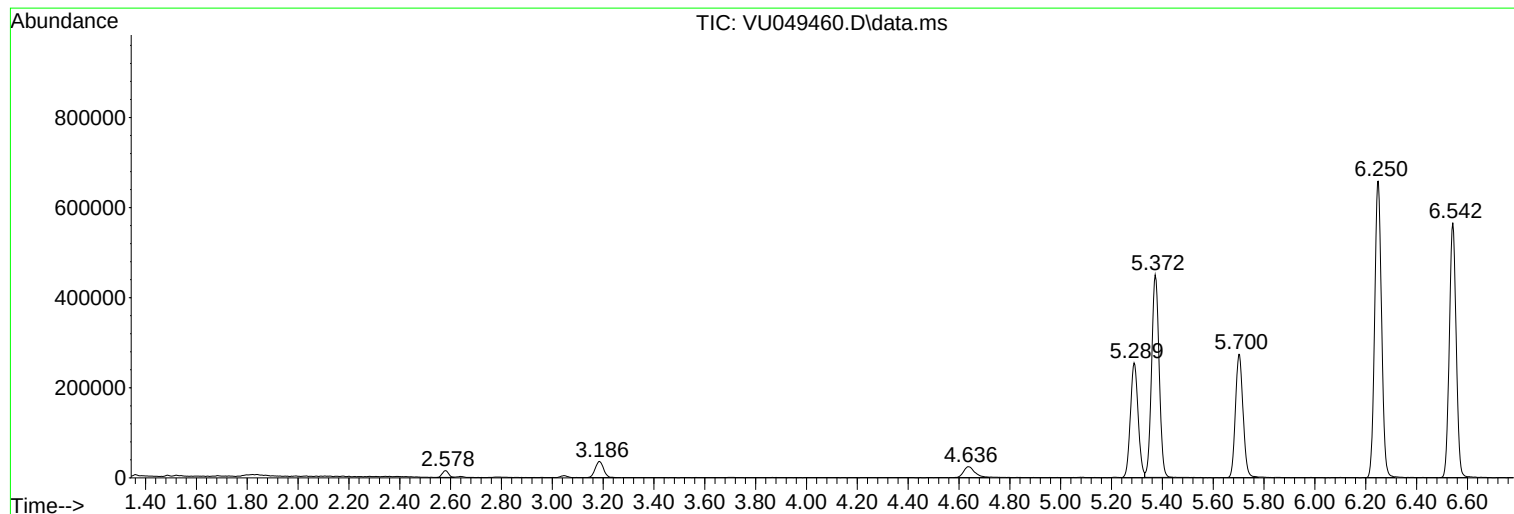

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049460.D
Acq On : 28 Jun 2022 15:57
Operator : SY/MD
Sample : N3458-10DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE120D2-20220622DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049460.D
Acq On : 28 Jun 2022 15:57
Operator : SY/MD
Sample : N3458-10DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE120D2-20220622DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------