

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
 Data File : VU049470.D
 Acq On : 28 Jun 2022 19:53
 Operator : SY/MD
 Sample : N3458-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 RE114D2-20220622

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
 Title : SW846 8260

Signal : TIC: VU049470.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	10	16	29	rVB2	13306	17583	1.07%	0.167%
2	2.578	370	385	399	rBV	96232	176538	10.77%	1.678%
3	4.668	1023	1035	1049	rBV2	8379	19333	1.18%	0.184%
4	5.289	1212	1228	1241	rBV	252122	532830	32.52%	5.065%
5	5.372	1241	1254	1276	rVB	437694	900096	54.94%	8.556%
6	5.703	1342	1357	1378	rBV	266129	551191	33.64%	5.239%
7	6.250	1508	1527	1546	rBV	640482	1220821	74.51%	11.605%
8	6.543	1603	1618	1644	rBV	713088	1325865	80.92%	12.603%
9	7.896	2024	2039	2057	rBV	940294	1638423	100.00%	15.574%
10	9.417	2497	2512	2536	rBV	858556	1413021	86.24%	13.432%
11	10.632	2877	2890	2913	rBV	665704	1066397	65.09%	10.137%
12	11.812	3243	3257	3274	rBV	831154	1328579	81.09%	12.629%
13	14.449	4066	4077	4084	rBV	20582	29343	1.79%	0.279%
14	15.211	4304	4314	4327	rBV8	14176	31212	1.91%	0.297%
15	15.401	4364	4373	4384	rBV4	40523	60533	3.69%	0.575%
16	15.976	4546	4552	4566	rVB3	18033	28812	1.76%	0.274%
17	16.291	4635	4650	4660	rBV3	50772	87772	5.36%	0.834%
18	16.407	4679	4686	4693	rBV5	10784	17025	1.04%	0.162%
19	17.131	4904	4911	4924	rVB	48722	74570	4.55%	0.709%




Sum of corrected areas: 10519944

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049470.D
Acq On : 28 Jun 2022 19:53
Operator : SY/MD
Sample : N3458-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE114D2-20220622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

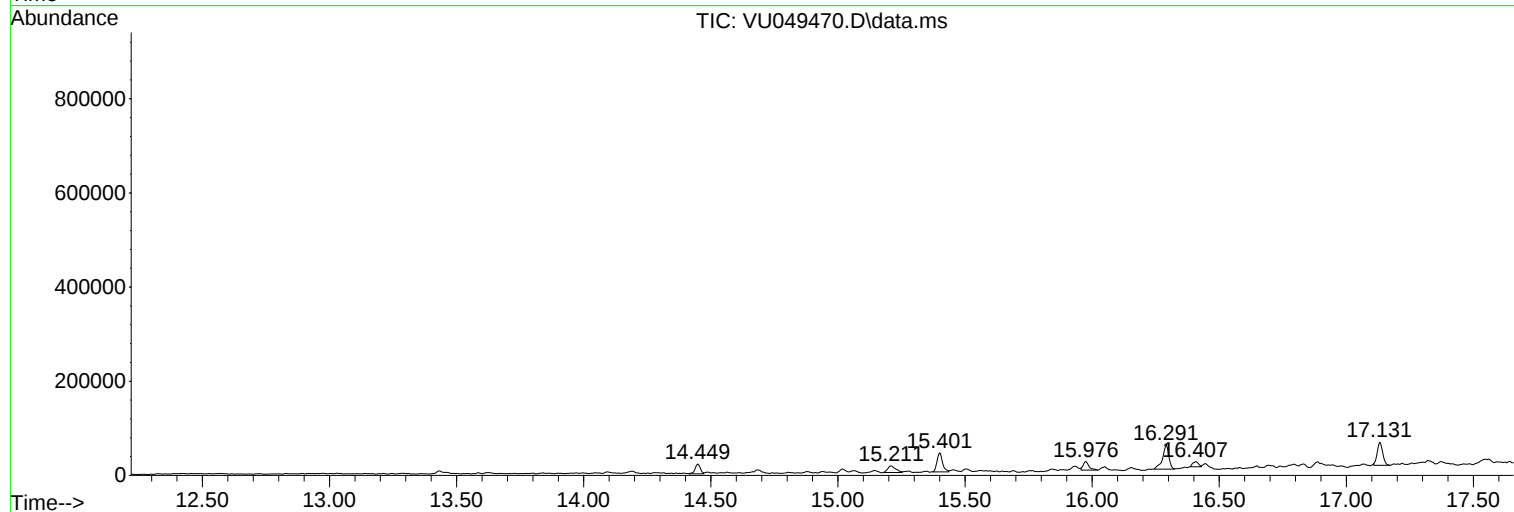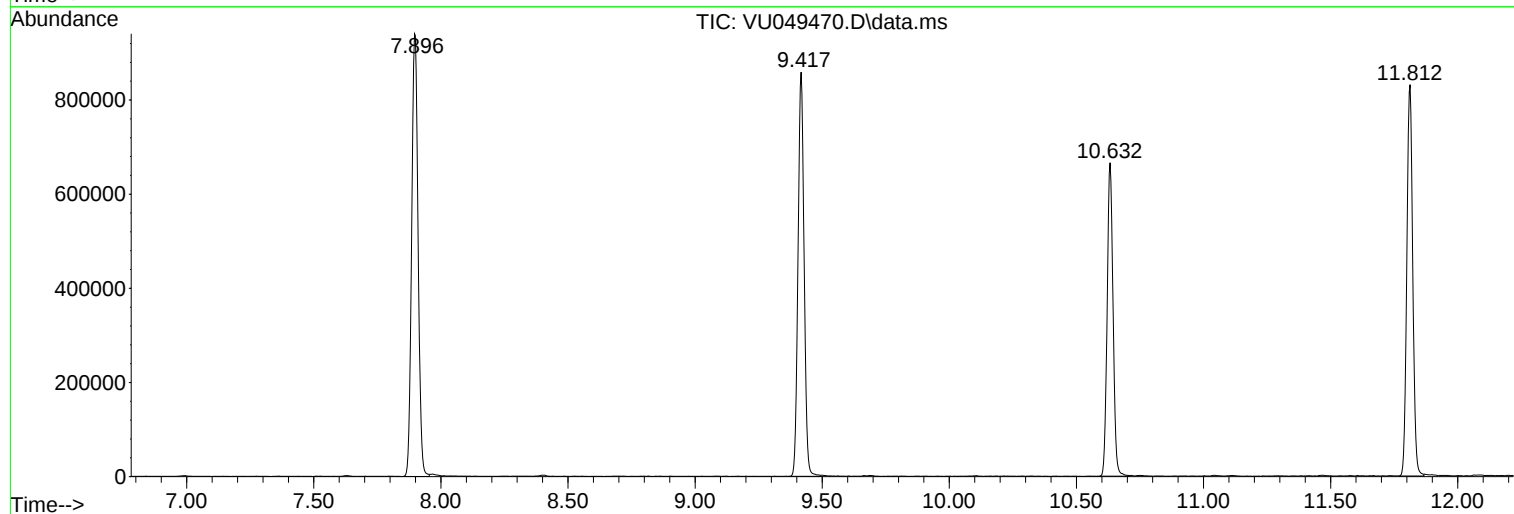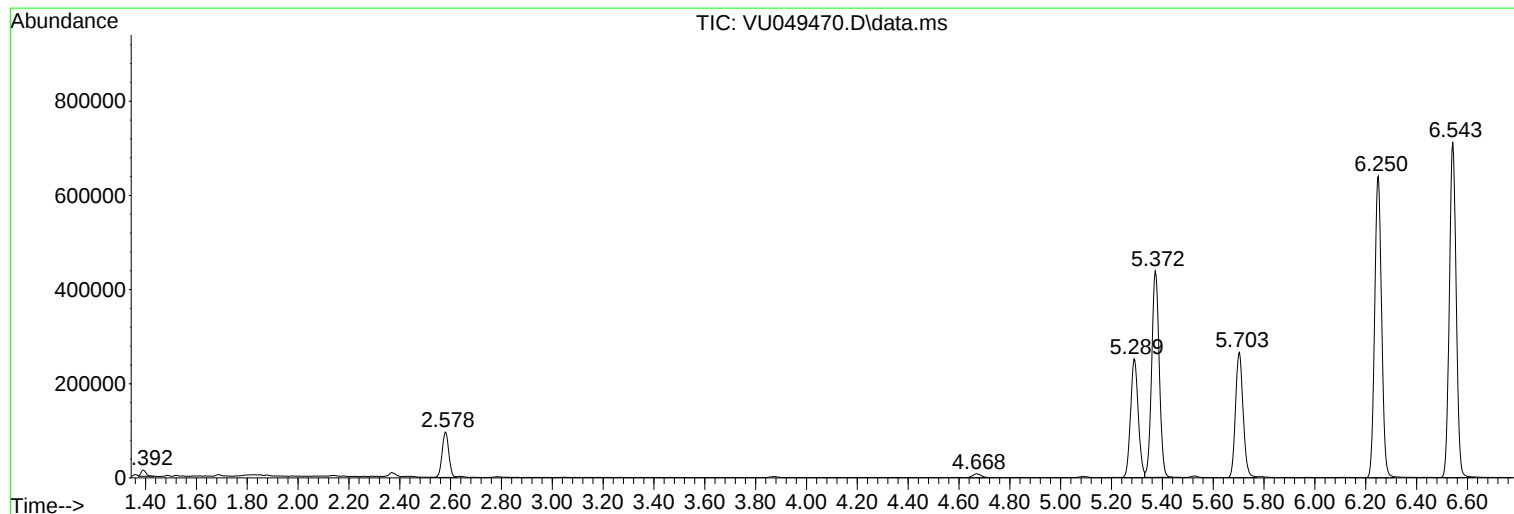

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049470.D
Acq On : 28 Jun 2022 19:53
Operator : SY/MD
Sample : N3458-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE114D2-20220622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049470.D
Acq On : 28 Jun 2022 19:53
Operator : SY/MD
Sample : N3458-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE114D2-20220622

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------