

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
 Data File : VU049487.D
 Acq On : 29 Jun 2022 02:58
 Operator : SY/MD
 Sample : N3457-18 20X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DUP03-20220621DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M

Title : SW846 8260

Signal : TIC: VU049487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.186	558	574	591	rBV	36418	82721	5.16%	0.930%
2	4.636	1005	1025	1054	rBV	33942	105926	6.60%	1.191%
3	5.289	1212	1228	1242	rBV2	245059	524395	32.68%	5.896%
4	5.372	1242	1254	1281	rVB	423713	883406	55.05%	9.932%
5	5.703	1339	1357	1394	rBV	262496	549462	34.24%	6.177%
6	6.250	1512	1527	1556	rBV	633731	1200490	74.82%	13.497%
7	6.543	1605	1618	1638	rBV2	152951	288124	17.96%	3.239%
8	7.896	2025	2039	2065	rBV	917175	1604601	100.00%	18.040%
9	9.417	2499	2512	2535	rBV	823259	1371945	85.50%	15.424%
10	10.632	2877	2890	2913	rBV	646165	1024293	63.83%	11.516%
11	11.812	3243	3257	3280	rBV	781346	1259390	78.49%	14.159%




Sum of corrected areas: 8894753

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049487.D
Acq On : 29 Jun 2022 02:58
Operator : SY/MD
Sample : N3457-18 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP03-20220621DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

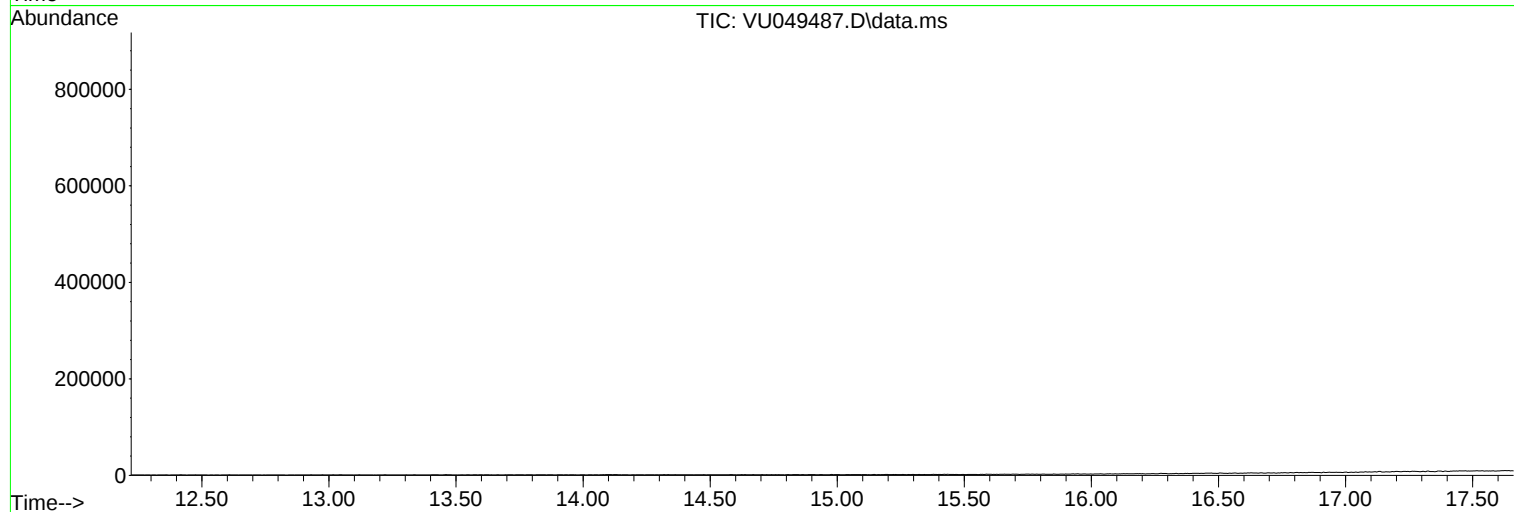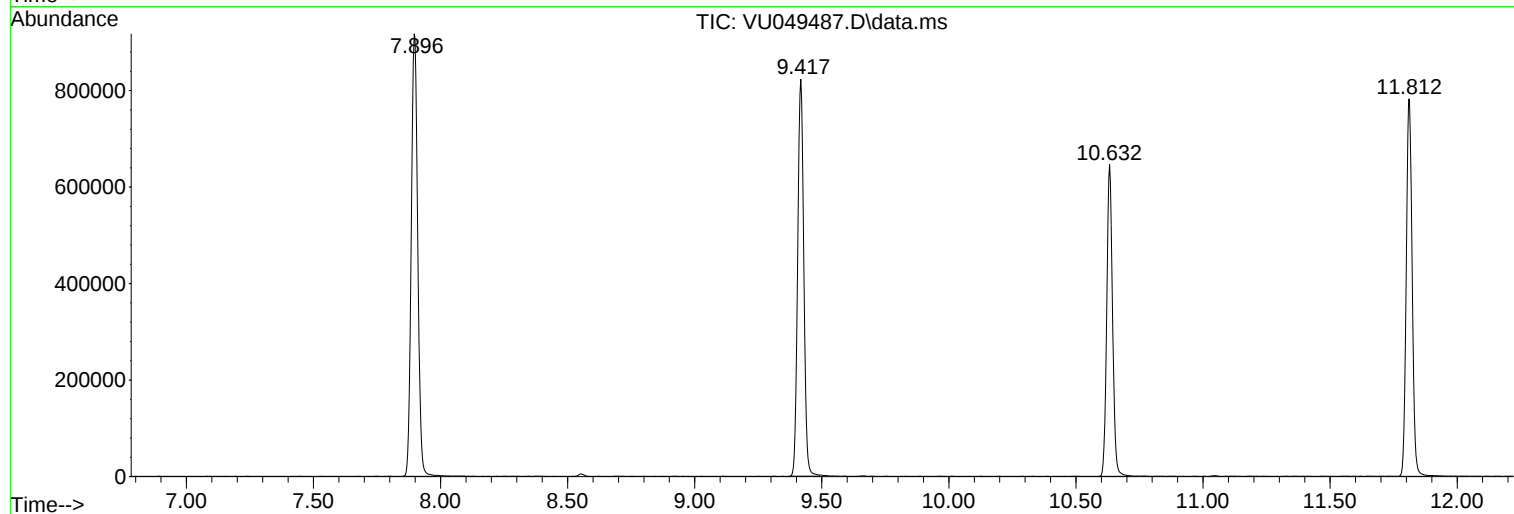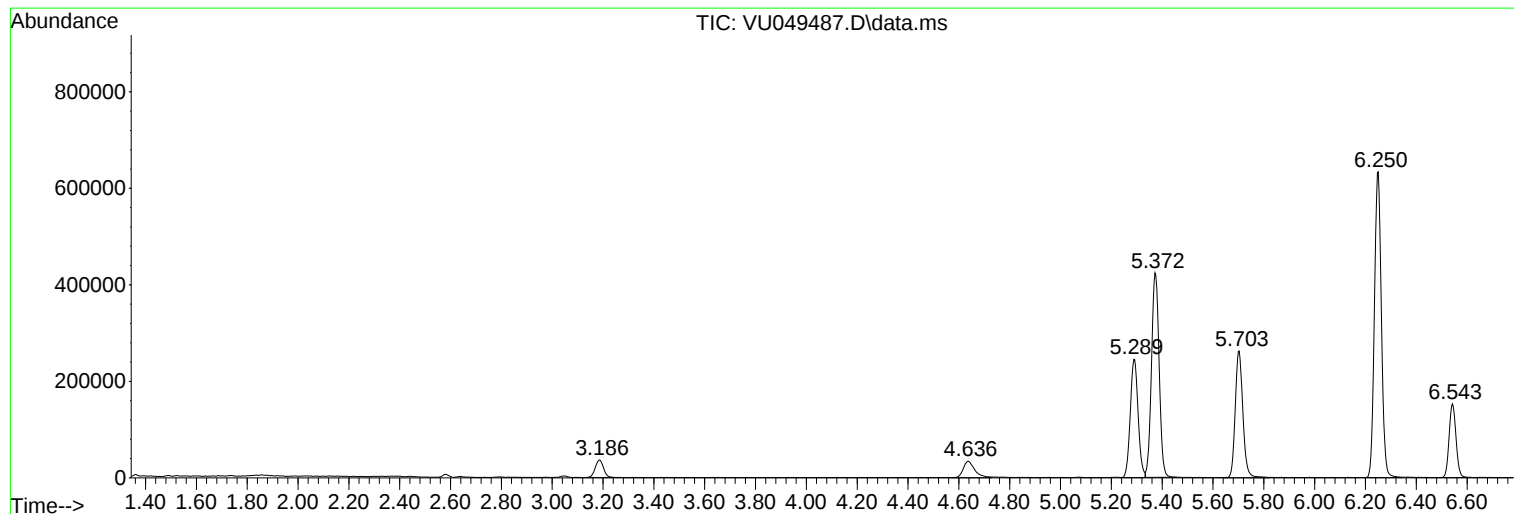

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049487.D
Acq On : 29 Jun 2022 02:58
Operator : SY/MD
Sample : N3457-18 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP03-20220621DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049487.D
Acq On : 29 Jun 2022 02:58
Operator : SY/MD
Sample : N3457-18 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP03-20220621DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------