

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049488.D
Acq On : 29 Jun 2022 03:22
Operator : SY/MD
Sample : N3457-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE134D4-20220616

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M

Title : SW846 8260

Signal : TIC: VU049488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.581	370	386	405	rBV	1700891	3174128	100.00%	25.154%
2	5.288	1213	1228	1241	rBV	250982	535324	16.87%	4.242%
3	5.372	1241	1254	1280	rVB	436459	905235	28.52%	7.174%
4	5.703	1341	1357	1378	rBV	272700	562975	17.74%	4.461%
5	6.247	1510	1526	1552	rBV	645172	1225767	38.62%	9.714%
6	6.542	1604	1618	1635	rBV	244774	454192	14.31%	3.599%
7	7.896	2024	2039	2067	rBV	964849	1651847	52.04%	13.090%
8	8.552	2231	2243	2259	rBV	180097	303961	9.58%	2.409%
9	9.417	2497	2512	2550	rBV	856501	1425838	44.92%	11.299%
10	10.632	2877	2890	2919	rBV	666343	1063405	33.50%	8.427%
11	11.812	3243	3257	3276	rBV	811744	1316095	41.46%	10.430%




Sum of corrected areas: 12618767

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049488.D
Acq On : 29 Jun 2022 03:22
Operator : SY/MD
Sample : N3457-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE134D4-20220616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

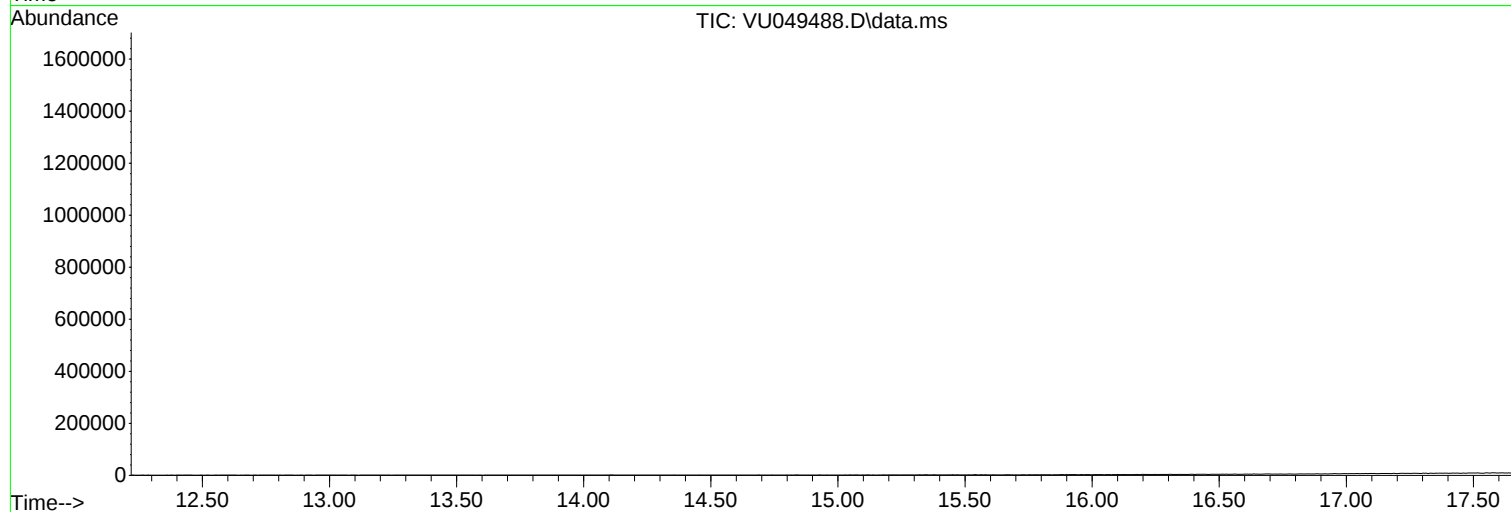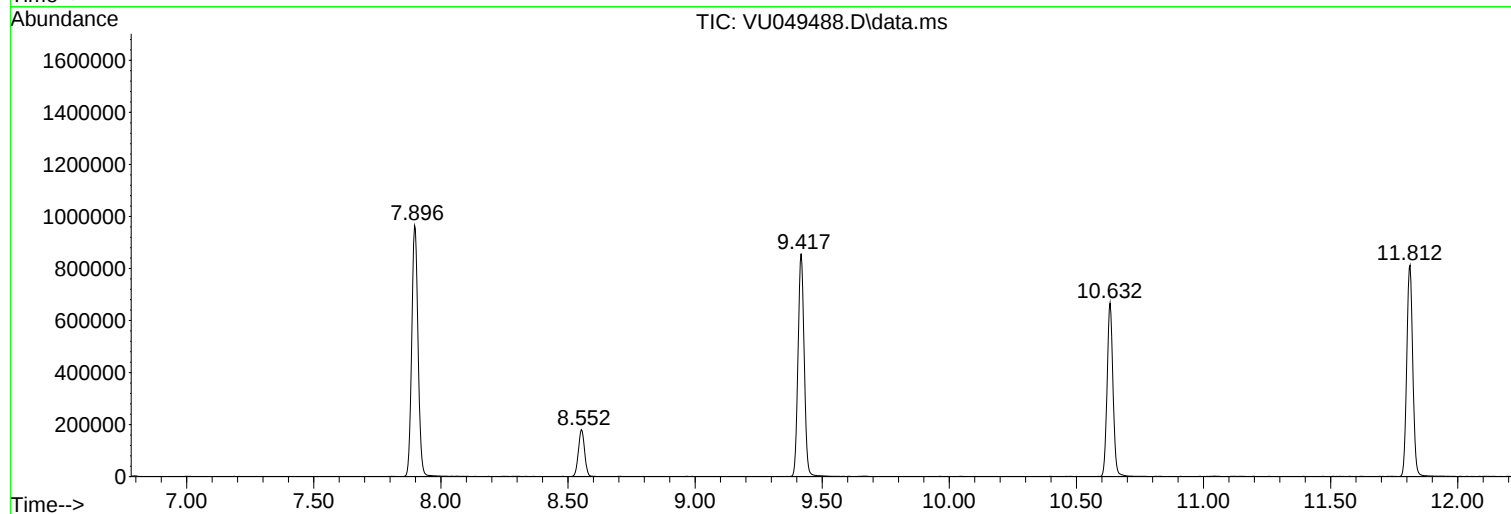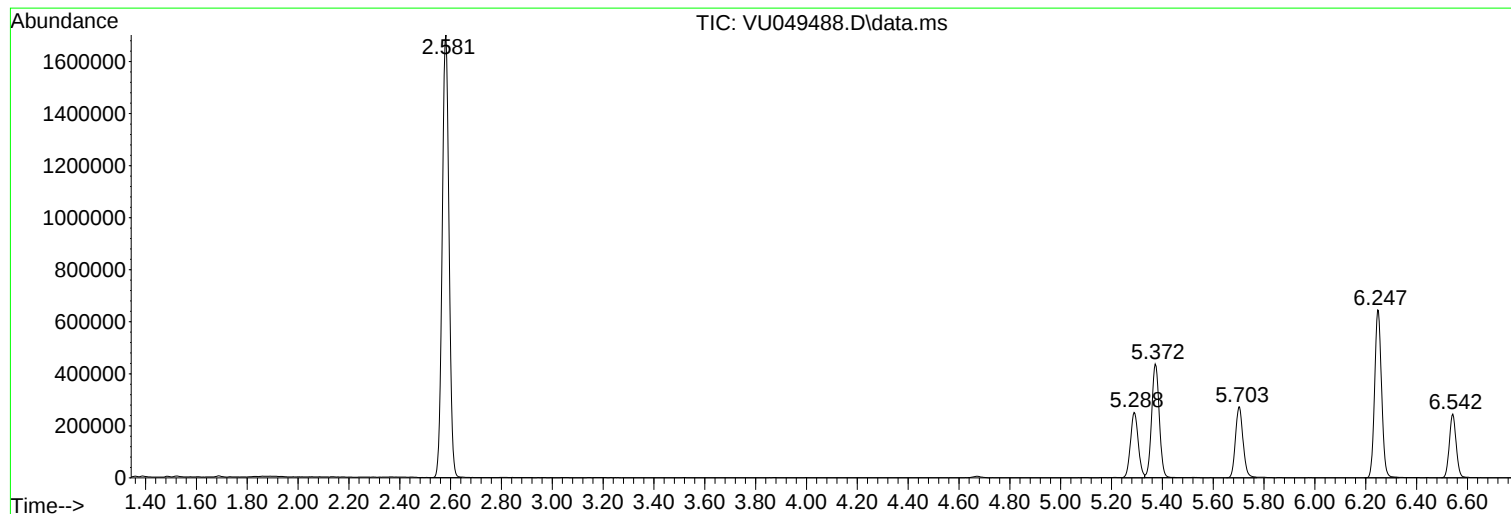

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049488.D
Acq On : 29 Jun 2022 03:22
Operator : SY/MD
Sample : N3457-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE134D4-20220616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049488.D
Acq On : 29 Jun 2022 03:22
Operator : SY/MD
Sample : N3457-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
RE134D4-20220616

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------