

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
 Data File : VU049490.D
 Acq On : 29 Jun 2022 04:09
 Operator : SY/MD
 Sample : N3457-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 MW179D2-20220617

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M

Title : SW846 8260

Signal : TIC: VU049490.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.668	1019	1035	1066	rBV2	233109	533475	10.18%	3.599%
2	5.289	1212	1228	1242	rBV	246432	535625	10.22%	3.614%
3	5.372	1242	1254	1278	rVB	428240	885260	16.90%	5.972%
4	5.700	1341	1356	1381	rBV	266308	552087	10.54%	3.725%
5	6.247	1509	1526	1553	rBV	635015	1202089	22.94%	8.110%
6	6.543	1600	1618	1656	rBV	2807866	5239651	100.00%	35.349%
7	7.896	2024	2039	2063	rBV	923390	1600142	30.54%	10.795%
8	8.552	2226	2243	2259	rBV	329795	559772	10.68%	3.776%
9	9.417	2498	2512	2547	rBV	832341	1393145	26.59%	9.399%
10	10.633	2877	2890	2912	rBV	644074	1035074	19.75%	6.983%
11	11.809	3244	3256	3278	rBV	796437	1286354	24.55%	8.678%




Sum of corrected areas: 14822674

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049490.D
Acq On : 29 Jun 2022 04:09
Operator : SY/MD
Sample : N3457-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW179D2-20220617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

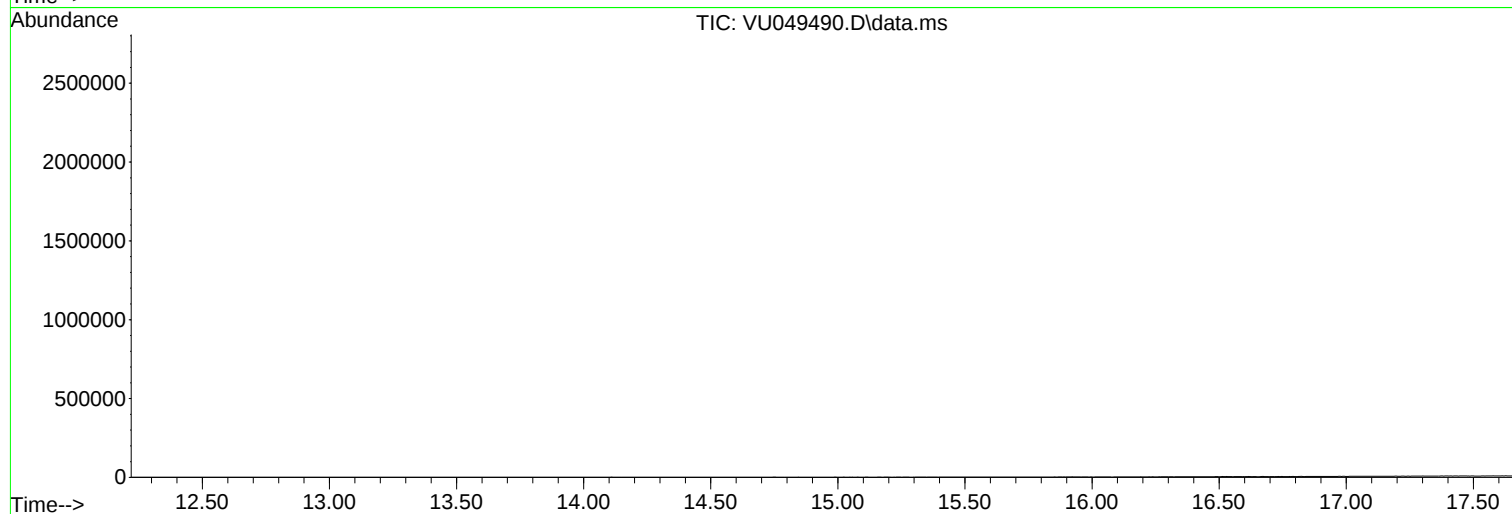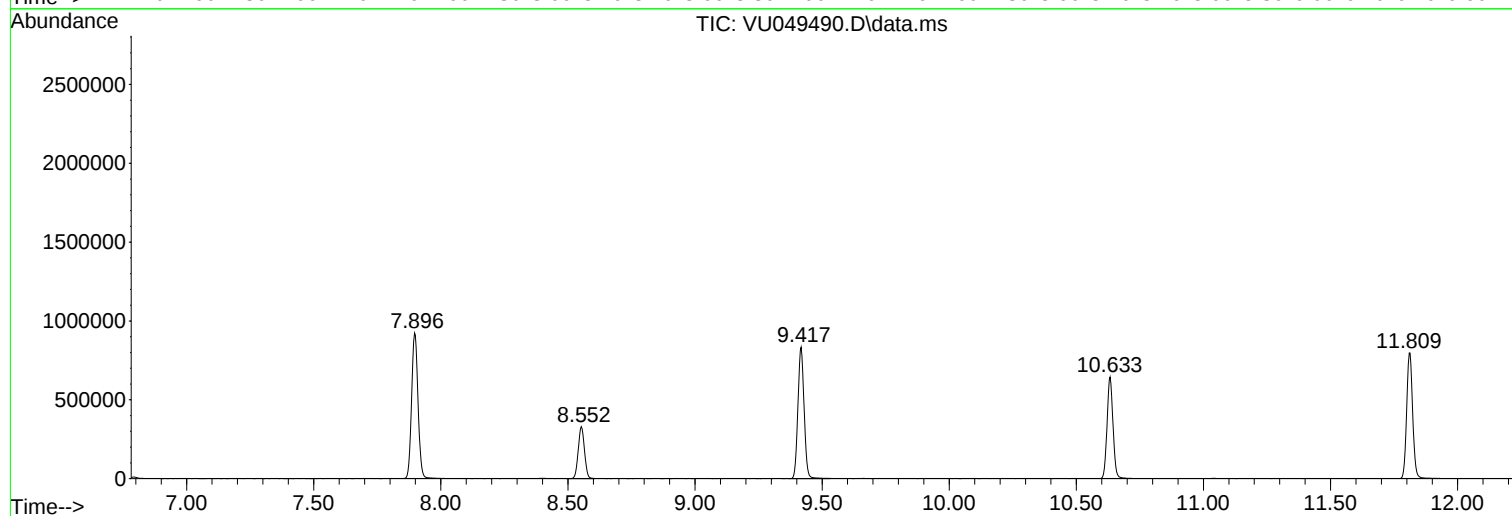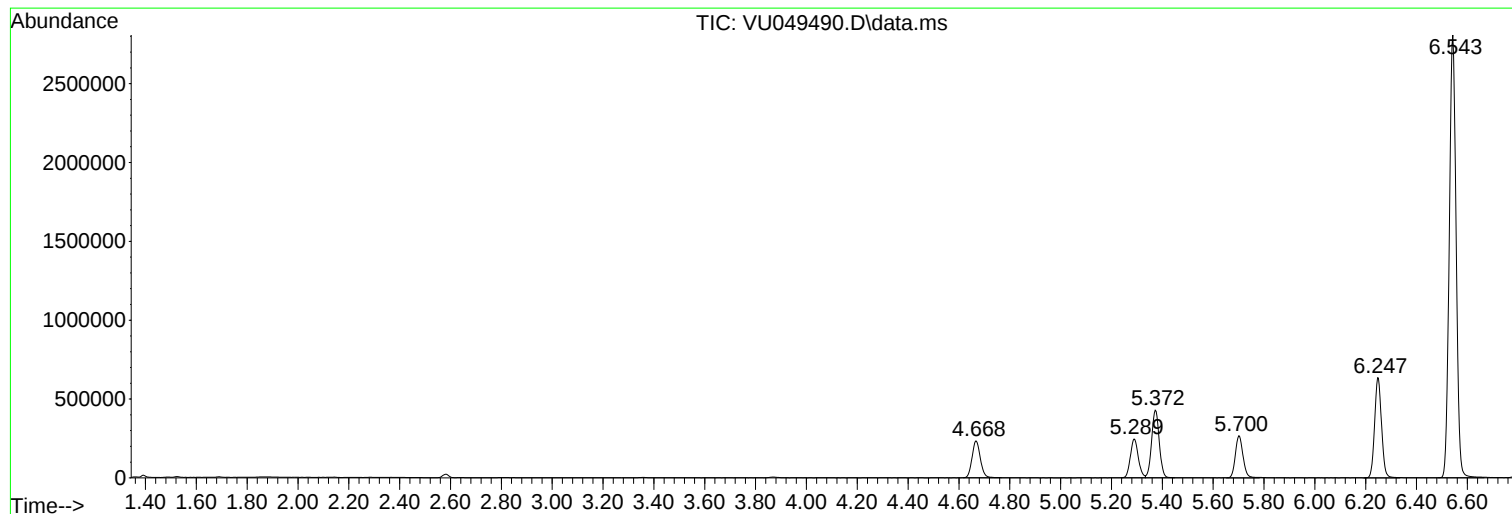

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049490.D
Acq On : 29 Jun 2022 04:09
Operator : SY/MD
Sample : N3457-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW179D2-20220617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
Data File : VU049490.D
Acq On : 29 Jun 2022 04:09
Operator : SY/MD
Sample : N3457-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
MW179D2-20220617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc