
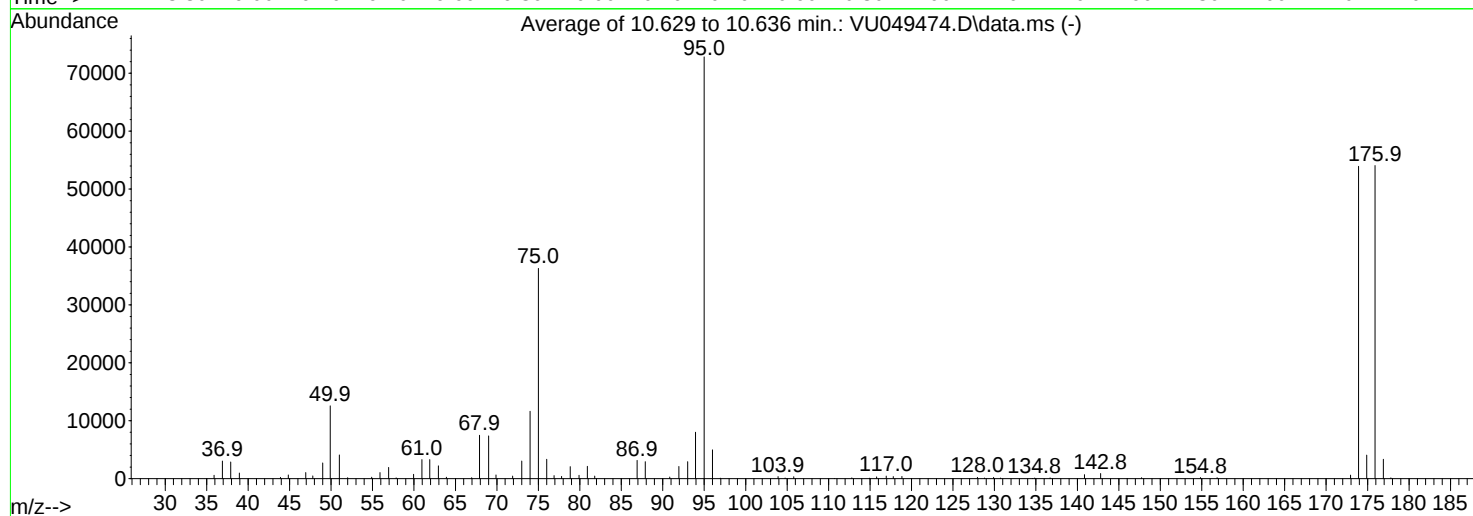


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062822\
 Data File : VU049474.D
 Acq On : 28 Jun 2022 21:27
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
 Title : SW846 8260
 Last Update : Tue Jun 28 10:35:43 2022

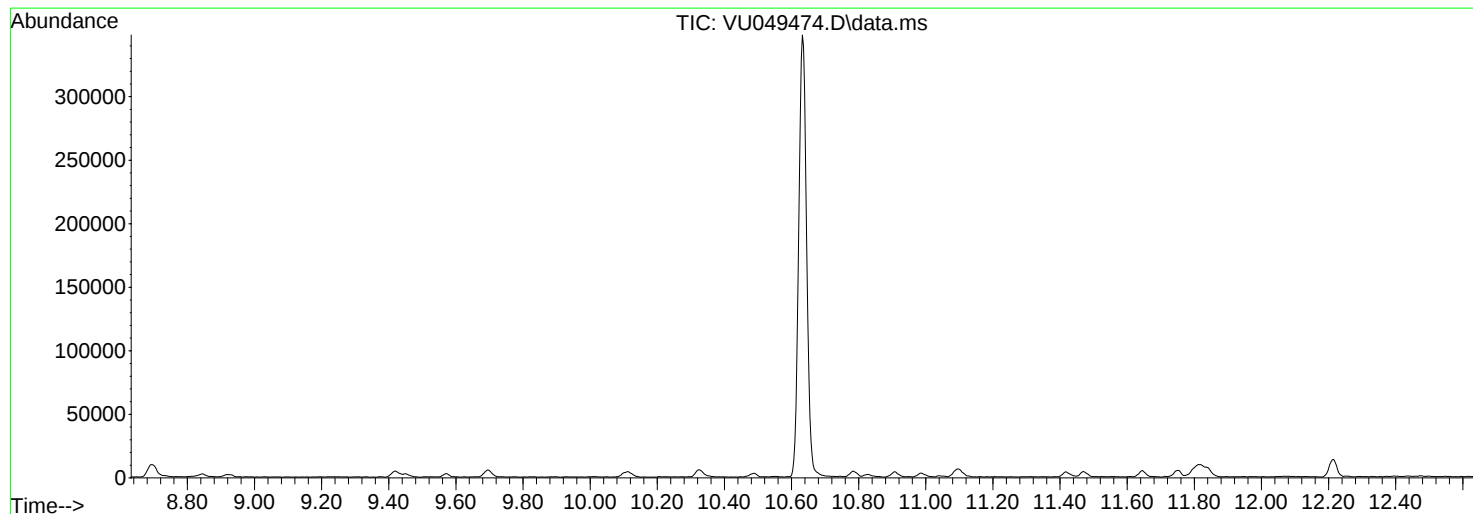

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	12563	PASS
75	95	30	60	49.9	36309	PASS
95	95	100	100	100.0	72835	PASS
96	95	5	9	6.8	4985	PASS
173	174	0.00	2	1.1	601	PASS
174	95	50	100	74.0	53931	PASS
175	174	5	9	7.6	4078	PASS
176	174	95	101	100.2	54061	PASS
177	176	5	9	6.2	3336	PASS