

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062823\
 Data File : VU054675.D
 Acq On : 28 Jun 2023 12:47
 Operator : MD/SY
 Sample : 03423-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 A46J0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU054675.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	115	rVB	140350	168786	15.80%	1.577%
2	1.731	132	137	144	rVB2	11741	13058	1.22%	0.122%
3	1.911	185	193	206	rBV	111431	150175	14.06%	1.403%
4	2.563	384	396	408	rBV	209220	339639	31.80%	3.172%
5	2.637	408	419	446	rVB2	102050	234999	22.00%	2.195%
6	3.042	532	545	565	rBV	99208	192361	18.01%	1.797%
7	3.181	569	588	613	rBV	261860	601438	56.31%	5.618%
8	4.628	1019	1038	1063	rBV3	246458	766578	71.77%	7.160%
9	4.817	1089	1097	1112	rVB	11073	25727	2.41%	0.240%
10	5.058	1157	1172	1197	rVB	191130	429380	40.20%	4.011%
11	5.721	1355	1378	1410	rBV3	378330	1005794	94.17%	9.395%
12	6.245	1525	1541	1563	rBV	402105	780804	73.10%	7.293%
13	6.689	1663	1679	1700	rBV2	241068	490013	45.88%	4.577%
14	7.563	1939	1951	1972	rBV	120704	219651	20.56%	2.052%
15	7.897	2041	2055	2071	rBV	429103	771539	72.24%	7.206%
16	7.968	2071	2077	2091	rVB2	15877	28215	2.64%	0.264%
17	8.177	2130	2142	2162	rBV	73892	134694	12.61%	1.258%
18	8.634	2272	2284	2314	rBV2	534811	1068082	100.00%	9.976%
19	8.788	2323	2332	2347	rBV3	30837	53597	5.02%	0.501%
20	9.415	2515	2527	2548	rVV	561251	942762	88.27%	8.806%
21	10.106	2729	2742	2746	rBV8	6747	11333	1.06%	0.106%
22	10.486	2853	2860	2870	rBV7	7688	12325	1.15%	0.115%
23	10.573	2875	2887	2895	rBV4	11831	23138	2.17%	0.216%
24	10.753	2928	2943	2961	rBV	181190	301578	28.24%	2.817%
25	11.473	3154	3167	3174	rBV8	6536	12930	1.21%	0.121%
26	11.611	3203	3210	3224	rVB5	9655	15107	1.41%	0.141%
27	11.688	3224	3234	3245	rBV9	9944	18087	1.69%	0.169%
28	11.743	3245	3251	3259	rVV7	10154	14790	1.38%	0.138%
29	11.811	3259	3272	3293	rVV	551147	900093	84.27%	8.407%
30	11.907	3293	3302	3314	rVB9	7802	14728	1.38%	0.138%
31	12.065	3339	3351	3371	rBV2	23563	63093	5.91%	0.589%
32	12.190	3378	3390	3412	rVB	398645	664282	62.19%	6.205%
33	12.528	3484	3495	3513	rBV2	33822	66288	6.21%	0.619%
34	12.884	3598	3606	3618	rVB3	39317	60380	5.65%	0.564%
35	13.685	3845	3855	3865	rBV3	4836	11855	1.11%	0.111%
36	13.846	3897	3905	3921	rBV3	9973	19687	1.84%	0.184%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062823\
Data File : VU054675.D
Acq On : 28 Jun 2023 12:47
Operator : MD/SY
Sample : 03423-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A46J0

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0

37	14.093	3971	3982	3993	rBV3	6972	11396	1.07%	0.106%
38	14.331	4049	4056	4067	rVB9	6841	10764	1.01%	0.101%
39	14.978	4247	4257	4270	rBV4	25606	42797	4.01%	0.400%
40	15.688	4471	4478	4488	rVB6	9089	14213	1.33%	0.133%


Sum of corrected areas: 10706156

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062823\
Data File : VU054675.D
Acq On : 28 Jun 2023 12:47
Operator : MD/SY
Sample : 03423-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A46J0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

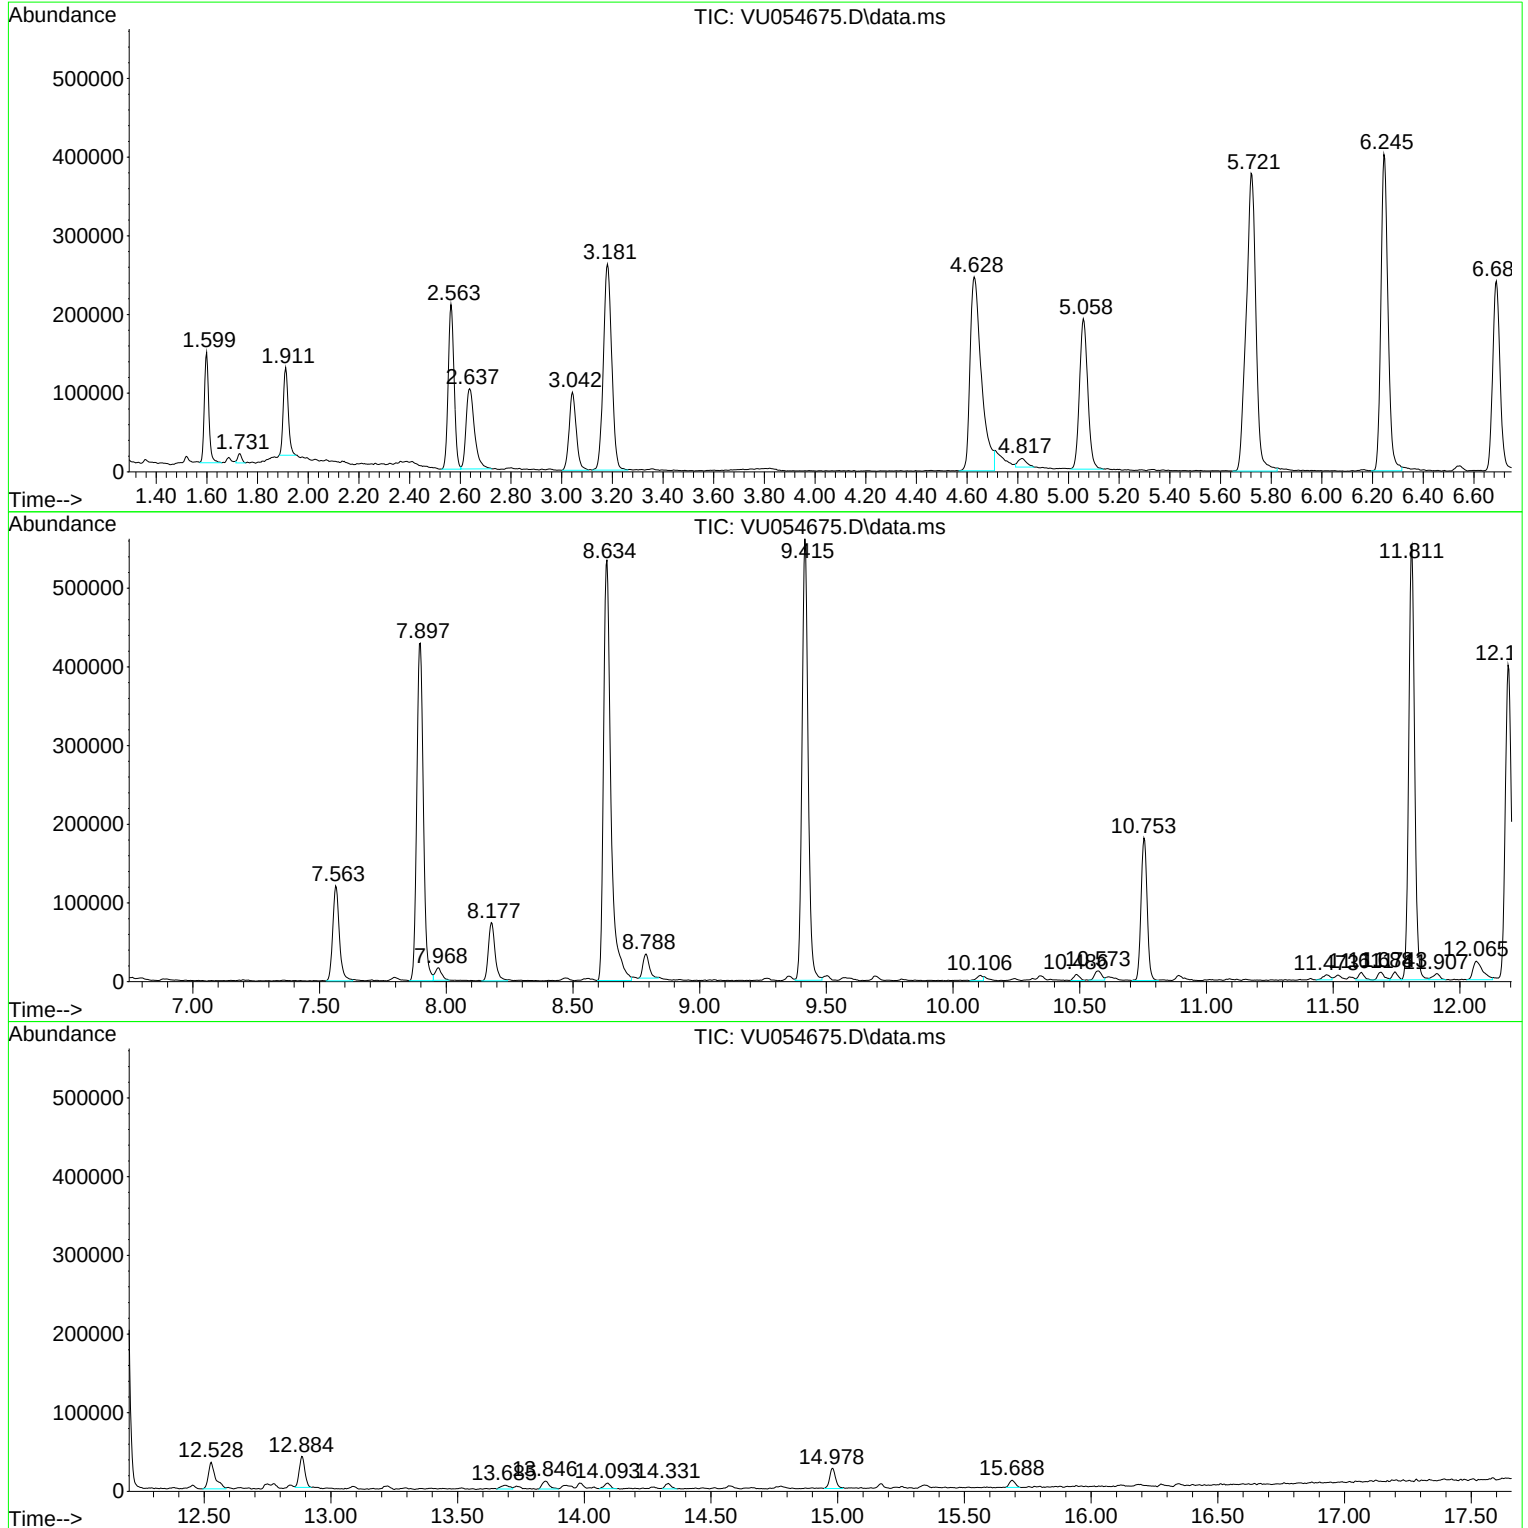

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062823\
Data File : VU054675.D
Acq On : 28 Jun 2023 12:47
Operator : MD/SY
Sample : 03423-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A46J0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062823\
Data File : VU054675.D
Acq On : 28 Jun 2023 12:47
Operator : MD/SY
Sample : 03423-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
A46J0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc