
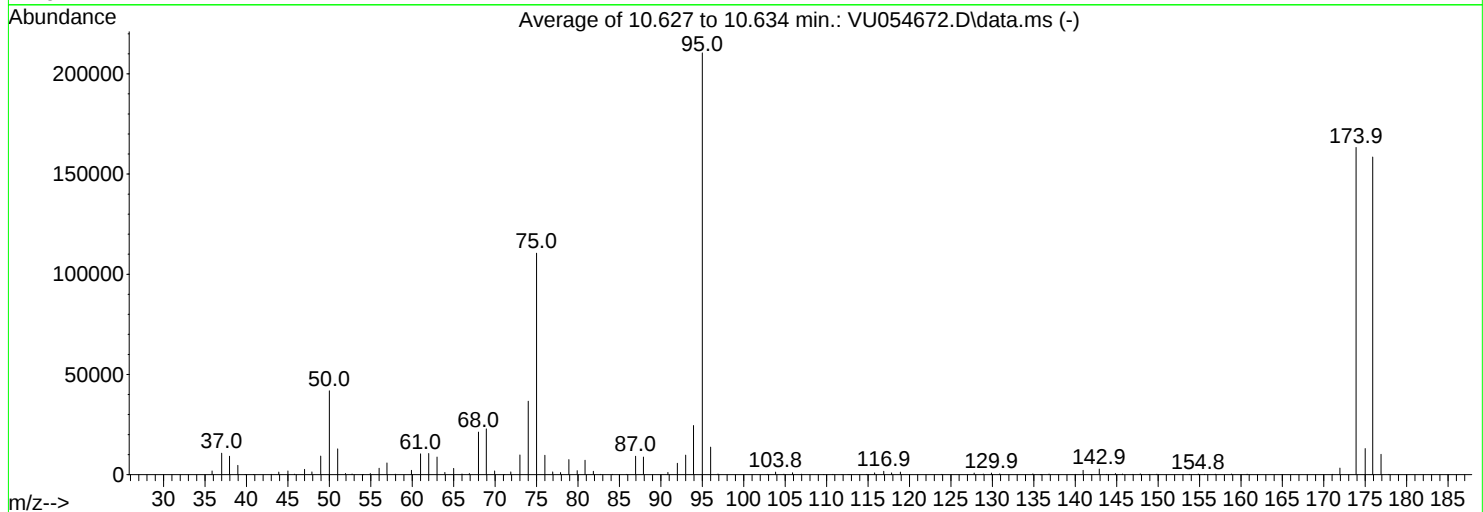


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062823\
Data File : VU054672.D
Acq On : 28 Jun 2023 09:02
Operator : MD/SY
Sample : BFB026
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB026

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jun 23 23:55:46 2023

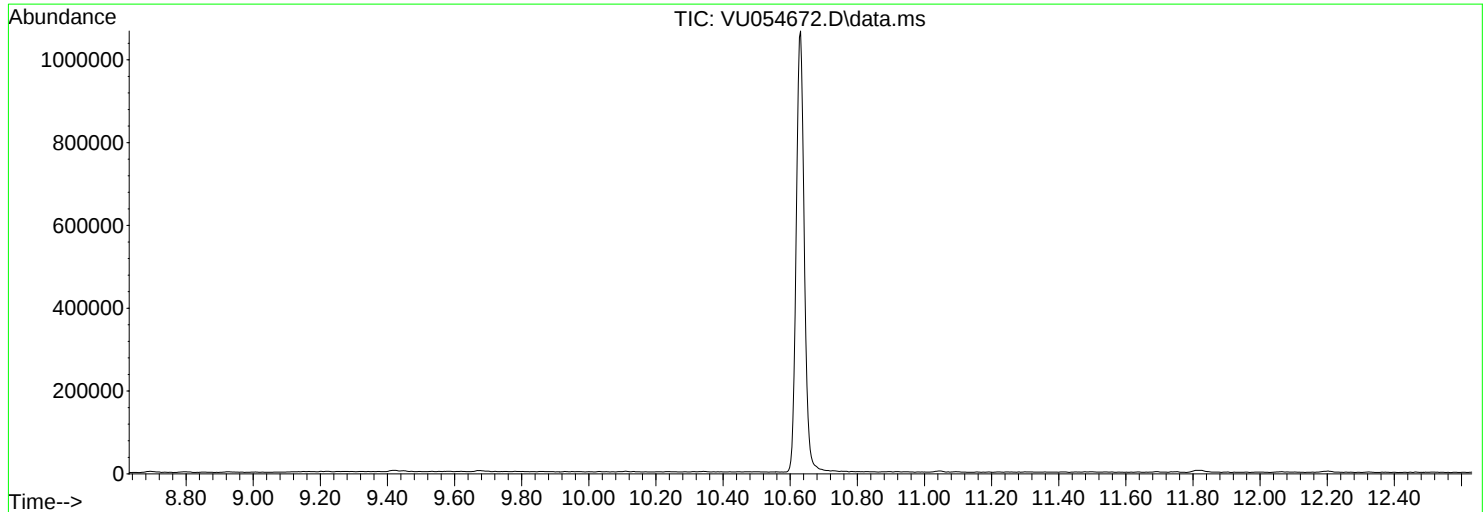

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	41869	PASS
75	95	30	80	52.5	110509	PASS
95	95	100	100	100.0	210496	PASS
96	95	5	9	6.5	13737	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.6	163264	PASS
175	174	5	9	8.0	13053	PASS
176	174	95	101	97.1	158507	PASS
177	176	5	9	6.4	10156	PASS

m/z	Abundance
35.90	2441.0
37.80	891.0
38.80	118.0
39.80	323.0
40.90	120.0
43.90	693.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.90	4349.0
37.00	10756.0
38.00	10541.0
39.00	4942.0
39.90	440.0
40.90	203.0
43.00	225.0
43.90	2155.0
45.00	1810.0
45.90	284.0
47.00	2979.0
47.90	1372.0
48.90	9742.0
50.00	43336.0
51.00	13442.0
51.90	599.0
52.80	270.0
54.00	129.0
55.00	584.0
56.00	3379.0
56.90	5746.0
57.90	322.0
59.90	2258.0
61.00	10815.0
62.00	11029.0
63.00	9377.0
63.90	1354.0
65.00	3217.0
66.00	266.0
66.90	676.0
68.00	21560.0
69.00	23520.0
69.90	1888.0
71.90	1205.0
73.00	9880.0
74.00	38104.0
75.00	113688.0
76.00	9594.0
77.00	1363.0
77.90	1118.0
78.90	7609.0
79.90	1952.0
80.90	7432.0
81.90	1701.0
82.70	151.0
84.10	118.0
85.90	440.0
87.00	9517.0
87.90	8903.0
90.80	1091.0
92.00	5571.0
93.00	9970.0
94.00	25240.0
95.00	213760.0
96.00	14312.0
96.90	385.0
102.80	152.0
103.90	1348.0
104.90	266.0
105.90	1051.0
107.00	251.0
109.70	117.0
110.80	172.0
111.90	146.0
112.60	193.0
114.90	137.0
115.80	792.0
116.90	1719.0
117.90	872.0
118.90	1285.0
123.90	140.0
127.80	874.0
128.90	334.0
129.90	859.0
130.90	446.0
134.90	380.0
135.80	108.0
136.80	347.0
140.10	229.0
140.90	2360.0
142.90	2635.0
143.70	135.0
144.90	641.0
145.70	354.0
146.90	118.0
147.90	429.0
148.80	159.0
149.90	240.0
153.80	164.0
154.80	311.0
155.60	170.0
156.90	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

158.90	295.0
160.70	217.0
172.00	3181.0
173.90	162880.0
175.00	13088.0
175.90	157312.0
176.90	10037.0
177.90	208.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.90	4307.0
37.00	11030.0
38.00	10348.0
39.00	4860.0
39.90	417.0
40.80	263.0
43.00	213.0
43.90	1989.0
45.00	1885.0
45.80	255.0
47.00	2721.0
47.90	1443.0
49.00	9640.0
50.00	43216.0
51.00	13261.0
52.00	574.0
52.70	306.0
54.90	572.0
56.00	3255.0
56.90	6048.0
58.00	264.0
59.90	2197.0
61.00	10639.0
62.00	10839.0
63.00	9006.0
64.00	1172.0
65.00	3230.0
66.00	308.0
66.90	599.0
68.00	21784.0
68.90	23600.0
70.00	1896.0
71.90	1414.0
73.00	10123.0
74.00	37696.0
75.00	113664.0
76.00	9980.0
76.90	1353.0
77.90	1144.0
78.90	7691.0
79.90	2040.0
80.90	7375.0
81.90	1712.0
82.70	146.0
84.10	142.0
86.90	9438.0
87.90	9232.0
90.80	1131.0
92.00	5903.0
93.00	9938.0
93.90	25264.0
95.00	216768.0
96.00	14077.0
96.90	379.0
102.80	181.0
103.80	1344.0
104.80	254.0
105.90	985.0
107.00	266.0
109.70	111.0
110.80	160.0
111.90	116.0
112.80	180.0
114.90	139.0
115.80	926.0
116.90	1678.0
117.80	927.0
118.90	1344.0
123.90	126.0
127.80	855.0
128.90	382.0
129.90	885.0
130.90	403.0
134.90	425.0
136.90	359.0
140.10	189.0
141.00	2239.0
142.90	2853.0
143.80	166.0
144.80	596.0
145.70	318.0
146.90	156.0
147.90	370.0
148.90	147.0
149.90	233.0
153.00	138.0
153.80	232.0
154.80	347.0
155.60	195.0
156.90	263.0
158.90	311.0
160.70	225.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

171.00	276.0
171.90	3320.0
173.90	167680.0
175.00	13493.0
175.90	164352.0
176.90	10398.0
177.80	194.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

m/z	Abundance
35.90	4089.0
37.00	10304.0
38.00	9437.0
39.00	4444.0
40.00	407.0
40.80	240.0
43.00	172.0
44.00	1814.0
45.00	1821.0
45.70	205.0
47.00	2271.0
47.90	1354.0
49.00	8524.0
50.00	39056.0
51.00	11938.0
52.00	608.0
52.70	310.0
54.90	510.0
56.00	2880.0
57.00	5773.0
58.00	175.0
59.90	2108.0
61.00	9692.0
62.00	9859.0
63.00	8062.0
64.00	964.0
65.00	2832.0
66.00	327.0
66.90	525.0
68.00	20296.0
68.90	21432.0
69.90	1641.0
71.00	101.0
71.90	1340.0
73.00	9504.0
74.00	34072.0
75.00	104176.0
76.00	9476.0
77.00	1246.0
77.90	968.0
78.90	7165.0
79.90	2016.0
80.80	6711.0
81.80	1620.0
82.80	135.0
84.20	125.0
86.90	8688.0
87.90	8245.0
90.90	1054.0
92.00	5654.0
93.00	9400.0
94.00	23152.0
95.00	200960.0
96.00	12822.0
96.90	307.0
102.90	173.0
103.80	1173.0
104.80	231.0
105.90	847.0
106.90	248.0
109.60	118.0
110.70	176.0
111.80	104.0
112.80	180.0
114.80	125.0
115.80	893.0
116.90	1544.0
117.80	953.0
118.90	1226.0
123.90	131.0
127.80	778.0
128.90	365.0
129.90	792.0
131.00	275.0
134.90	429.0
136.90	288.0
139.90	141.0
140.90	1994.0
141.90	331.0
142.90	2889.0
143.90	189.0
144.80	542.0
145.70	237.0
147.00	113.0
147.70	337.0
149.00	148.0
149.80	199.0
153.00	175.0
153.80	194.0
154.90	366.0
155.60	164.0
156.90	297.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026

158.80	308.0
160.80	195.0
171.10	314.0
172.00	3278.0
173.90	159232.0
175.00	12578.0
175.90	153856.0
176.90	10034.0
177.80	180.0

Instrument :
MSVOA_U
ClientSampleId :
BFB026