




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062824\
Data File : VU059606.D
Acq On : 28 Jun 2024 09:01
Operator : MD/SY
Sample : P3007-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JMRG5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:13:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 02:08:17 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

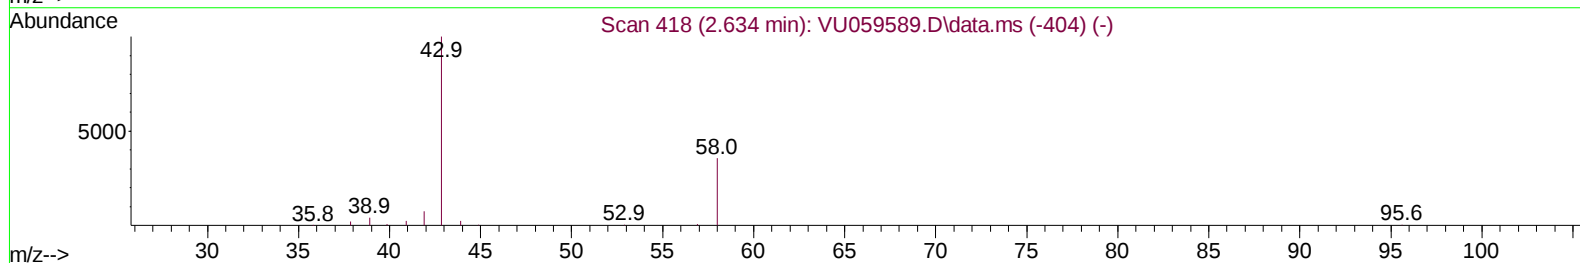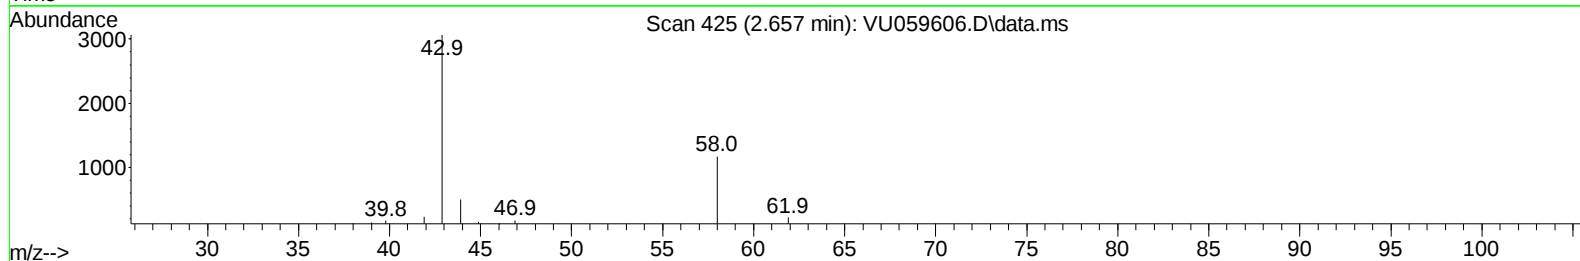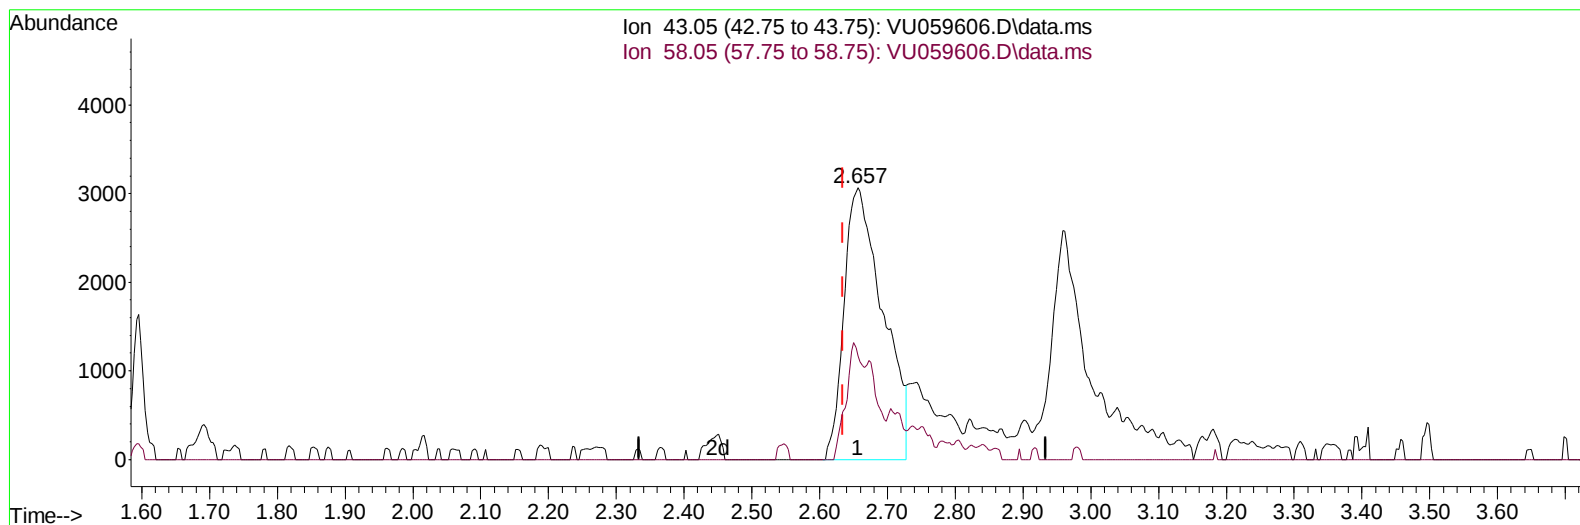

TIC: VU059606.D\data.ms

(13) Acetone (T)

2.657min (+ 0.022) 9.08 ug/L

response 12179

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	18.61
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062824\
Data File : VU059606.D
Acq On : 28 Jun 2024 09:01
Operator : MD/SY
Sample : P3007-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JMRG5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:13:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 02:08:17 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

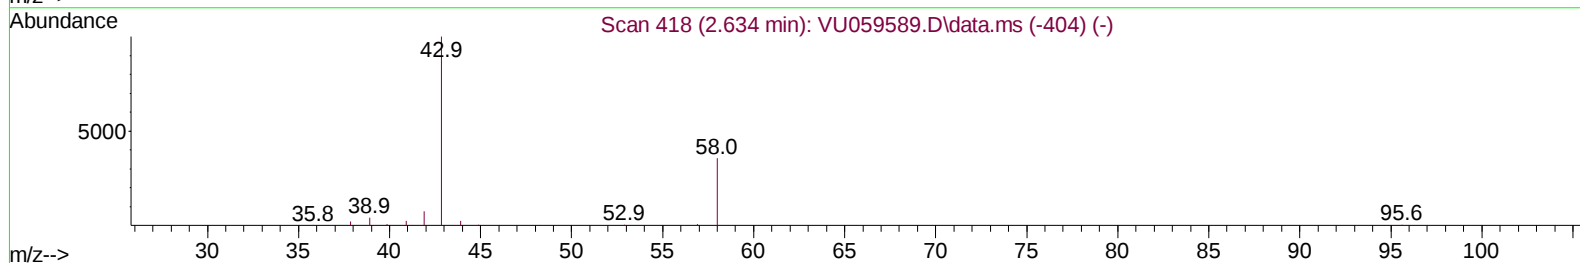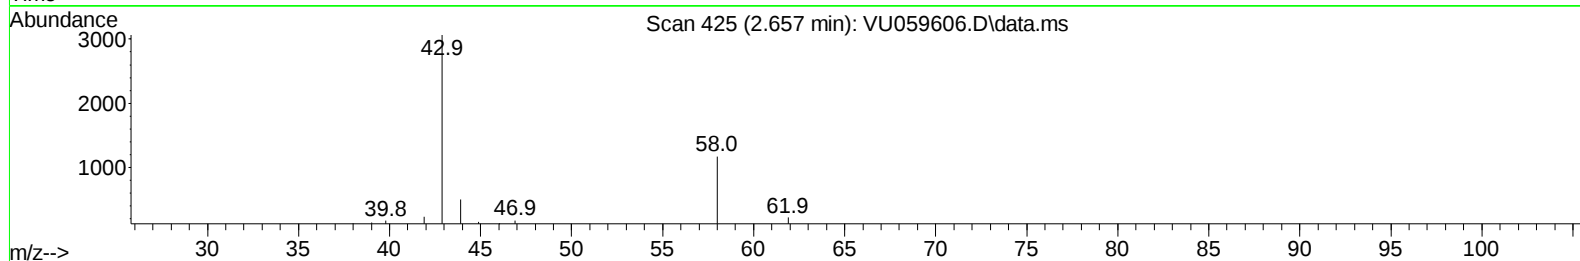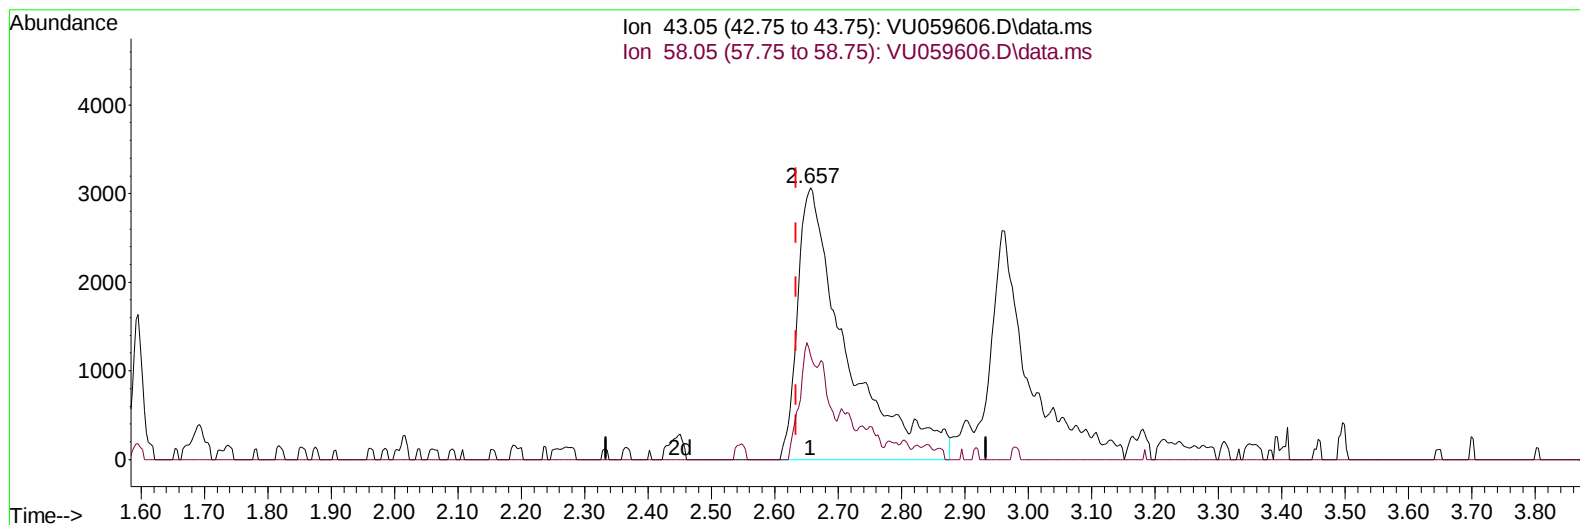

TIC: VU059606.D\data.ms

(13) Acetone (T)

2.657min (+ 0.022) 12.30 ug/L m

response 16485

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	13.75
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062824\
Data File : VU059606.D
Acq On : 28 Jun 2024 09:01
Operator : MD/SY
Sample : P3007-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JMRG5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:13:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 02:08:17 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

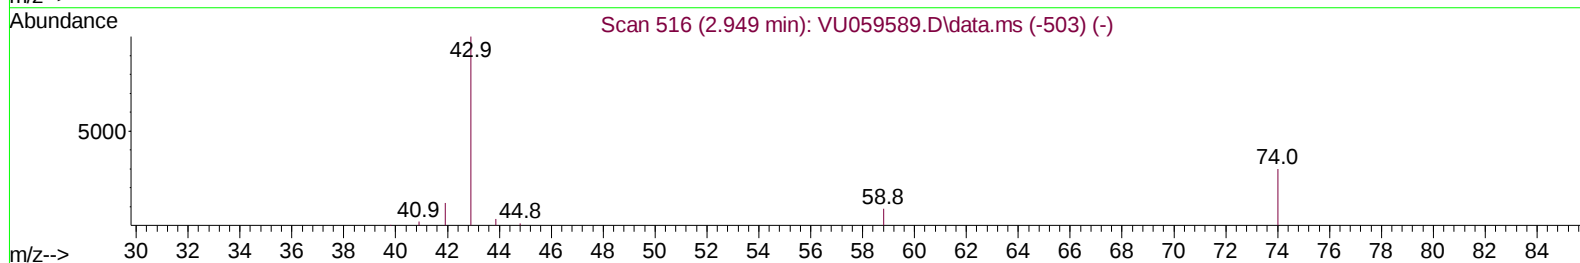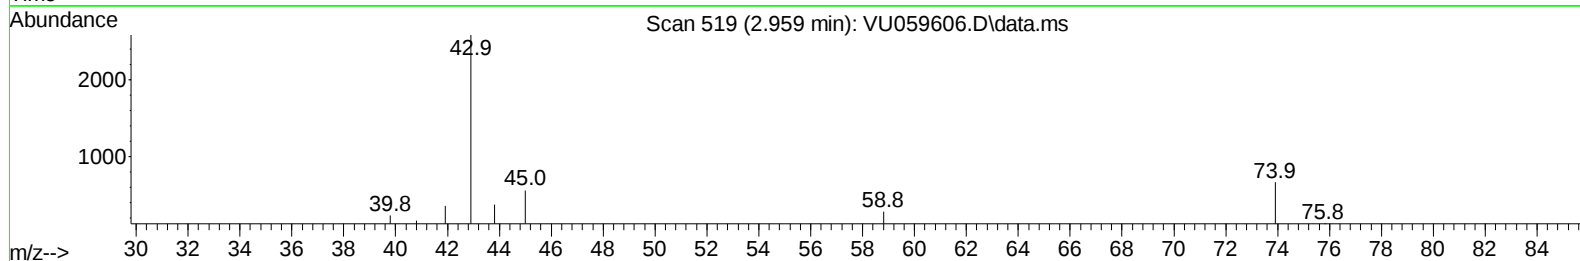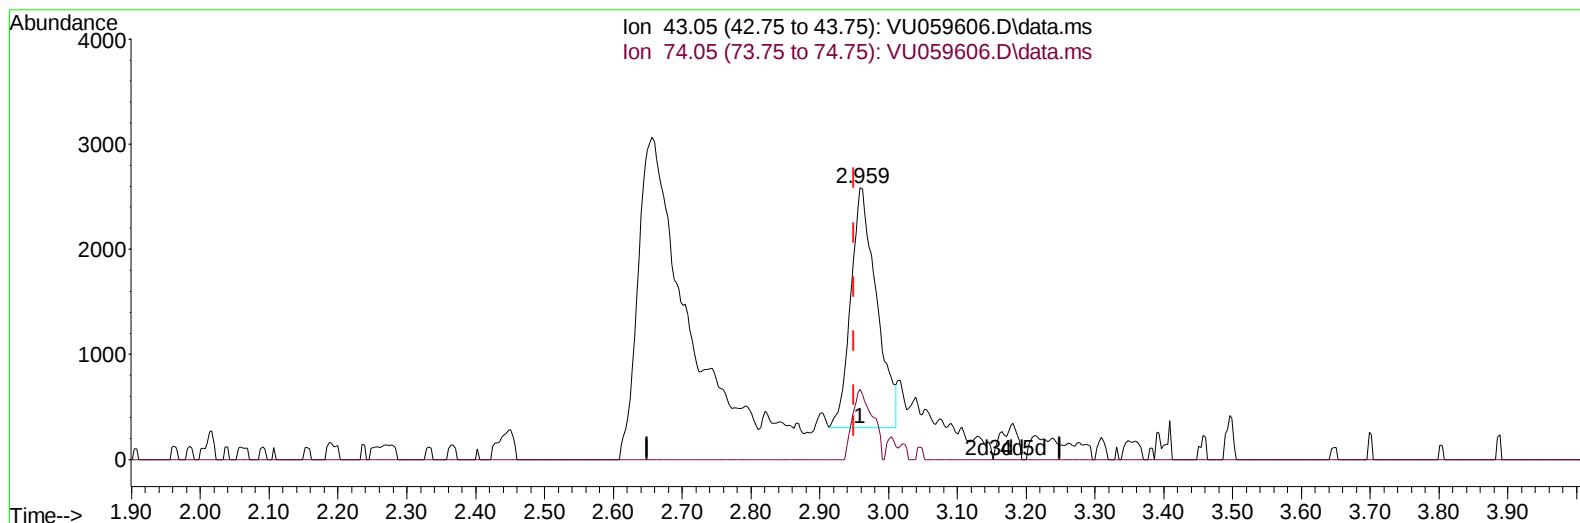

TIC: VU059606.D\data.ms

(15) Methyl Acetate (T)

2.959min (+ 0.010) 1.68 ug/L

response 5945

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	24.00	22.66
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062824\
Data File : VU059606.D
Acq On : 28 Jun 2024 09:01
Operator : MD/SY
Sample : P3007-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JMRG5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:13:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 02:08:17 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

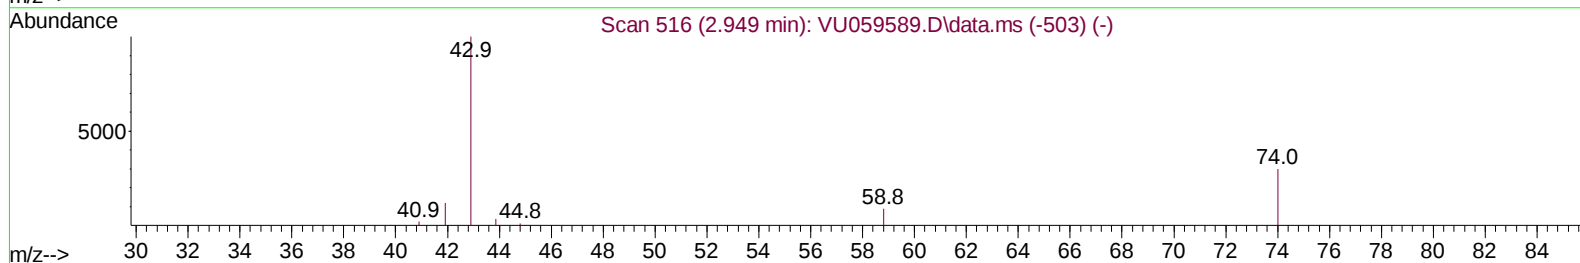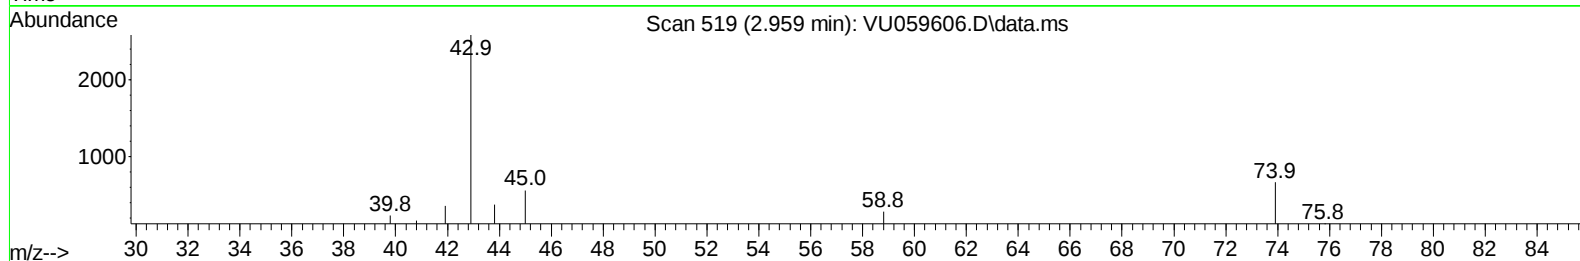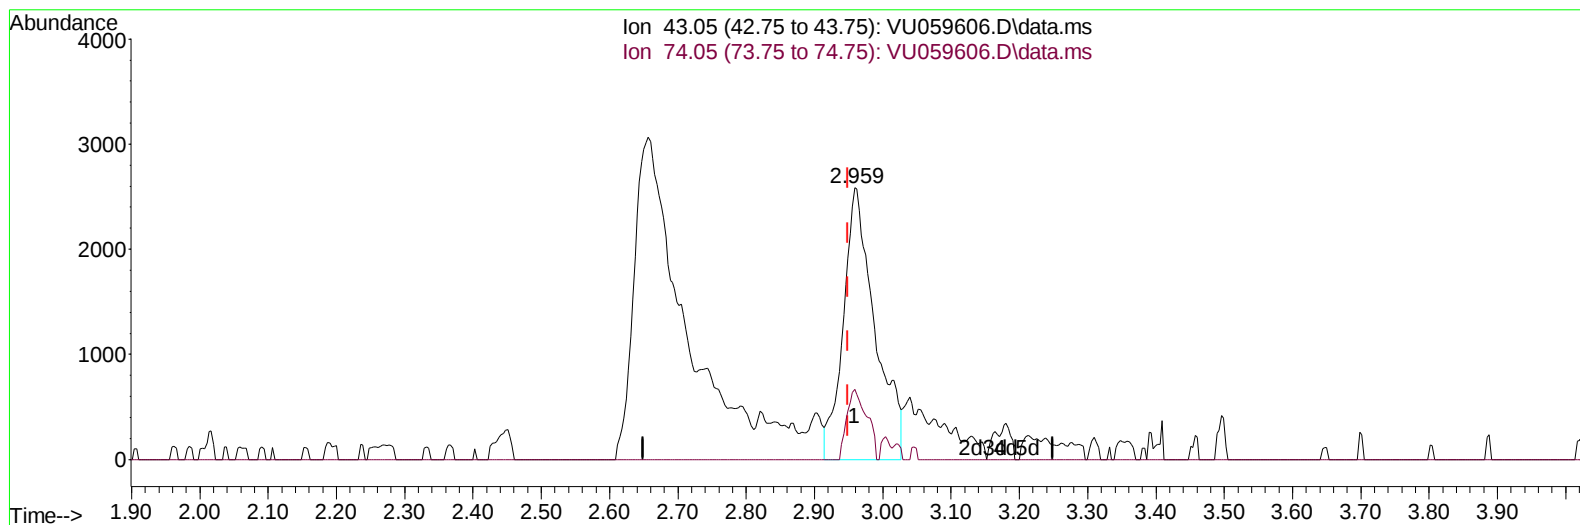

TIC: VU059606.D\data.ms

(15) Methyl Acetate (T)

2.959min (+ 0.010) 2.35 ug/L m

response 8306

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	24.00	16.22#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062824\
 Data File : VU059606.D
 Acq On : 28 Jun 2024 09:01
 Operator : MD/SY
 Sample : P3007-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JMRG5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:13:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 28 02:08:17 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		144304	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		152230	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		69171	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.592	65		41016	4.088	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	81.800%		
7) Chloroethane-d5	1.907	69		42199	4.371	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	87.400%		
11) 1,1-Dichloroethene-d2	2.557	65		18902	4.541	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	90.800%		
20) 2-Butanone-d5	4.637	46		89355	43.231	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130		Recovery =	86.460%		
24) Chloroform-d	5.052	84		97990	4.758	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	95.200%		
26) 1,2-Dichloroethane-d4	5.695	65		45863	4.623	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	92.400%		
32) Benzene-d6	5.721	84		191902	4.580	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	91.600%		
36) 1,2-Dichloropropane-d6	6.682	67		60619	4.722	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	94.400%		
41) Toluene-d8	7.891	98		162754	4.179	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	83.600%		
43) trans-1,3-Dichloroprop...	8.177	79		16661	4.145	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	82.800%		
46) 2-Hexanone-d5	8.627	63		85049	50.918	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	101.840%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84		52853	4.983	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	99.600%		
66) 1,2-Dichlorobenzene-d4	12.187	152		66442	5.397	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	108.000%		
Target Compounds							
							Qvalue
13) Acetone	2.657	43		16485m	12.295	ug/L	
15) Methyl Acetate	2.959	43		8306m	2.348	ug/L	
16) Methylene chloride	3.036	84		2835	0.234	ug/L	88
34) Trichloroethene	6.534	95		35934	2.870	ug/L	95
42) Toluene	7.965	91		34138	0.698	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062824\
Data File : VU059606.D
Acq On : 28 Jun 2024 09:01
Operator : MD/SY
Sample : P3007-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JMRG5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:13:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 02:08:17 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

