




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062824\  
 Data File : VU059611.D  
 Acq On : 28 Jun 2024 10:57  
 Operator : MD/SY  
 Sample : P3007-21MS  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 JMRJOMS

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:14:24 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR061724WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Jun 28 02:08:17 2024  
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024  
 Supervised By :Semsettin Yesilyurt 07/01/2024

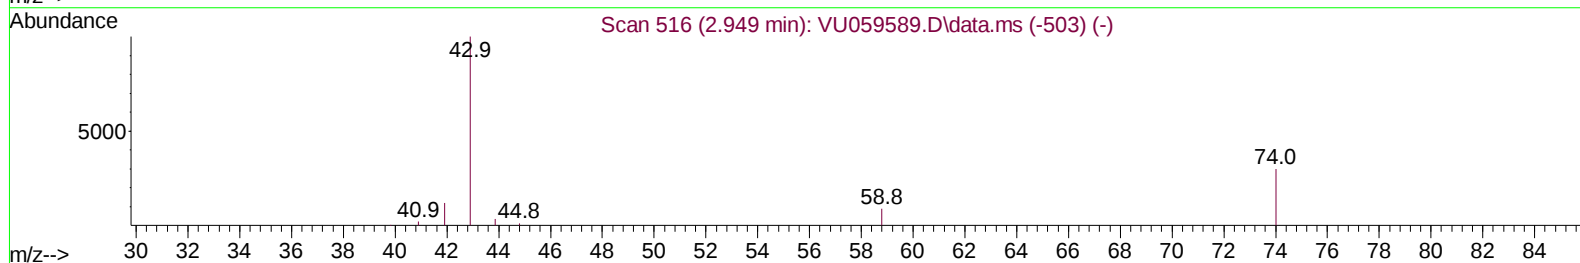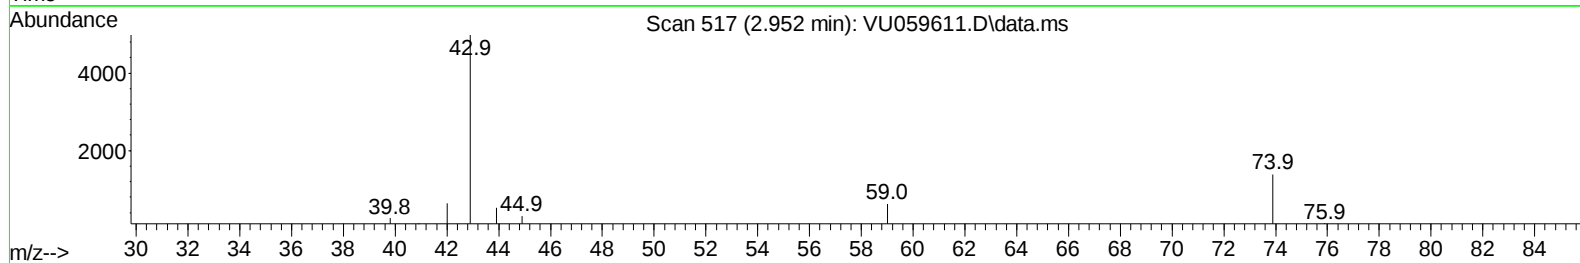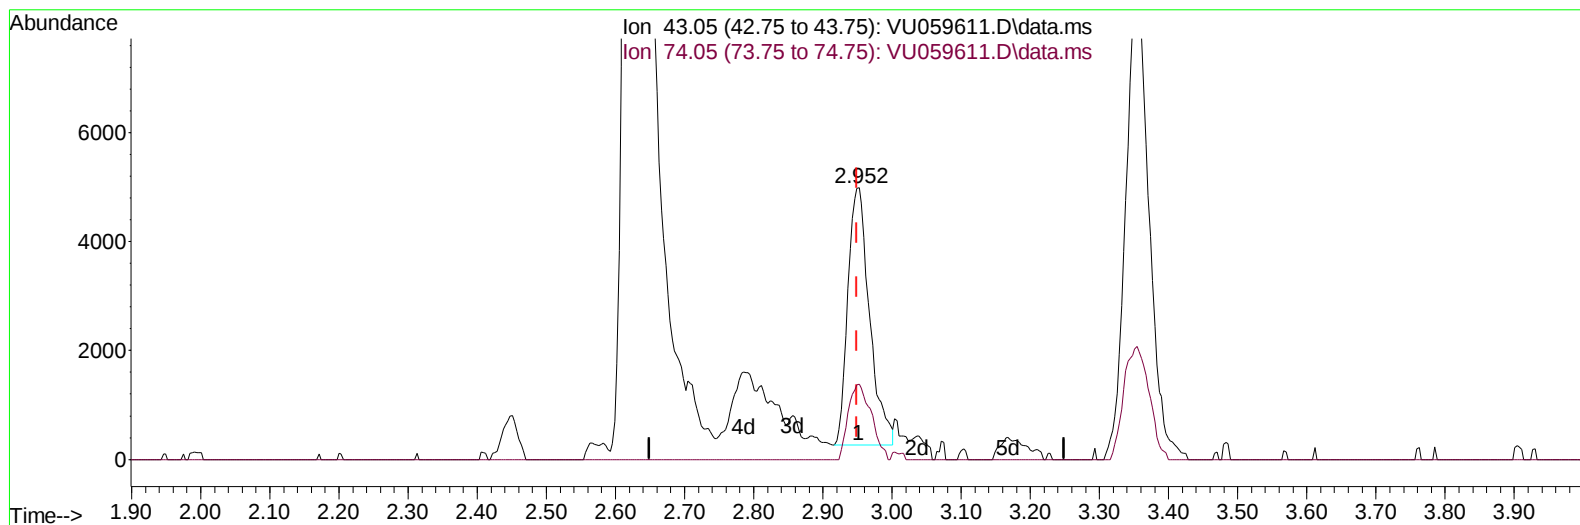

TIC: VU059611.D\data.ms

(15) Methyl Acetate (T)

2.952min (+ 0.003) 2.80 ug/L

response 10221

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 74.05 | 24.00  | 31.10# |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |




Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062824\  
 Data File : VU059611.D  
 Acq On : 28 Jun 2024 10:57  
 Operator : MD/SY  
 Sample : P3007-21MS  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 JMRJOMS

## Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/01/2024  
 Supervised By :Semsettin Yesilyurt 07/01/2024

Quant Time: Jun 28 23:14:24 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR061724WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Jun 28 02:08:17 2024  
 Response via : Initial Calibration

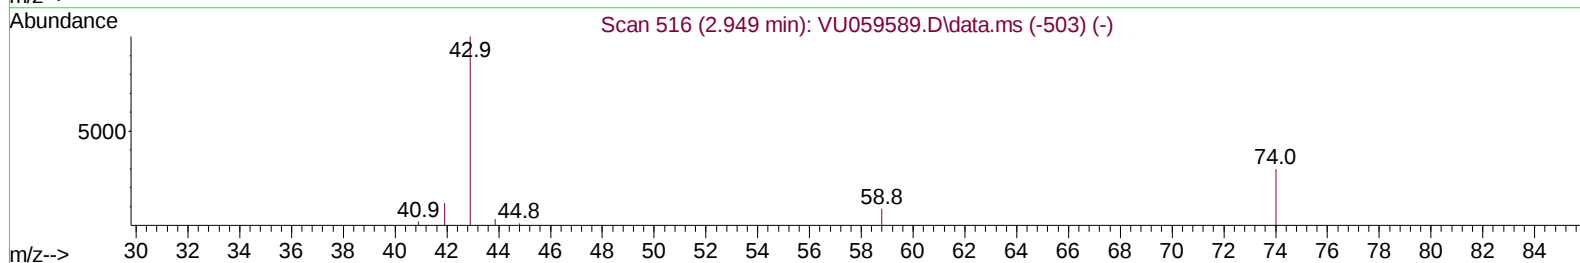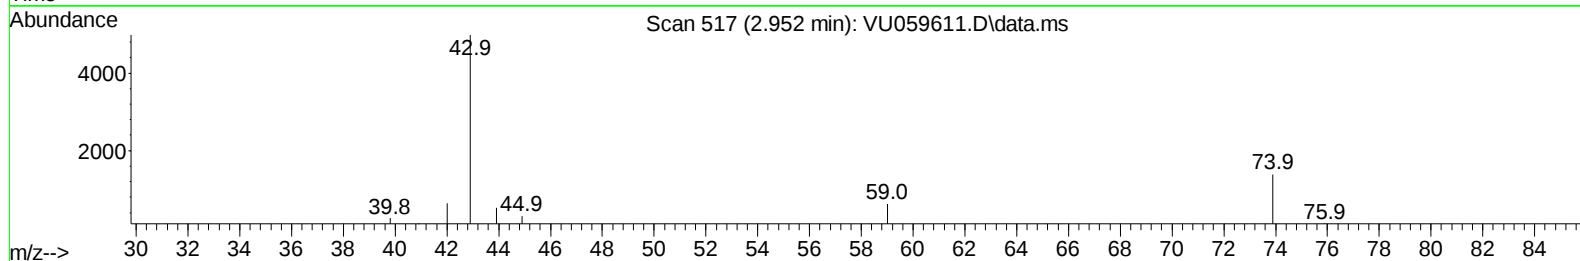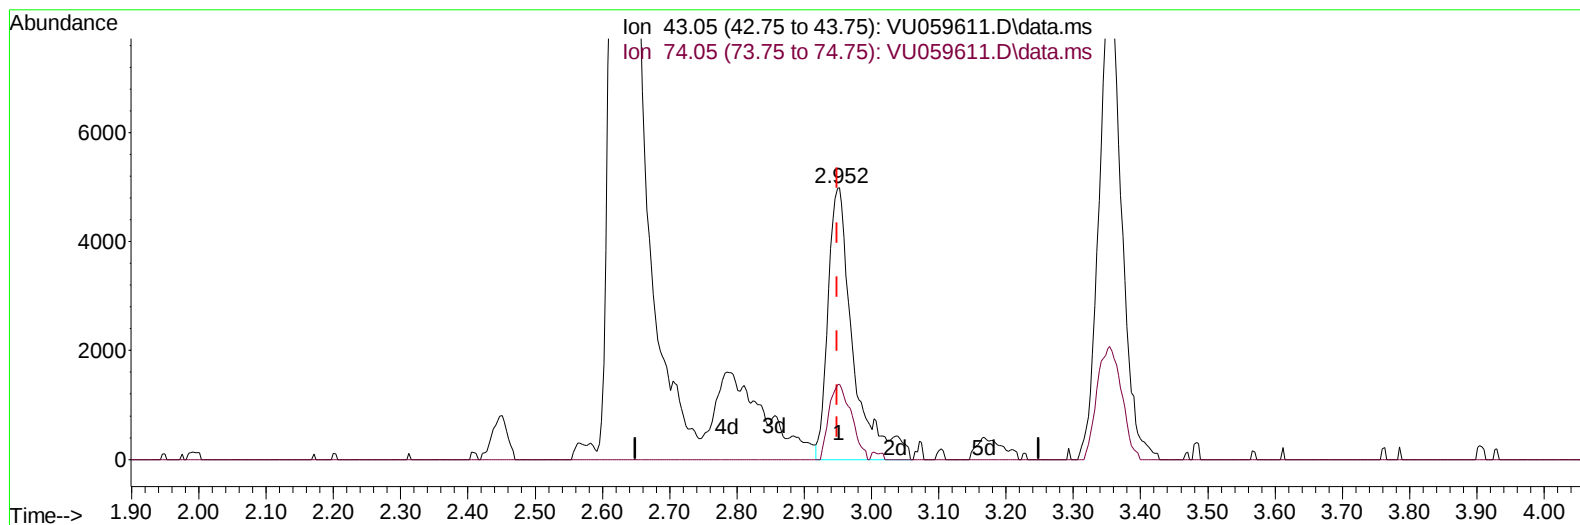

TIC: VU059611.D\data.ms

## (15) Methyl Acetate (T)

2.952min (+ 0.003) 3.53 ug/L m

response 12890

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 74.05 | 24.00  | 24.66  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062824\  
 Data File : VU059611.D  
 Acq On : 28 Jun 2024 10:57  
 Operator : MD/SY  
 Sample : P3007-21MS  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 JMRJOMS

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:14:24 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR061724WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Jun 28 02:08:17 2024  
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024  
 Supervised By :Semsettin Yesilyurt 07/01/2024

| Compound                      | R.T.     | QIon  | Response | Conc   | Units    | Dev(Min) |
|-------------------------------|----------|-------|----------|--------|----------|----------|
| -----                         |          |       |          |        |          |          |
| Internal Standards            |          |       |          |        |          |          |
| 1) 1,4-Difluorobenzene        | 6.242    | 114   | 149136   | 5.000  | ug/L     | 0.00     |
| 28) Chlorobenzene-d5          | 9.412    | 117   | 153662   | 5.000  | ug/L     | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.807   | 152   | 81118    | 5.000  | ug/L     | 0.00     |
| System Monitoring Compounds   |          |       |          |        |          |          |
| 4) Vinyl Chloride-d3          | 1.595    | 65    | 38173    | 3.681  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 40 | - 130 | Recovery | =      | 73.600%  |          |
| 7) Chloroethane-d5            | 1.907    | 69    | 42390    | 4.248  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 65 | - 130 | Recovery | =      | 85.000%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.560    | 65    | 17922    | 4.166  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 60 | - 125 | Recovery | =      | 83.400%  |          |
| 20) 2-Butanone-d5             | 4.618    | 46    | 106213   | 49.723 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 40 | - 130 | Recovery | =      | 99.440%  |          |
| 24) Chloroform-d              | 5.055    | 84    | 97845    | 4.597  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 125 | Recovery | =      | 92.000%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.692    | 65    | 46015    | 4.488  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 130 | Recovery | =      | 89.800%  |          |
| 32) Benzene-d6                | 5.721    | 84    | 195739   | 4.628  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 125 | Recovery | =      | 92.600%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.682    | 67    | 60408    | 4.662  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 60 | - 140 | Recovery | =      | 93.200%  |          |
| 41) Toluene-d8                | 7.891    | 98    | 184722   | 4.699  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 70 | - 130 | Recovery | =      | 94.000%  |          |
| 43) trans-1,3-Dichloroprop... | 8.174    | 79    | 18465    | 4.550  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 55 | - 130 | Recovery | =      | 91.000%  |          |
| 46) 2-Hexanone-d5             | 8.624    | 63    | 89223    | 52.919 | ug/L     | 0.00     |
| Spiked Amount 50.000          | Range 45 | - 130 | Recovery | =      | 105.840% |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.746   | 84    | 52276    | 4.882  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 65 | - 120 | Recovery | =      | 97.600%  |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.187   | 152   | 67173    | 4.653  | ug/L     | 0.00     |
| Spiked Amount 5.000           | Range 80 | - 120 | Recovery | =      | 93.000%  |          |
| Target Compounds              |          |       |          |        |          |          |
|                               |          |       |          |        |          | Qvalue   |
| 2) Dichlorodifluoromethane    | 1.380    | 85    | 59883    | 4.739  | ug/L     | 98       |
| 3) Chloromethane              | 1.518    | 50    | 68096    | 5.007  | ug/L     | 99       |
| 5) Vinyl chloride             | 1.602    | 62    | 73520    | 4.893  | ug/L     | 100      |
| 6) Bromomethane               | 1.853    | 94    | 35622    | 3.410  | ug/L     | 96       |
| 8) Chloroethane               | 1.930    | 64    | 49471    | 5.465  | ug/L     | 97       |
| 9) Trichlorofluoromethane     | 2.132    | 101   | 92830    | 5.133  | ug/L     | 96       |
| 10) 1,1,2-Trichloro-1,2,2-... | 2.573    | 101   | 56181    | 4.907  | ug/L     | 94       |
| 12) 1,1-Dichloroethene        | 2.573    | 96    | 53227    | 5.032  | ug/L     | 85       |
| 13) Acetone                   | 2.628    | 43    | 71560    | 51.643 | ug/L     | 91       |
| 14) Carbon disulfide          | 2.788    | 76    | 170972   | 4.845  | ug/L     | 100      |
| 15) Methyl Acetate            | 2.952    | 43    | 12890m   | 3.525  | ug/L     |          |
| 16) Methylene chloride        | 3.036    | 84    | 63012    | 5.027  | ug/L     | 91       |
| 17) Methyl tert-butyl Ether   | 3.354    | 73    | 116300   | 5.102  | ug/L     | 98       |
| 18) trans-1,2-Dichloroethene  | 3.345    | 96    | 55140    | 5.013  | ug/L     | 90       |
| 19) 1,1-Dichloroethane        | 3.859    | 63    | 103723   | 5.113  | ug/L     | 98       |
| 21) 2-Butanone                | 4.698    | 43    | 117543   | 52.887 | ug/L     | 92       |
| 22) cis-1,2-Dichloroethene    | 4.656    | 96    | 61976    | 5.111  | ug/L     | 95       |
| 23) Bromochloromethane        | 4.965    | 128   | 29856    | 5.401  | ug/L     | 84       |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062824\  
 Data File : VU059611.D  
 Acq On : 28 Jun 2024 10:57  
 Operator : MD/SY  
 Sample : P3007-21MS  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 JMRJOMS

## Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/01/2024  
 Supervised By :Semsettin Yesilyurt 07/01/2024

Quant Time: Jun 28 23:14:24 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR061724WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Jun 28 02:08:17 2024  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| 25) Chloroform                | 5.078  | 83   | 109598   | 5.130  | ug/L   | 99       |
| 27) 1,2-Dichloroethane        | 5.785  | 62   | 65238    | 5.039  | ug/L   | 99       |
| 29) 1,1,1-Trichloroethane     | 5.309  | 97   | 90497    | 5.100  | ug/L   | 96       |
| 30) Cyclohexane               | 5.380  | 56   | 74994    | 4.787  | ug/L   | 92       |
| 31) Carbon tetrachloride      | 5.518  | 117  | 74624    | 5.023  | ug/L   | 99       |
| 33) Benzene                   | 5.766  | 78   | 245286   | 5.257  | ug/L   | 100      |
| 34) Trichloroethene           | 6.534  | 95   | 61676    | 4.881  | ug/L   | 96       |
| 35) Methylcyclohexane         | 6.756  | 83   | 82741    | 4.601  | ug/L   | 93       |
| 37) 1,2-Dichloropropane       | 6.782  | 63   | 62944    | 5.212  | ug/L   | 98       |
| 38) Bromodichloromethane      | 7.097  | 83   | 77849    | 5.165  | ug/L   | 95       |
| 39) cis-1,3-Dichloropropene   | 7.598  | 75   | 76703    | 4.645  | ug/L   | 100      |
| 40) 4-Methyl-2-pentanone      | 7.782  | 43   | 288993   | 51.647 | ug/L   | 96       |
| 42) Toluene                   | 7.962  | 91   | 264489   | 5.354  | ug/L   | 99       |
| 44) trans-1,3-Dichloropropene | 8.203  | 75   | 62400    | 4.708  | ug/L   | 99       |
| 45) 1,1,2-Trichloroethane     | 8.393  | 97   | 48164    | 5.413  | ug/L   | 97       |
| 47) Tetrachloroethene         | 8.547  | 164  | 49346    | 5.032  | ug/L   | 98       |
| 48) 2-Hexanone                | 8.676  | 43   | 209302   | 52.411 | ug/L # | 92       |
| 49) Dibromochloromethane      | 8.801  | 129  | 51491    | 5.224  | ug/L   | 100      |
| 50) 1,2-Dibromoethane         | 8.917  | 107  | 43831    | 5.334  | ug/L   | 98       |
| 51) Chlorobenzene             | 9.441  | 112  | 162878   | 5.198  | ug/L   | 95       |
| 52) Ethylbenzene              | 9.563  | 91   | 259371   | 5.118  | ug/L   | 96       |
| 53) m,p-Xylene                | 9.688  | 106  | 104302   | 5.359  | ug/L   | 92       |
| 54) o-Xylene                  | 10.094 | 106  | 97039    | 5.253  | ug/L   | 97       |
| 55) Styrene                   | 10.110 | 104  | 165807   | 5.273  | ug/L   | 95       |
| 57) 1,1,2,2-Tetrachloroethane | 10.775 | 83   | 58081    | 5.380  | ug/L   | 98       |
| 59) Bromoform                 | 10.283 | 173  | 31712    | 5.108  | ug/L # | 98       |
| 60) Isopropylbenzene          | 10.476 | 105  | 253798   | 5.065  | ug/L   | 99       |
| 61) 1,2,3-Trichloropropane    | 10.814 | 75   | 37838    | 5.048  | ug/L   | 96       |
| 62) 1,3,5-Trimethylbenzene    | 11.081 | 105  | 191146   | 4.815  | ug/L   | 97       |
| 63) 1,2,4-Trimethylbenzene    | 11.460 | 105  | 191720   | 5.051  | ug/L   | 98       |
| 64) 1,3-Dichlorobenzene       | 11.740 | 146  | 131627   | 5.165  | ug/L   | 99       |
| 65) 1,4-Dichlorobenzene       | 11.830 | 146  | 130541   | 4.976  | ug/L   | 98       |
| 67) 1,2-Dichlorobenzene       | 12.206 | 146  | 121914   | 5.083  | ug/L   | 98       |
| 68) 1,2-Dibromo-3-chloropr... | 12.991 | 75   | 7551     | 5.164  | ug/L # | 73       |
| 69) 1,3,5-Trichlorobenzene    | 13.212 | 180  | 90540    | 4.799  | ug/L   | 98       |
| 70) 1,2,4-trichlorobenzene    | 13.833 | 180  | 70862    | 4.896  | ug/L   | 99       |
| 71) Naphthalene               | 14.081 | 128  | 95576    | 4.614  | ug/L   | 98       |
| 72) 1,2,3-Trichlorobenzene    | 14.322 | 180  | 66598    | 4.956  | ug/L   | 98       |

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062824\  
 Data File : VU059611.D  
 Acq On : 28 Jun 2024 10:57  
 Operator : MD/SY  
 Sample : P3007-21MS  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 51 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 JMRJOMS

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:14:24 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR061724WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Fri Jun 28 02:08:17 2024  
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024  
 Supervised By :Semsettin Yesilyurt 07/01/2024

