


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062824\
Data File : VU059563.D
Acq On : 27 Jun 2024 15:07
Operator : MD/SY
Sample : BFB166
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB166

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Jun 29 01:51:23 2024

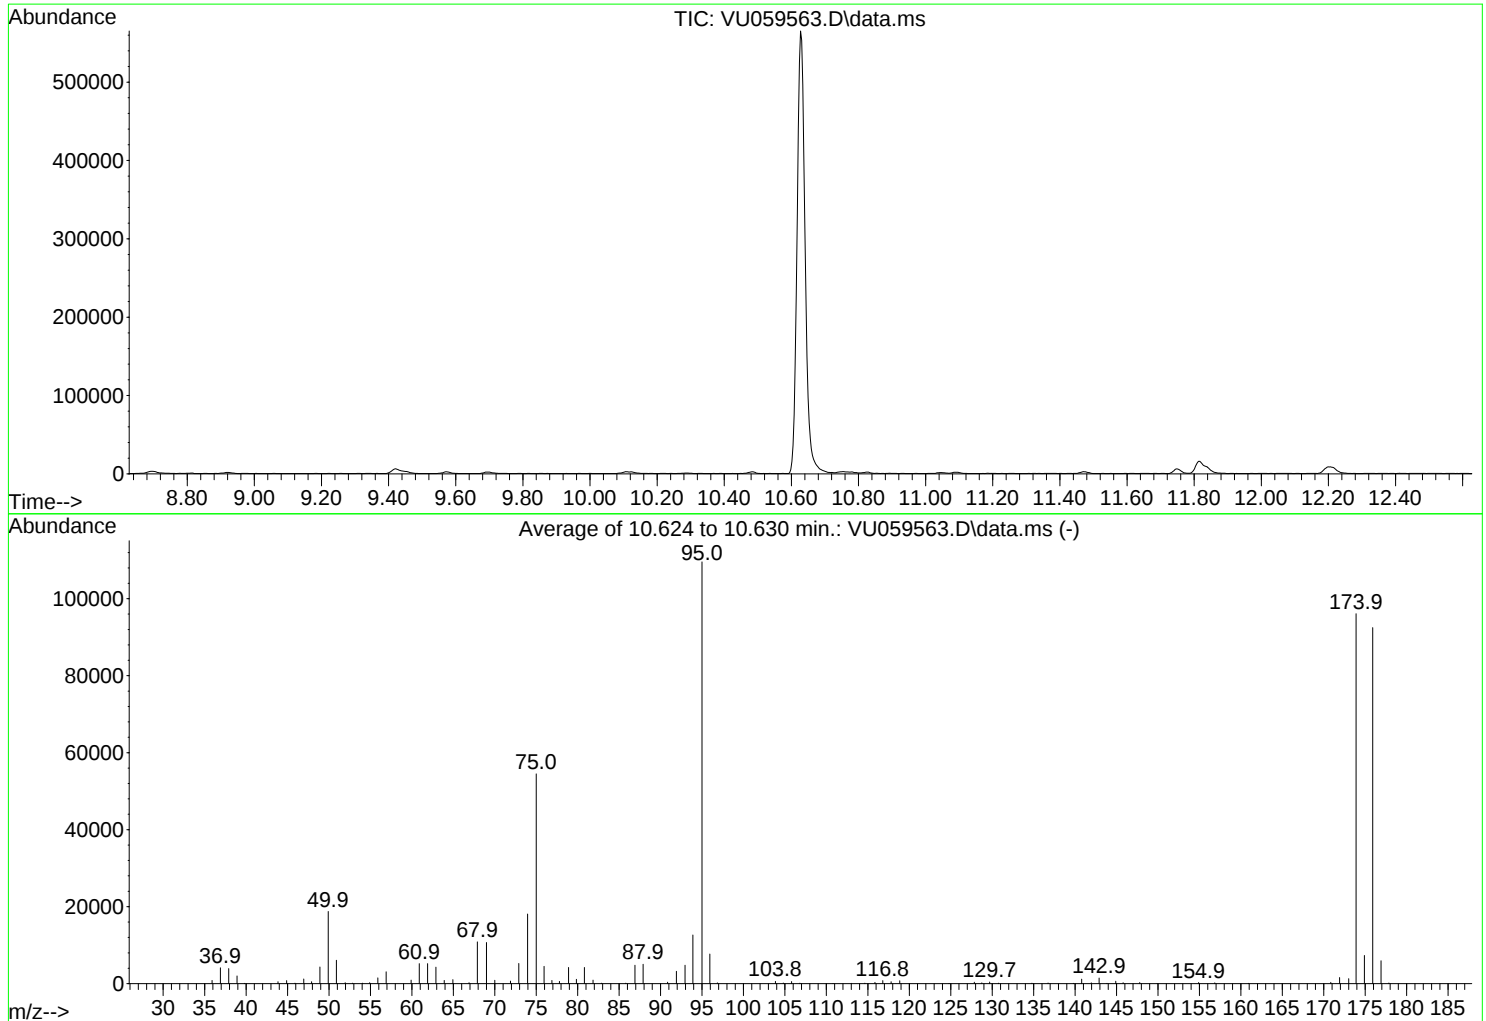

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.1	18768	PASS
75	95	30	80	49.7	54493	PASS
95	95	100	100	100.0	109579	PASS
96	95	5	9	7.0	7678	PASS
173	174	0.00	2	1.3	1282	PASS
174	95	50	120	87.7	96085	PASS
175	174	5	9	7.6	7300	PASS
176	174	95	101	96.3	92493	PASS
177	176	5	9	6.4	5935	PASS

m/z	Abundance
39.80	201.0
43.80	285.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166

m/z	Abundance
35.90	750.0
36.90	4007.0
37.90	3639.0
38.90	1956.0
39.90	320.0
43.90	787.0
44.90	836.0
45.90	137.0
47.00	1112.0
47.90	521.0
48.90	4153.0
49.90	18000.0
50.90	6113.0
52.00	226.0
52.90	108.0
54.10	120.0
54.90	252.0
55.90	1408.0
56.90	3041.0
59.90	850.0
60.90	5052.0
61.90	5186.0
62.90	4156.0
63.90	879.0
64.90	963.0
66.90	175.0
67.90	10273.0
69.00	10537.0
70.00	811.0
71.90	656.0
72.90	5006.0
74.00	17824.0
75.00	52656.0
76.00	4238.0
76.90	793.0
77.80	562.0
78.90	4086.0
79.90	984.0
80.80	4206.0
81.80	821.0
85.80	131.0
86.90	4598.0
87.90	4582.0
90.80	364.0
91.90	3029.0
93.00	4777.0
93.90	12643.0
95.00	105224.0
96.00	7196.0
96.90	138.0
103.80	554.0
104.80	124.0
105.80	487.0
106.80	109.0
113.00	105.0
114.80	108.0
115.90	323.0
116.80	755.0
117.80	440.0
118.90	772.0
124.80	103.0
127.80	392.0
128.80	231.0
129.70	414.0
130.70	123.0
134.80	103.0
136.70	166.0
140.80	1044.0
142.00	188.0
142.90	1392.0
144.90	655.0
145.80	194.0
147.80	317.0
154.90	300.0
156.80	161.0
170.90	354.0
171.90	1521.0
173.00	1236.0
173.90	90664.0
174.90	7034.0
175.90	87776.0
176.90	5520.0
177.80	174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166

m/z	Abundance
35.90	830.0
36.90	4226.0
37.90	4031.0
38.90	2088.0
39.80	300.0
43.90	817.0
44.90	820.0
45.90	146.0
46.90	1249.0
47.90	509.0
48.90	4454.0
49.90	19360.0
50.90	6287.0
52.00	247.0
52.80	121.0
54.10	123.0
54.90	253.0
55.90	1534.0
56.90	3183.0
59.90	947.0
60.90	5360.0
61.90	5352.0
62.90	4412.0
63.90	837.0
64.90	1044.0
66.90	241.0
67.90	11179.0
69.00	10988.0
70.00	934.0
71.90	679.0
72.90	5472.0
74.00	18640.0
75.00	56168.0
76.00	4588.0
76.90	884.0
77.80	625.0
78.90	4304.0
79.80	1148.0
80.80	4354.0
81.80	923.0
82.90	153.0
85.80	120.0
86.90	4885.0
87.90	5106.0
90.90	424.0
91.90	3313.0
93.00	4979.0
93.90	13048.0
95.00	113128.0
95.90	8041.0
96.80	216.0
103.90	584.0
104.80	159.0
105.80	548.0
106.80	147.0
113.00	100.0
114.60	132.0
115.90	364.0
116.80	817.0
117.80	516.0
118.90	770.0
127.80	411.0
128.70	236.0
129.70	427.0
130.70	128.0
134.80	128.0
136.70	207.0
139.80	108.0
140.80	1222.0
141.90	213.0
142.90	1488.0
143.90	108.0
144.90	664.0
145.80	263.0
147.80	328.0
154.90	272.0
156.90	206.0
160.90	118.0
170.90	343.0
171.90	1601.0
173.00	1318.0
173.90	99152.0
174.90	7601.0
175.90	95264.0
176.90	6034.0
177.80	165.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166

m/z	Abundance
35.90	856.0
36.90	4104.0
37.90	4062.0
38.90	1896.0
39.80	264.0
43.90	803.0
44.90	751.0
45.90	131.0
46.90	1218.0
47.90	508.0
48.90	4306.0
49.90	18944.0
50.90	5787.0
51.90	233.0
52.80	107.0
54.00	137.0
54.90	228.0
55.90	1509.0
56.90	3023.0
59.90	1010.0
60.90	5171.0
61.90	5077.0
62.90	4281.0
63.90	767.0
65.00	1069.0
66.90	313.0
67.90	11147.0
69.00	10467.0
70.00	865.0
71.90	619.0
72.90	5283.0
73.90	17792.0
75.00	54656.0
75.90	4652.0
76.90	829.0
77.80	562.0
78.90	4229.0
79.80	1253.0
80.80	3983.0
81.90	973.0
82.80	171.0
85.80	107.0
86.90	4816.0
87.90	5397.0
90.90	402.0
91.90	3213.0
92.90	4613.0
93.90	12175.0
95.00	110384.0
95.90	7798.0
96.80	251.0
103.90	621.0
104.80	170.0
105.80	582.0
106.80	157.0
110.80	102.0
114.60	168.0
115.80	376.0
116.80	803.0
117.80	552.0
118.80	659.0
127.90	373.0
128.80	208.0
129.70	372.0
130.80	171.0
134.80	156.0
136.80	189.0
139.80	110.0
140.80	1216.0
141.90	181.0
142.90	1436.0
143.80	129.0
144.90	584.0
145.80	258.0
147.80	276.0
149.90	108.0
154.90	251.0
156.80	224.0
160.90	112.0
170.80	282.0
171.90	1585.0
173.00	1292.0
173.90	98440.0
174.90	7265.0
175.90	94440.0
176.90	6252.0
177.90	139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB166