


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062918\
Data File : VU025060.D
Acq On : 29 Jun 2018 09:47
Operator : MD/SY
Sample : BFB40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB40

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM062918WMA.M
Title : VOC Analysis
Last Update : Fri Jun 29 23:41:20 2018

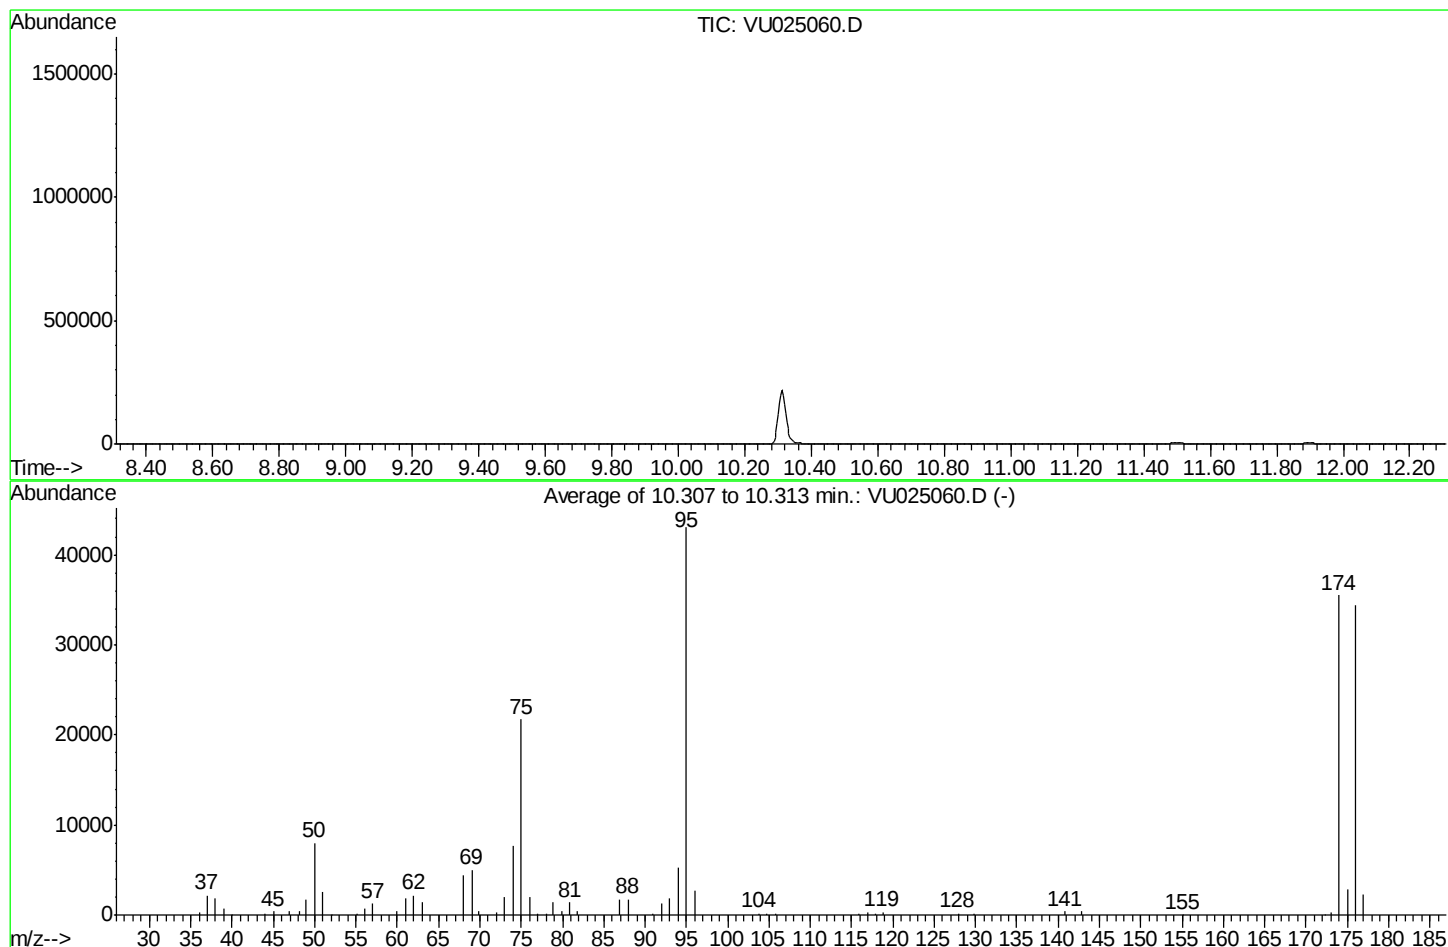

AutoFind: Scans 3022, 3023, 3024; Background Corrected with Scan 3011

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	7963	PASS
75	95	30	80	50.4	21685	PASS
95	95	100	100	100.0	43050	PASS
96	95	5	9	6.4	2772	PASS
173	174	0.00	2	0.7	246	PASS
174	95	50	120	82.5	35528	PASS
175	174	5	9	7.9	2795	PASS
176	174	95	101	96.8	34381	PASS
177	176	5	9	6.7	2289	PASS

Scan 3011 (10.272 min): VU025060.D
BFB40

m/z	Abundance
40.00	114.0
43.90	442.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	301.0
37.00	2218.0
38.00	1712.0
39.00	660.0
39.90	142.0
44.00	525.0
45.00	403.0
47.00	399.0
48.10	393.0
49.00	1590.0
50.00	7908.0
51.00	2404.0
52.10	110.0
55.00	147.0
56.00	650.0
57.00	1192.0
60.00	368.0
61.00	1864.0
62.00	2067.0
63.00	1324.0
68.00	4157.0
69.00	4575.0
69.90	421.0
71.90	241.0
73.00	1853.0
74.00	7347.0
75.00	20832.0
76.00	2021.0
77.10	142.0
78.00	163.0
78.90	1342.0
79.80	362.0
80.90	1279.0
81.90	347.0
87.00	1797.0
88.00	1594.0
91.00	153.0
92.00	1164.0
93.00	1752.0
94.00	5104.0
95.00	40712.0
96.00	2682.0
103.80	196.0
104.70	100.0
105.70	162.0
115.90	142.0
116.90	311.0
117.90	111.0
118.80	275.0
128.00	137.0
129.80	151.0
140.80	387.0
142.80	350.0
174.00	32592.0
175.00	2563.0
176.00	31440.0
177.00	2156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	321.0
37.00	2232.0
38.00	1915.0
39.00	689.0
39.90	165.0
44.00	565.0
45.00	433.0
46.90	377.0
48.10	401.0
49.00	1750.0
50.00	8251.0
51.00	2596.0
55.10	108.0
56.00	659.0
57.00	1287.0
60.00	426.0
61.00	1924.0
62.00	2202.0
63.00	1457.0
68.00	4514.0
69.00	5191.0
69.90	422.0
71.90	211.0
73.00	2005.0
74.00	8028.0
75.00	22328.0
76.00	2066.0
77.00	155.0
78.00	195.0
78.90	1466.0
79.90	380.0
80.90	1411.0
81.80	396.0
87.00	1831.0
88.00	1800.0
91.00	215.0
92.00	1335.0
93.00	1880.0
94.00	5501.0
95.00	44280.0
96.00	2878.0
103.80	188.0
104.80	120.0
105.70	187.0
115.80	146.0
116.90	280.0
117.90	132.0
118.80	314.0
127.90	179.0
129.80	144.0
140.90	425.0
142.90	435.0
172.30	121.0
173.00	345.0
174.00	36552.0
175.00	2882.0
176.00	35464.0
177.00	2402.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40

m/z	Abundance
36.00	314.0
37.00	1955.0
38.00	1815.0
39.00	686.0
39.90	194.0
44.00	581.0
45.00	376.0
46.90	340.0
48.10	318.0
49.00	1850.0
50.00	7730.0
51.00	2568.0
56.00	653.0
57.00	1265.0
60.00	399.0
61.00	1966.0
62.00	2194.0
63.00	1470.0
68.00	4497.0
69.00	5166.0
69.90	357.0
72.00	206.0
73.00	2124.0
74.00	7769.0
75.00	21896.0
76.00	1933.0
77.00	189.0
78.00	175.0
78.90	1380.0
79.90	388.0
80.90	1415.0
81.80	397.0
86.90	1684.0
87.90	1920.0
90.90	231.0
92.00	1307.0
93.00	1763.0
94.00	5191.0
95.00	44160.0
96.00	2756.0
103.80	180.0
104.80	110.0
105.80	190.0
115.80	163.0
116.90	239.0
117.90	135.0
118.80	299.0
127.90	190.0
129.90	136.0
140.90	455.0
142.90	464.0
155.10	111.0
173.00	393.0
174.00	37440.0
175.00	2941.0
176.00	36240.0
177.00	2311.0

Instrument :
MSVOA_U
ClientSampleId :
BFB40