


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU062919\
Data File : VU033067.D
Acq On : 28 Jun 2019 12:32
Operator : JC/SP
Sample : BFB22
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB22

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR062719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Sat Jun 29 03:29:42 2019

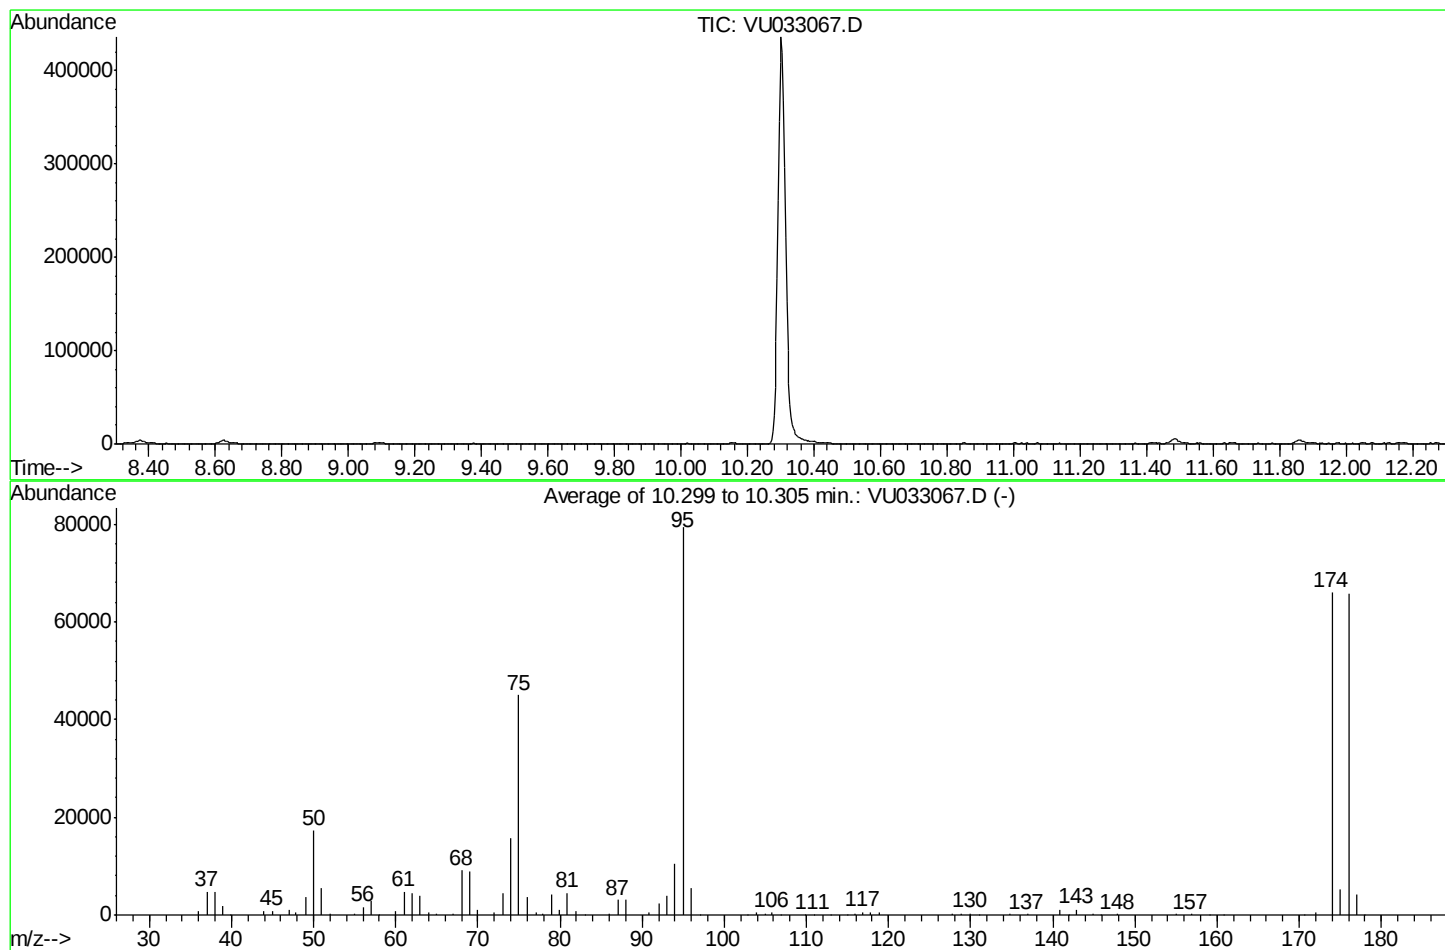

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	17274	PASS
75	95	30	80	56.7	44984	PASS
95	95	100	100	100.0	79341	PASS
96	95	5	9	6.8	5419	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.2	65992	PASS
175	174	5	9	7.8	5164	PASS
176	174	95	101	99.6	65733	PASS
177	176	5	9	6.5	4272	PASS

Scan 2852 (10.260 min): VU033067.D
BFB22

m/z	Abundance
39.80	148.0
43.90	372.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
36.00	827.0
37.00	4868.0
38.00	4721.0
39.00	1956.0
39.90	231.0
44.00	1099.0
45.00	782.0
47.10	930.0
47.80	558.0
49.00	3684.0
50.00	17280.0
51.00	5469.0
51.90	244.0
55.10	287.0
56.00	1565.0
57.00	2815.0
58.00	127.0
60.00	850.0
61.00	4646.0
62.00	4387.0
63.00	3819.0
63.90	437.0
65.00	309.0
67.00	317.0
68.00	9019.0
69.00	8913.0
70.00	946.0
71.90	493.0
73.00	4406.0
74.00	15420.0
75.00	44368.0
76.00	3694.0
77.10	491.0
77.90	353.0
78.90	4227.0
79.90	1115.0
80.90	4435.0
81.90	730.0
83.00	139.0
86.00	177.0
87.00	3078.0
88.00	2965.0
90.80	413.0
92.00	2495.0
93.00	3898.0
94.00	10169.0
95.00	77072.0
96.00	5178.0
97.00	137.0
102.80	118.0
103.90	473.0
105.00	162.0
105.80	467.0
110.80	128.0
112.90	116.0
115.90	289.0
116.90	617.0
117.80	409.0
118.90	463.0
127.90	287.0
128.80	156.0
129.90	345.0
134.70	171.0
136.90	145.0
140.90	1112.0
141.90	134.0
142.90	1124.0
144.80	223.0
145.90	108.0
147.90	207.0
155.00	181.0
156.80	183.0
172.00	630.0
174.00	62704.0
175.00	4881.0
176.00	62424.0
177.00	4205.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
36.00	927.0
37.00	4944.0
38.00	4864.0
39.00	1985.0
39.90	244.0
44.00	1099.0
45.00	889.0
47.10	995.0
47.80	546.0
49.00	3814.0
50.00	17864.0
51.00	5643.0
52.00	253.0
55.00	236.0
56.00	1611.0
57.00	2878.0
58.00	139.0
59.90	864.0
61.00	4993.0
62.00	4560.0
63.00	3989.0
63.90	443.0
64.90	328.0
67.10	316.0
68.00	9351.0
69.00	9213.0
70.00	1050.0
72.00	565.0
73.00	4541.0
74.00	16369.0
75.00	46776.0
76.00	3812.0
77.00	507.0
77.90	370.0
78.90	4397.0
79.90	1189.0
80.90	4645.0
82.00	779.0
83.00	142.0
86.00	205.0
87.00	3241.0
87.90	3160.0
90.90	455.0
92.00	2504.0
93.00	4133.0
94.00	10677.0
95.00	82136.0
96.00	5663.0
97.00	105.0
102.80	143.0
104.00	535.0
105.00	143.0
105.80	533.0
106.80	117.0
109.90	102.0
110.80	137.0
112.90	149.0
114.90	123.0
115.90	351.0
116.90	683.0
117.80	441.0
118.90	576.0
127.80	276.0
128.80	173.0
129.90	346.0
131.00	108.0
134.80	144.0
136.90	154.0
140.90	1185.0
141.90	129.0
142.90	1180.0
144.80	208.0
145.90	145.0
147.90	244.0
155.00	170.0
156.90	196.0
160.80	103.0
170.60	110.0
172.00	709.0
174.00	67944.0
175.00	5344.0
176.00	68136.0
177.00	4426.0
177.90	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22

m/z	Abundance
36.00	956.0
37.00	4602.0
38.00	4499.0
39.00	1814.0
39.90	260.0
44.00	1074.0
45.00	942.0
47.10	962.0
47.80	528.0
49.00	3701.0
50.00	16680.0
51.00	5263.0
52.00	297.0
54.90	194.0
56.00	1575.0
57.00	2655.0
58.00	147.0
59.90	847.0
61.00	4843.0
62.00	4332.0
63.00	3733.0
64.00	402.0
64.90	338.0
67.10	299.0
68.00	8902.0
69.00	8672.0
70.00	930.0
72.00	573.0
73.00	4294.0
74.00	15689.0
75.00	43808.0
76.00	3511.0
77.00	458.0
77.90	333.0
78.90	4144.0
79.90	1113.0
80.90	4401.0
82.00	770.0
83.00	107.0
86.00	163.0
87.00	3070.0
87.90	3061.0
90.90	414.0
92.00	2319.0
93.00	3852.0
94.00	10254.0
95.00	78816.0
96.00	5417.0
102.80	116.0
103.90	514.0
104.90	116.0
105.90	532.0
106.90	107.0
109.90	100.0
110.90	120.0
112.90	153.0
114.90	129.0
115.90	355.0
116.90	681.0
117.90	461.0
118.90	654.0
127.70	289.0
128.90	167.0
130.00	347.0
130.90	122.0
134.80	129.0
136.90	178.0
140.90	1102.0
141.70	136.0
142.90	1164.0
144.90	154.0
145.90	147.0
147.90	227.0
154.80	176.0
156.90	163.0
159.00	113.0
160.70	110.0
170.50	103.0
172.00	648.0
174.00	67328.0
175.00	5269.0
176.00	66640.0
177.00	4187.0
177.90	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB22