

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
 Data File : VU049502.D
 Acq On : 29 Jun 2022 11:05
 Operator : SY/MD
 Sample : VU0629MBL01
 Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0629MBL01

Quant Time: Jun 30 00:47:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 28 10:35:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.372	168	281800	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.250	114	489430	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.417	117	440427	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	196861	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.703	65	192252	44.299	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	88.600%
35) Dibromofluoromethane	5.289	113	153377	44.792	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	89.580%
50) Toluene-d8	7.896	98	592647	48.525	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	97.060%
62) 4-Bromofluorobenzene	10.632	95	208145	44.490	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	88.980%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
Data File : VU049502.D
Acq On : 29 Jun 2022 11:05
Operator : SY/MD
Sample : VU0629MBL01
Misc : 5.00g/10mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0629MBL01

Quant Time: Jun 30 00:47:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 28 10:35:43 2022
Response via : Initial Calibration




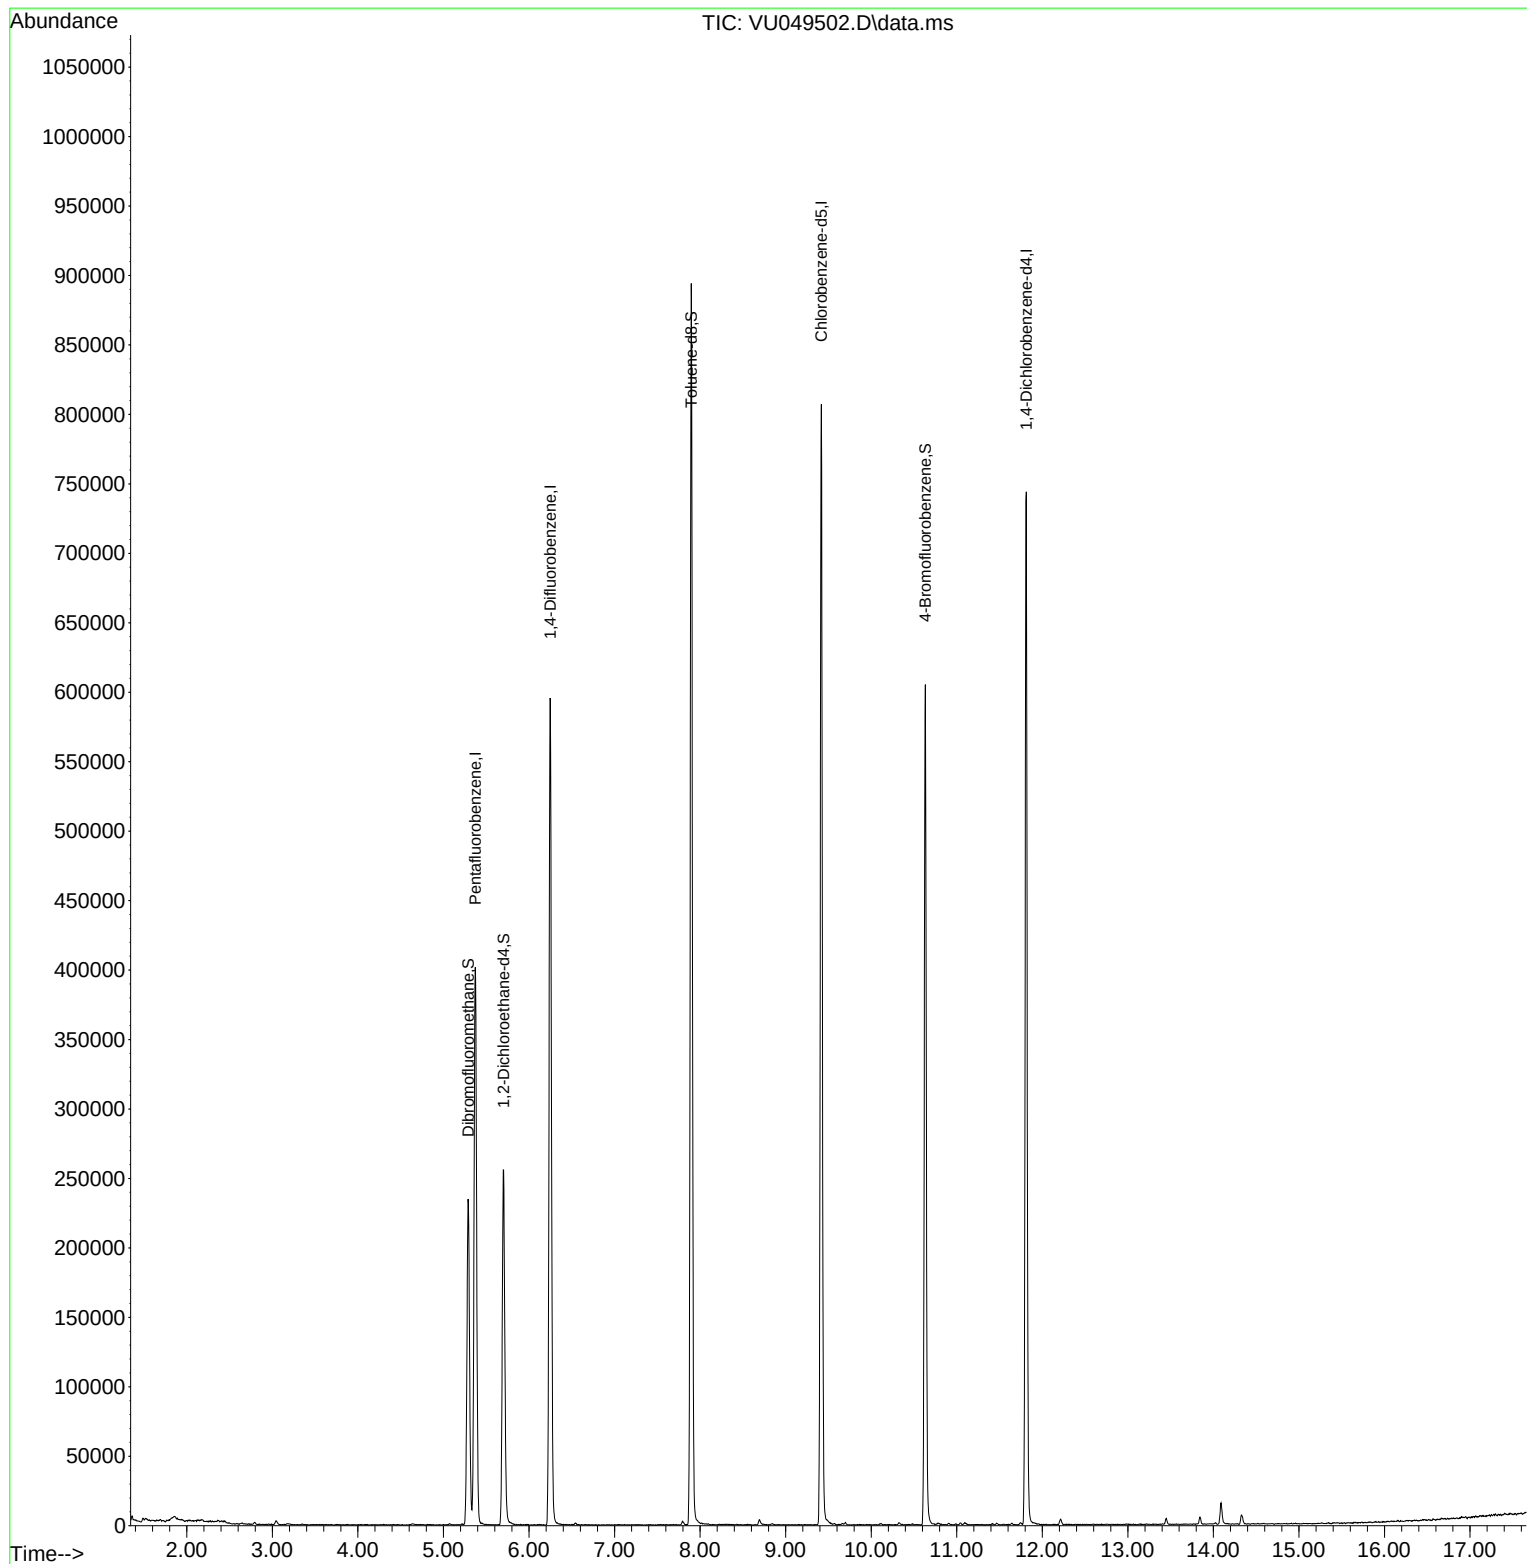


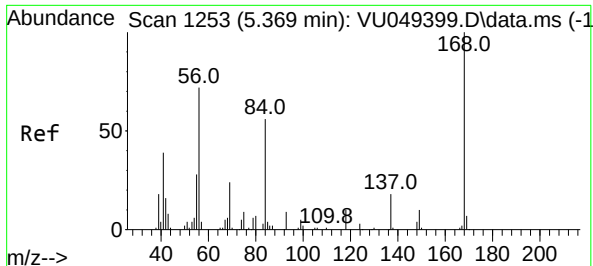

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.372 min Scan# 11
Delta R.T. 0.003 min
Lab File: VU049502.D
Acq: 29 Jun 2022 11:05




Instrument :
MSVOA_U
ClientSampleId :
VU0629MBL01


Tgt Ion:168 Resp: 281800
Ion Ratio Lower Upper
168 100
99 59.7 39.3 58.9#

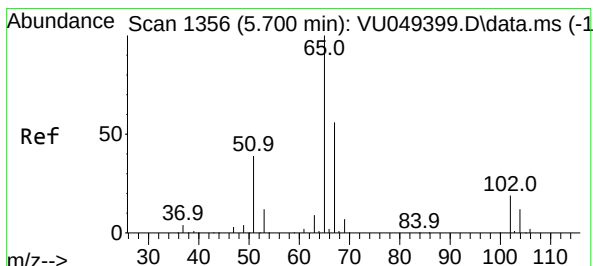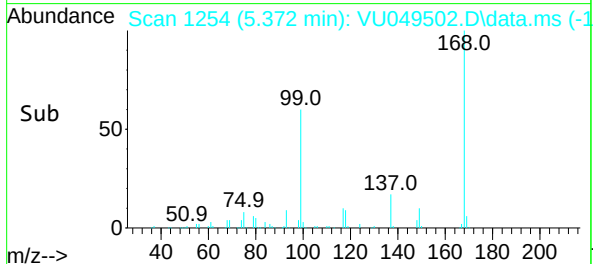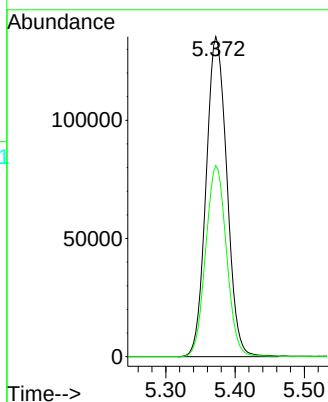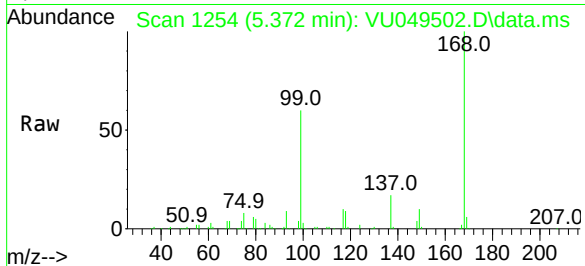

#33
1,2-Dichloroethane-d4
Concen: 44.299 ug/l
RT: 5.703 min Scan# 1357
Delta R.T. 0.003 min
Lab File: VU049502.D
Acq: 29 Jun 2022 11:05

Tgt Ion: 65 Resp: 192252
Ion Ratio Lower Upper
65 100
67 54.3 0.0 108.0

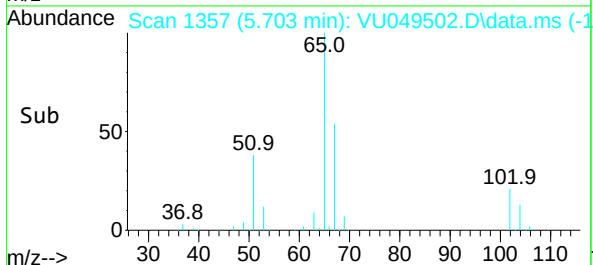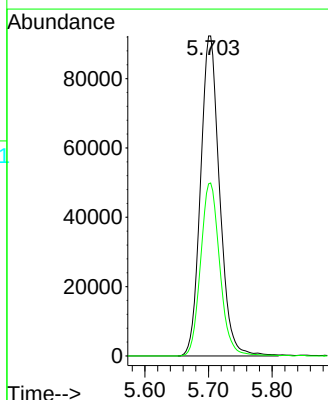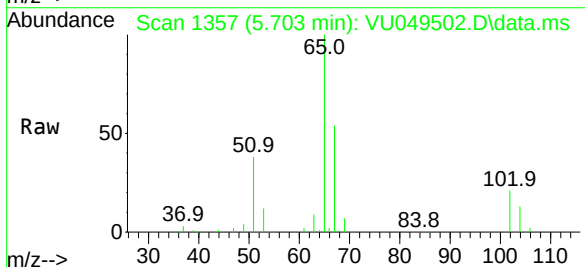

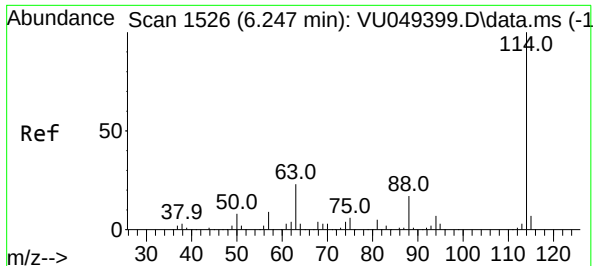

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.250 min Scan# 11

Delta R.T. 0.003 min

Lab File: VU049502.D

Acq: 29 Jun 2022 11:05

Instrument :

MSVOA_U

ClientSampleId :

VU0629MBL01





Tgt Ion:114 Resp: 489430

Ion Ratio Lower Upper

114 100

63 22.1 0.0 37.8

88 16.9 0.0 29.2

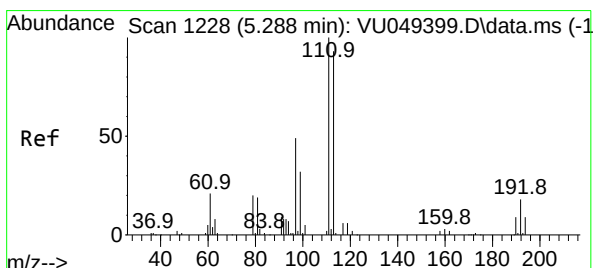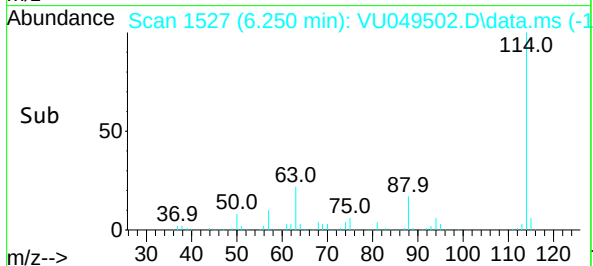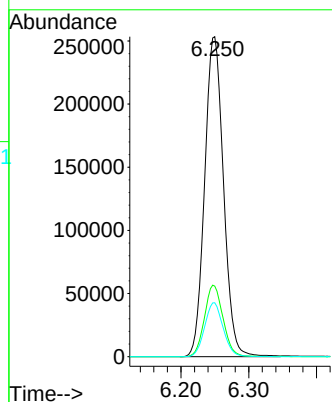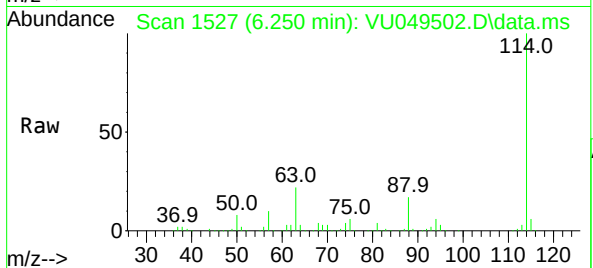

#35

Dibromofluoromethane

Concen: 44.792 ug/l

RT: 5.289 min Scan# 1228

Delta R.T. 0.000 min

Lab File: VU049502.D

Acq: 29 Jun 2022 11:05




Tgt Ion:113 Resp: 153377


Ion Ratio Lower Upper

113 100

111 104.8 82.1 123.1

192 19.3 18.0 27.0


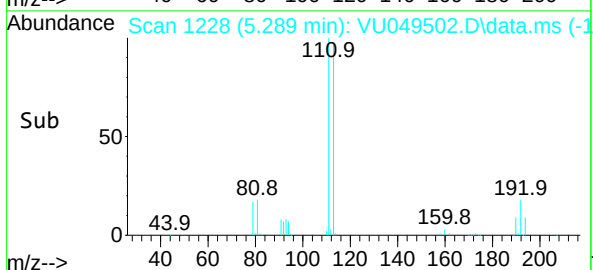
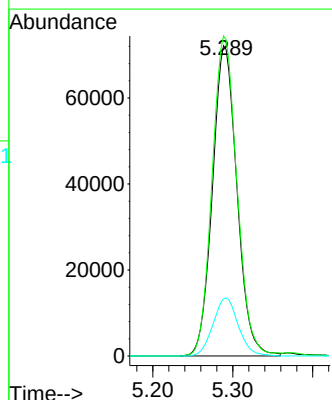
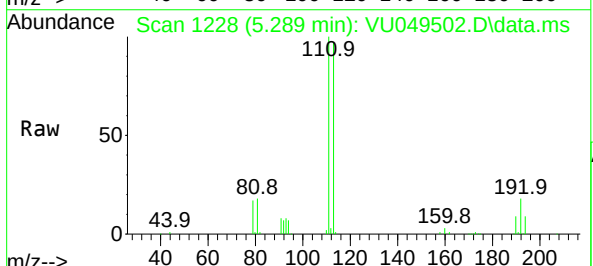


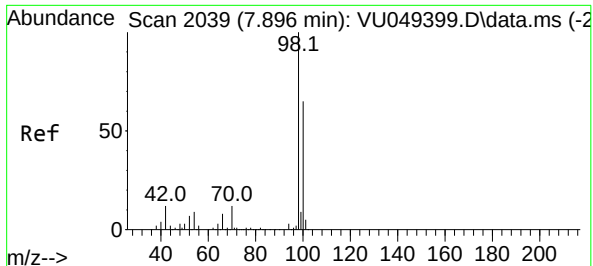

#50
Toluene-d8
Concen: 48.525 ug/l
RT: 7.896 min Scan# 2039
Delta R.T. 0.000 min
Lab File: VU049502.D
Acq: 29 Jun 2022 11:05




Instrument :
MSVOA_U
ClientSampleId :
VU0629MBL01


Tgt Ion: 98 Resp: 592647
Ion Ratio Lower Upper
98 100
100 64.8 51.7 77.5

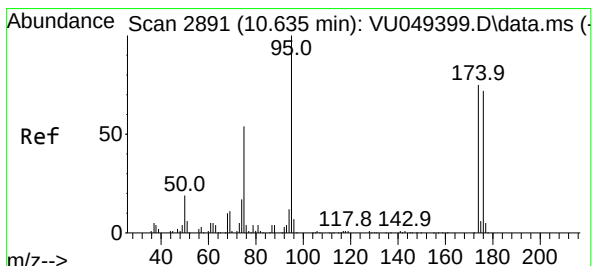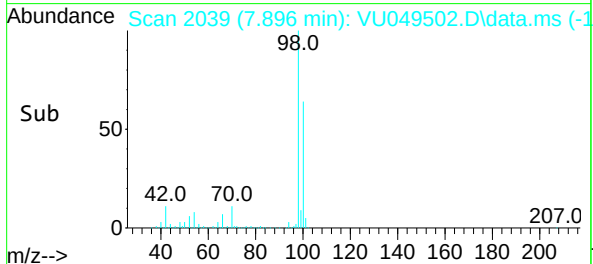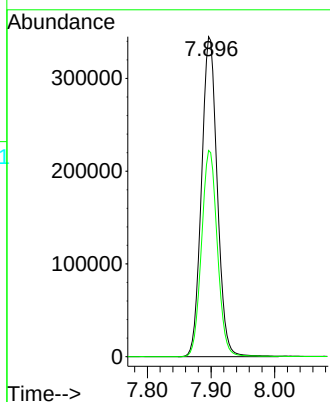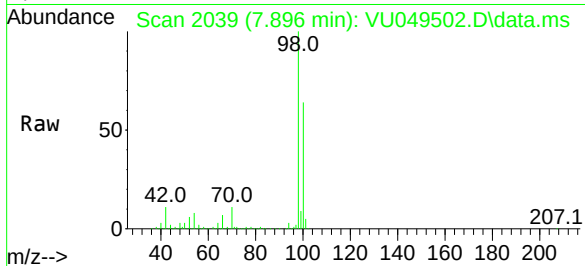

#62
4-Bromofluorobenzene
Concen: 44.490 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.003 min
Lab File: VU049502.D
Acq: 29 Jun 2022 11:05

Tgt Ion: 95 Resp: 208145
Ion Ratio Lower Upper
95 100
174 75.6 0.0 182.0
176 73.6 0.0 177.8


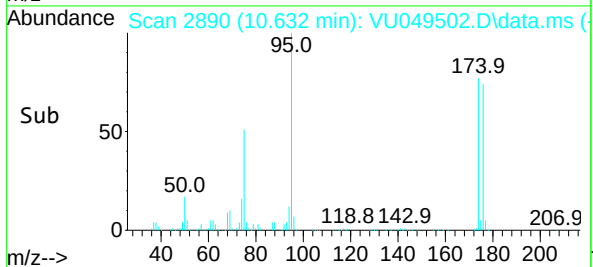
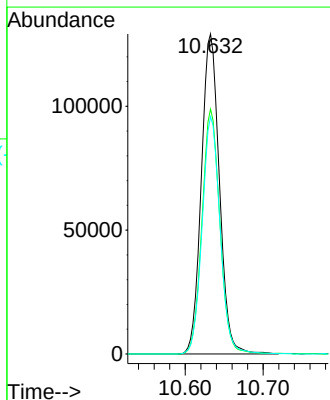
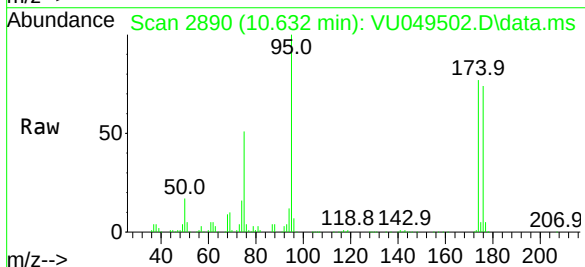


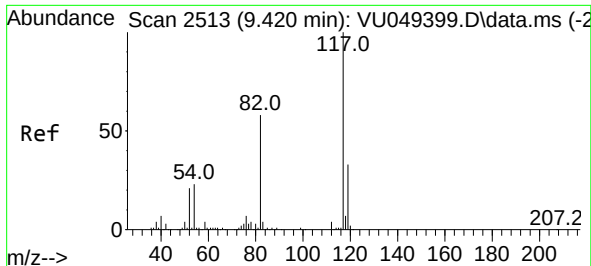

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.417 min Scan# 21
Delta R.T. -0.003 min
Lab File: VU049502.D
Acq: 29 Jun 2022 11:05

Instrument :
MSVOA_U
ClientSampleId :
VU0629MBL01

Tgt Ion:117 Resp: 440427
Ion Ratio Lower Upper
117 100
82 58.5 41.7 62.5
119 32.0 25.7 38.5

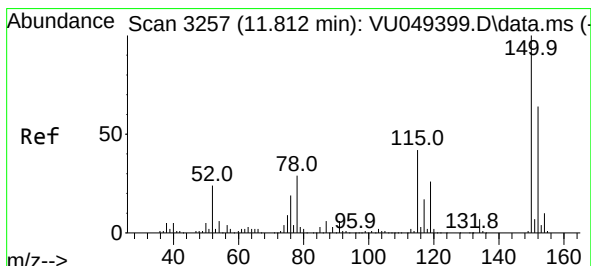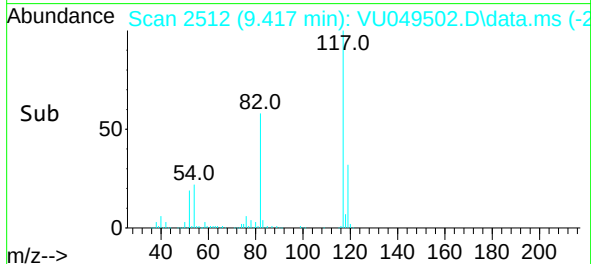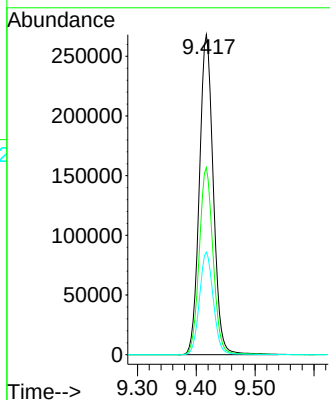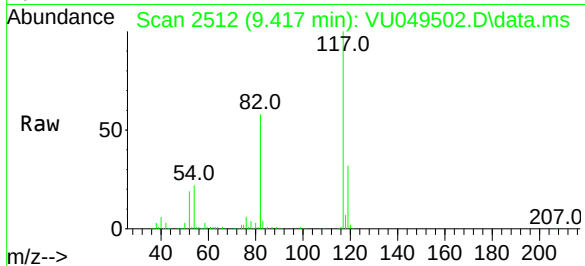

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.812 min Scan# 3257
Delta R.T. 0.000 min
Lab File: VU049502.D
Acq: 29 Jun 2022 11:05

Tgt Ion:152 Resp: 196861
Ion Ratio Lower Upper
152 100
115 62.1 37.0 110.9
150 156.6 0.0 342.2

