

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
 Data File : VU049530.D
 Acq On : 29 Jun 2022 22:49
 Operator : SY/MD
 Sample : VU0629WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0629WBL02

Quant Time: Jun 30 00:51:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 28 10:35:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.372	168	250298	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.250	114	439498	50.000	ug/l	0.00
63) Chlorobenzene-d5	9.417	117	400511	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	11.812	152	179313	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.703	65	174878	45.367	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	90.740%
35) Dibromofluoromethane	5.288	113	139122	45.245	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.500%
50) Toluene-d8	7.899	98	525740	47.938	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	95.880%
62) 4-Bromofluorobenzene	10.632	95	190822	45.421	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	90.840%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
Data File : VU049530.D
Acq On : 29 Jun 2022 22:49
Operator : SY/MD
Sample : VU0629WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0629WBL02

Quant Time: Jun 30 00:51:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260
QLast Update : Tue Jun 28 10:35:43 2022
Response via : Initial Calibration




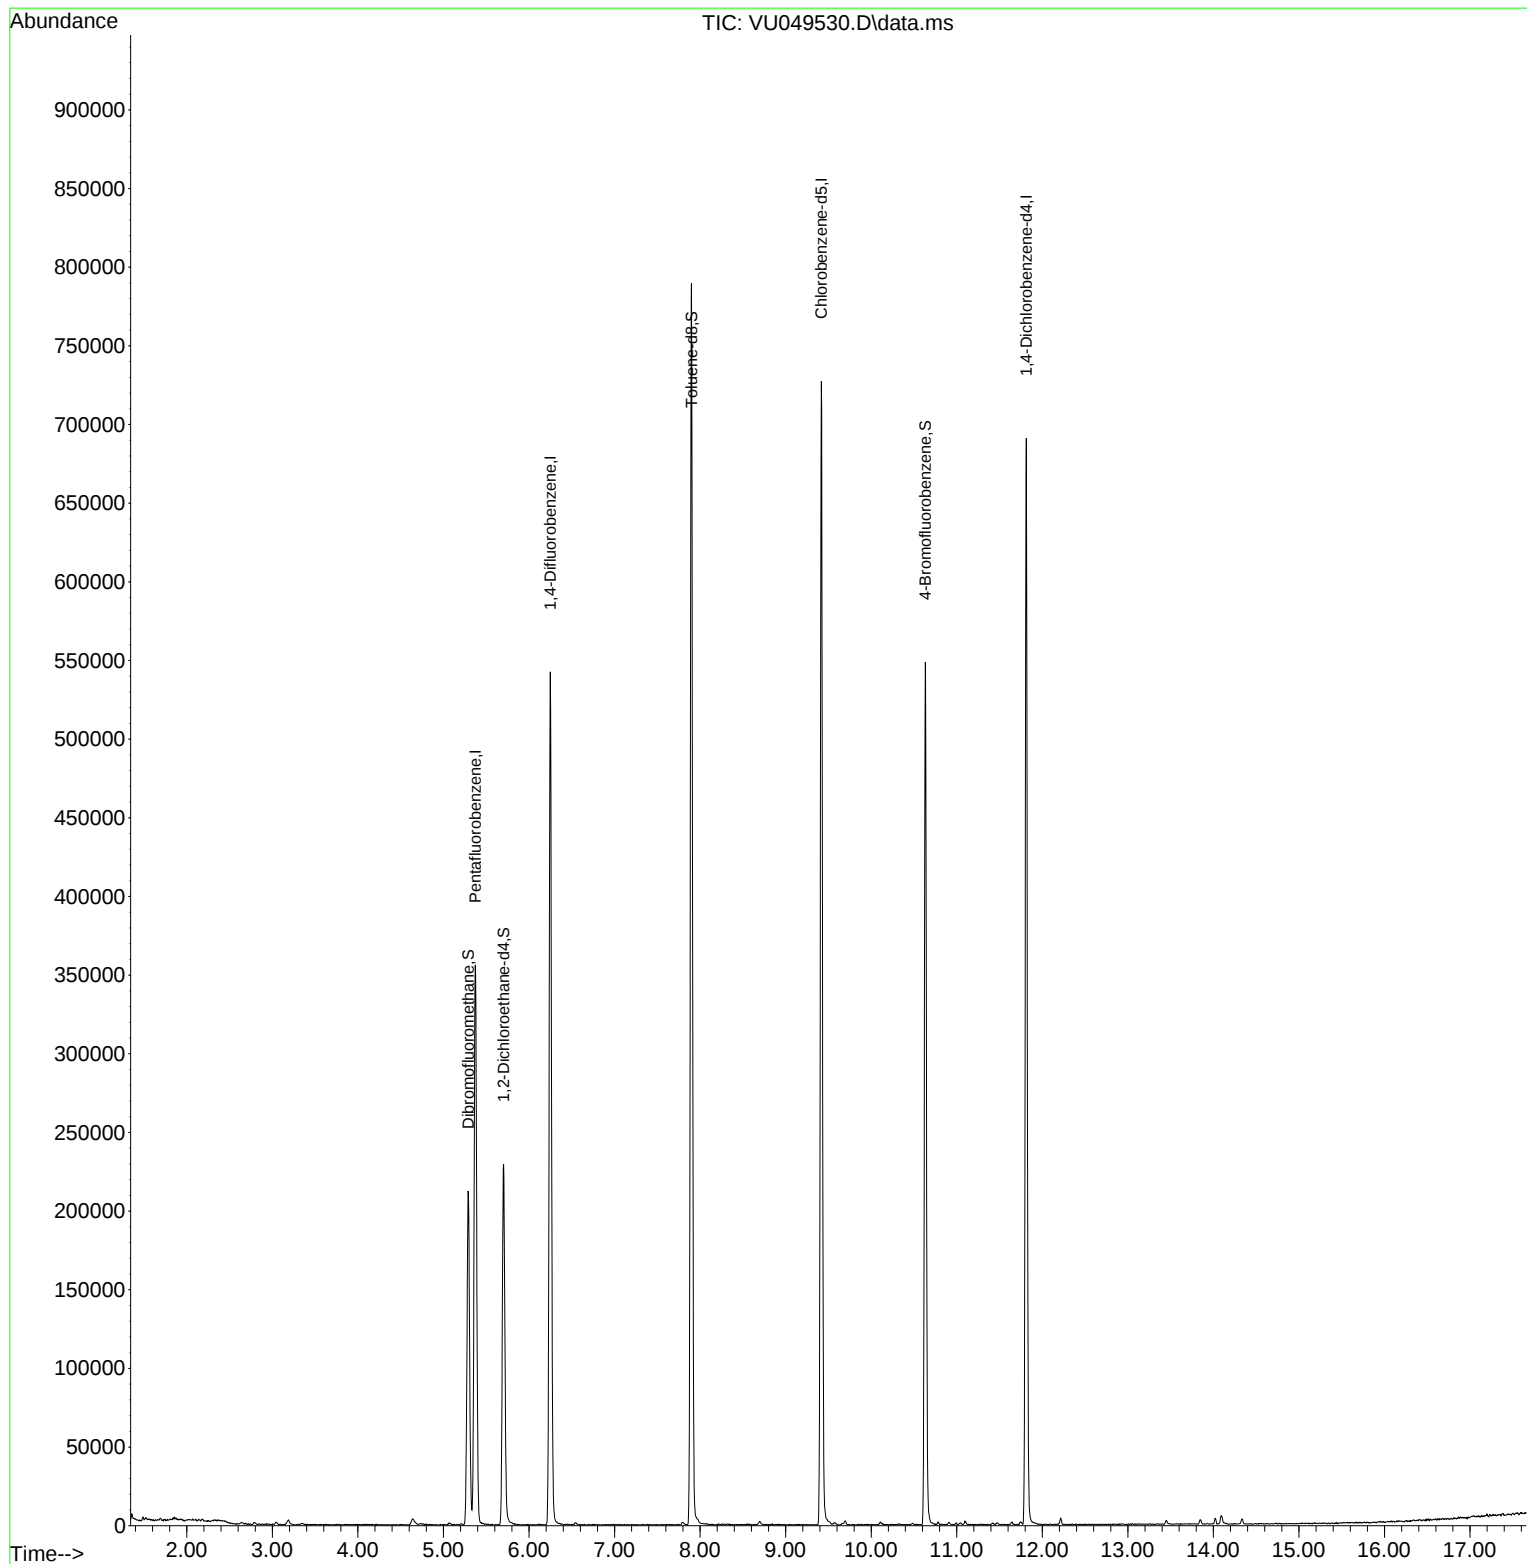


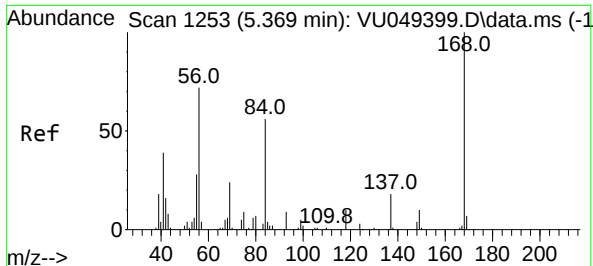

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.372 min Scan# 11
Delta R.T. 0.003 min
Lab File: VU049530.D
Acq: 29 Jun 2022 22:49




Instrument :
MSVOA_U
ClientSampleId :
VU0629WBL02


Tgt Ion:168 Resp: 250298
Ion Ratio Lower Upper
168 100
99 60.4 39.3 58.9#

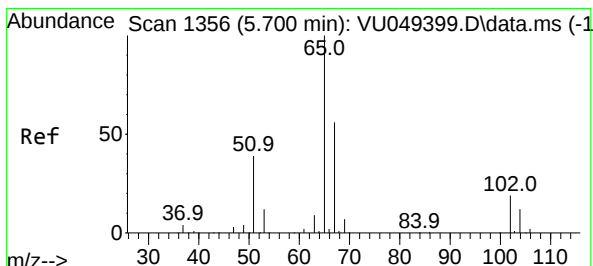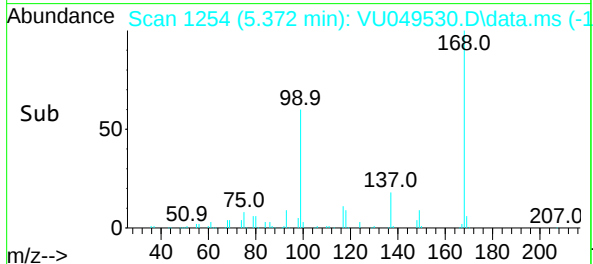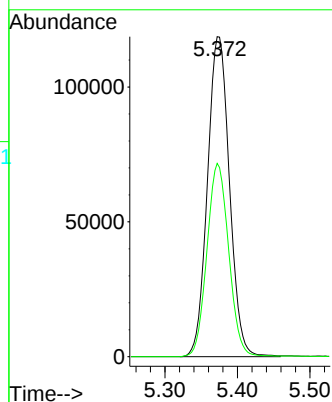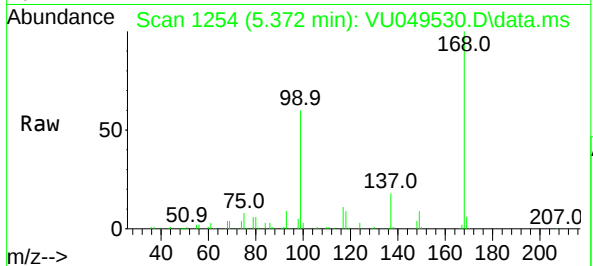

#33
1,2-Dichloroethane-d4
Concen: 45.367 ug/l
RT: 5.703 min Scan# 1357
Delta R.T. 0.003 min
Lab File: VU049530.D
Acq: 29 Jun 2022 22:49

Tgt Ion: 65 Resp: 174878
Ion Ratio Lower Upper
65 100
67 53.3 0.0 108.0

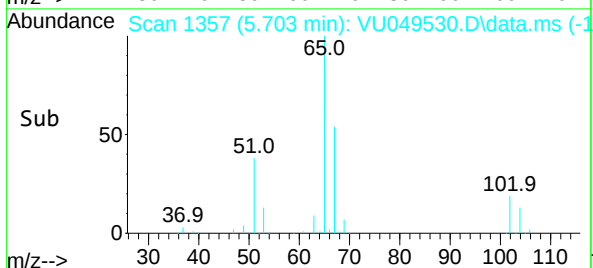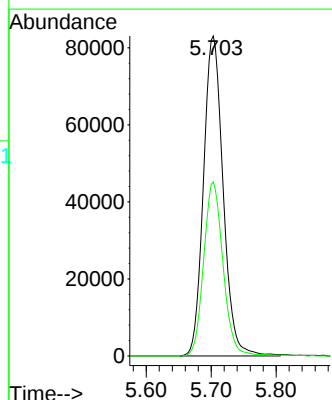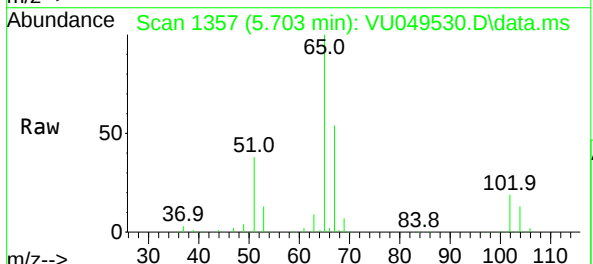

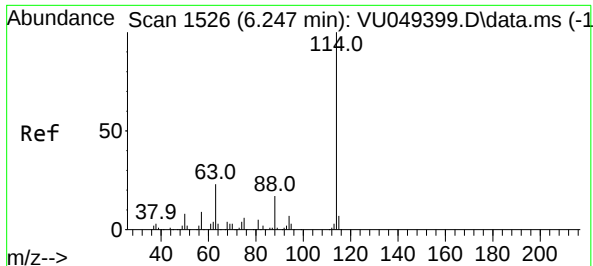

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.250 min Scan# 11

Delta R.T. 0.003 min

Lab File: VU049530.D

Acq: 29 Jun 2022 22:49

Instrument :

MSVOA_U

ClientSampleId :

VU0629WBL02





Tgt Ion:114 Resp: 439498

Ion Ratio Lower Upper

114 100

63 21.8 0.0 37.8

88 16.1 0.0 29.2

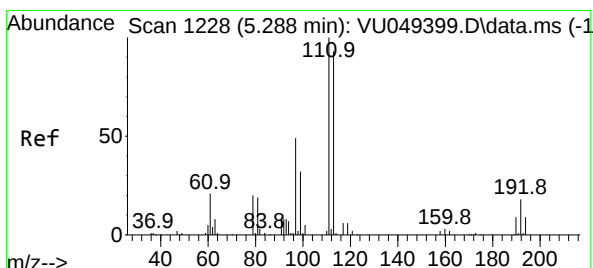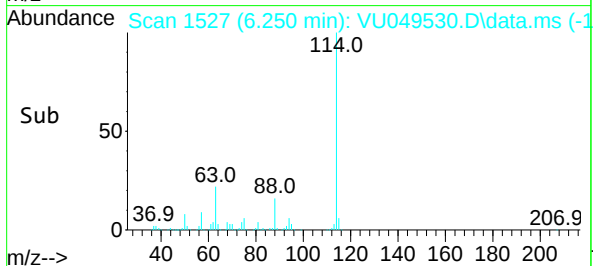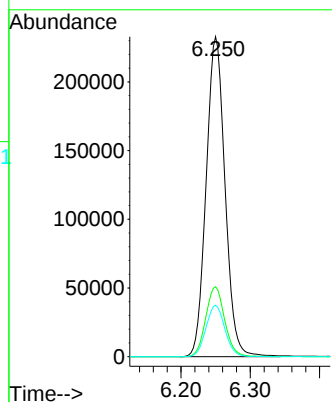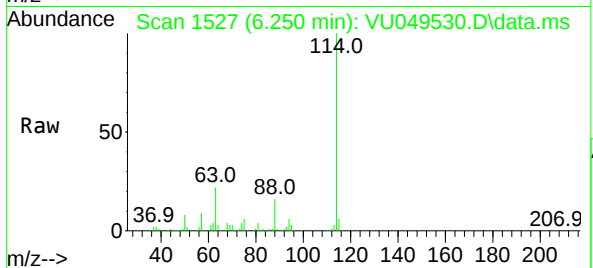

#35

Dibromofluoromethane

Concen: 45.245 ug/l

RT: 5.288 min Scan# 1228

Delta R.T. 0.000 min

Lab File: VU049530.D

Acq: 29 Jun 2022 22:49




Tgt Ion:113 Resp: 139122


Ion Ratio Lower Upper

113 100

111 102.2 82.1 123.1

192 19.0 18.0 27.0


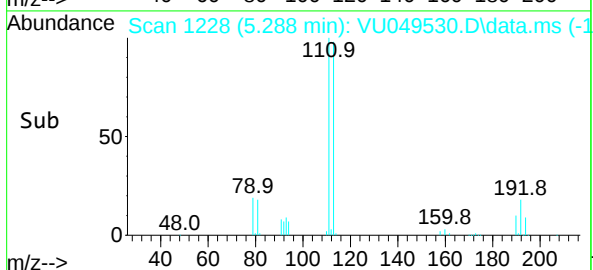
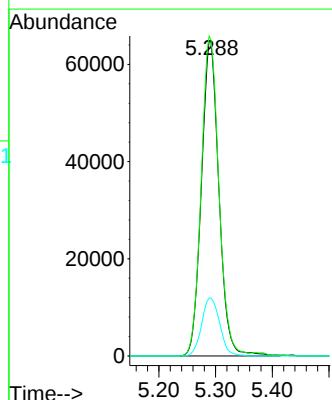
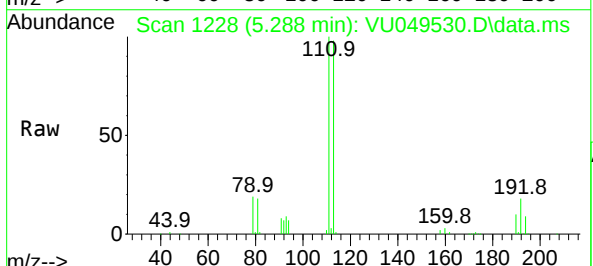


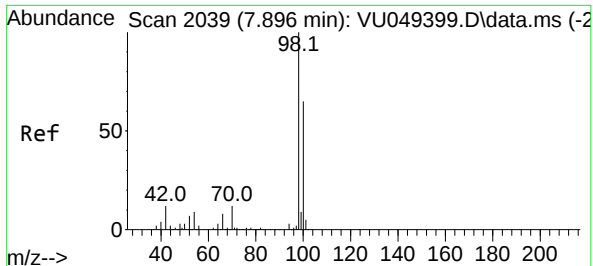

#50
Toluene-d8
Concen: 47.938 ug/l
RT: 7.899 min Scan# 2039
Delta R.T. 0.003 min
Lab File: VU049530.D
Acq: 29 Jun 2022 22:49




Instrument :
MSVOA_U
ClientSampleId :
VU0629WBL02


Tgt Ion: 98 Resp: 525740
Ion Ratio Lower Upper
98 100
100 65.3 51.7 77.5

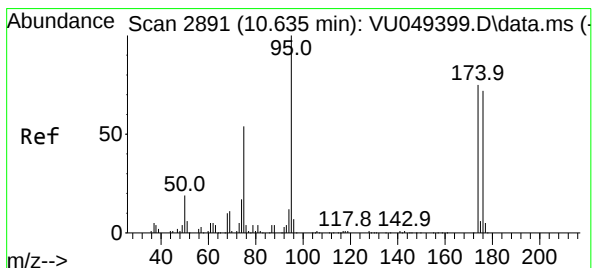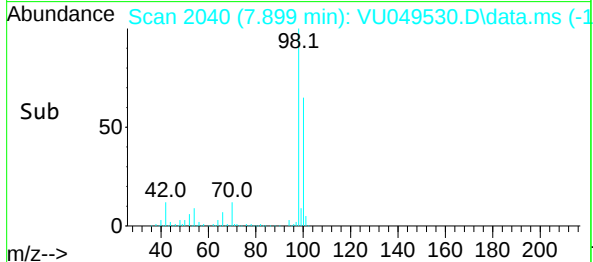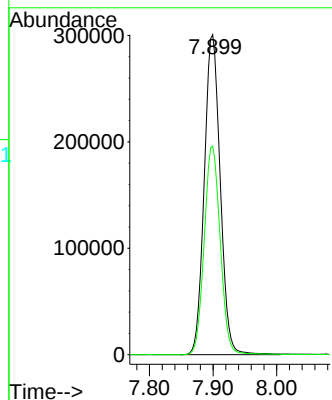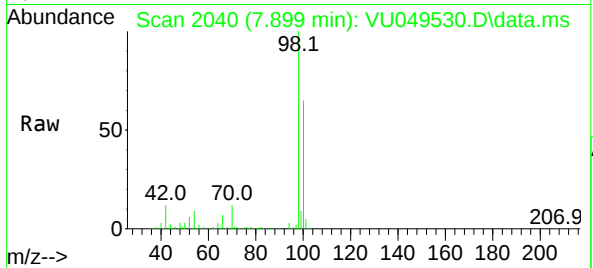

#62
4-Bromofluorobenzene
Concen: 45.421 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.003 min
Lab File: VU049530.D
Acq: 29 Jun 2022 22:49

Tgt Ion: 95 Resp: 190822
Ion Ratio Lower Upper
95 100
174 75.7 0.0 182.0
176 72.6 0.0 177.8


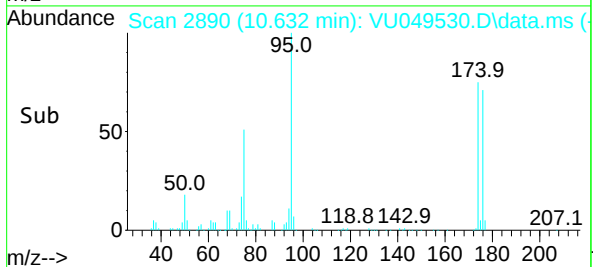
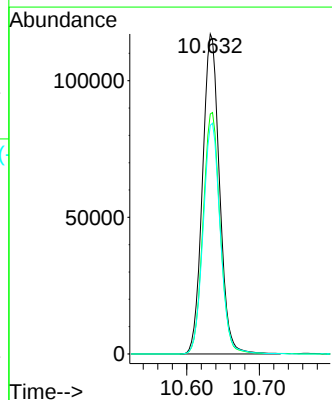
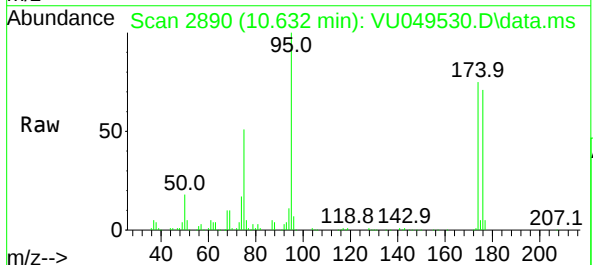


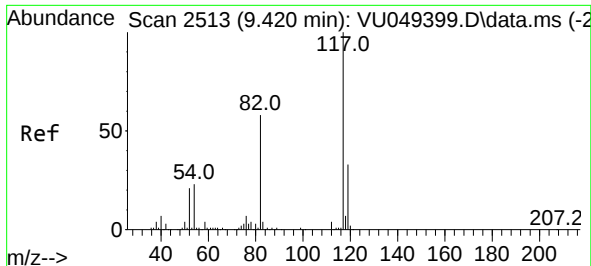

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 9.417 min Scan# 2512
Delta R.T. -0.003 min
Lab File: VU049530.D
Acq: 29 Jun 2022 22:49

Instrument :
MSVOA_U
ClientSampleId :
VU0629WBL02

Tgt Ion:117 Resp: 400511
Ion Ratio Lower Upper
117 100
82 57.5 41.7 62.5
119 32.6 25.7 38.5

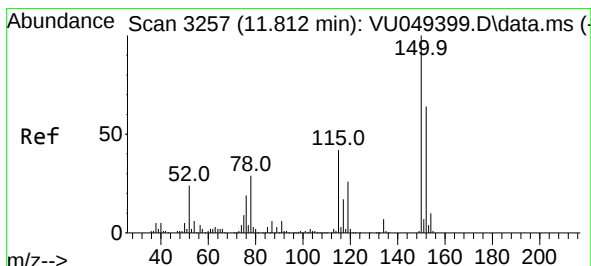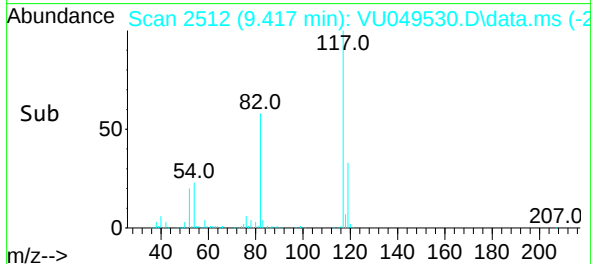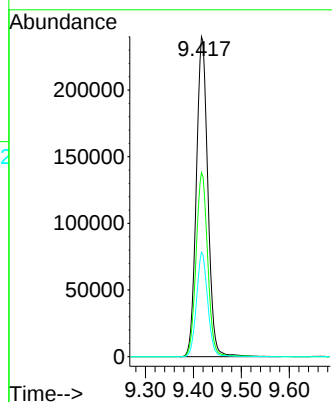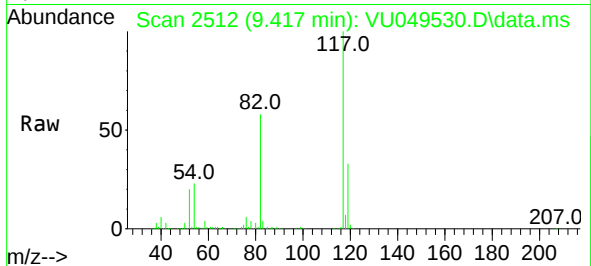

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 11.812 min Scan# 3257
Delta R.T. 0.000 min
Lab File: VU049530.D
Acq: 29 Jun 2022 22:49

Tgt Ion:152 Resp: 179313
Ion Ratio Lower Upper
152 100
115 62.8 37.0 110.9
150 157.8 0.0 342.2

