

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
Data File : VU049521.D
Acq On : 29 Jun 2022 18:18
Operator : SY/MD
Sample : N3457-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP02-20220617

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Title : SW846 8260

Signal : TIC: VU049521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.668	1019	1035	1061	rBV	216087	488715	10.55%	3.592%
2	5.288	1213	1228	1242	rBV	231058	496305	10.72%	3.647%
3	5.372	1242	1254	1274	rVB	399984	817778	17.66%	6.010%
4	5.703	1342	1357	1376	rBV	252312	520052	11.23%	3.822%
5	6.250	1512	1527	1551	rBV	595713	1118718	24.16%	8.222%
6	6.542	1601	1618	1643	rBV	2500088	4630771	100.00%	34.033%
7	7.896	2023	2039	2055	rBV	876585	1513505	32.68%	11.123%
8	8.552	2230	2243	2267	rVB	285472	485010	10.47%	3.564%
9	9.417	2499	2512	2534	rBV	799753	1308045	28.25%	9.613%
10	10.632	2878	2890	2913	rVB	628157	989480	21.37%	7.272%
11	11.812	3244	3257	3277	rBV	776458	1238394	26.74%	9.101%




Sum of corrected areas: 13606773

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
Data File : VU049521.D
Acq On : 29 Jun 2022 18:18
Operator : SY/MD
Sample : N3457-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP02-20220617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

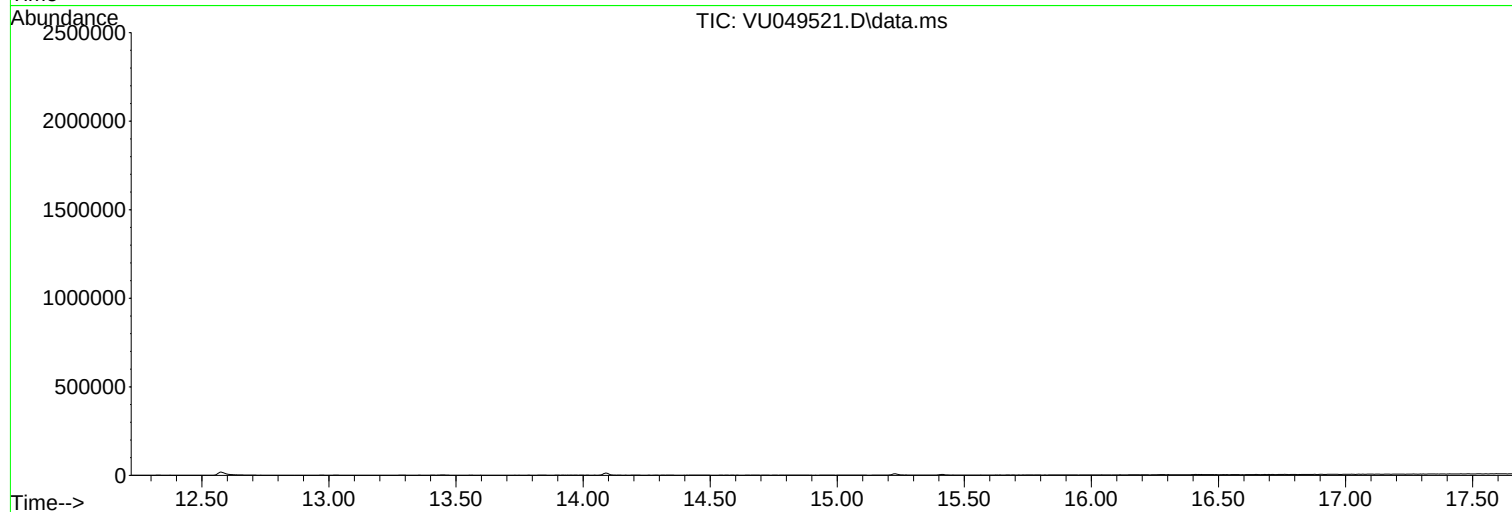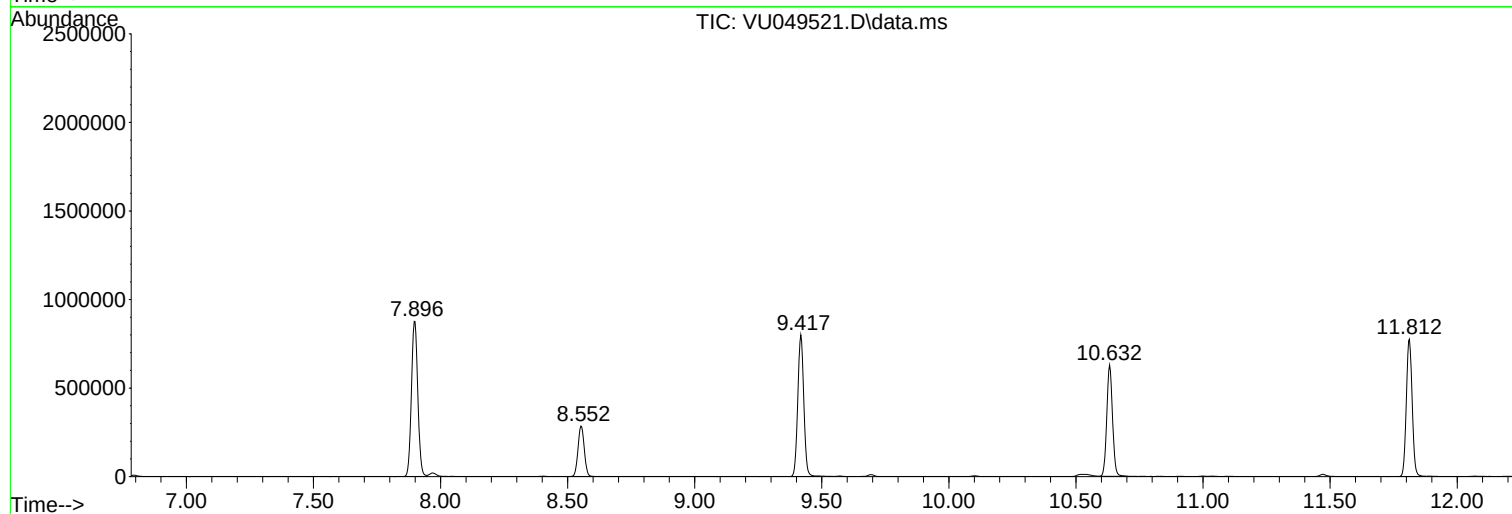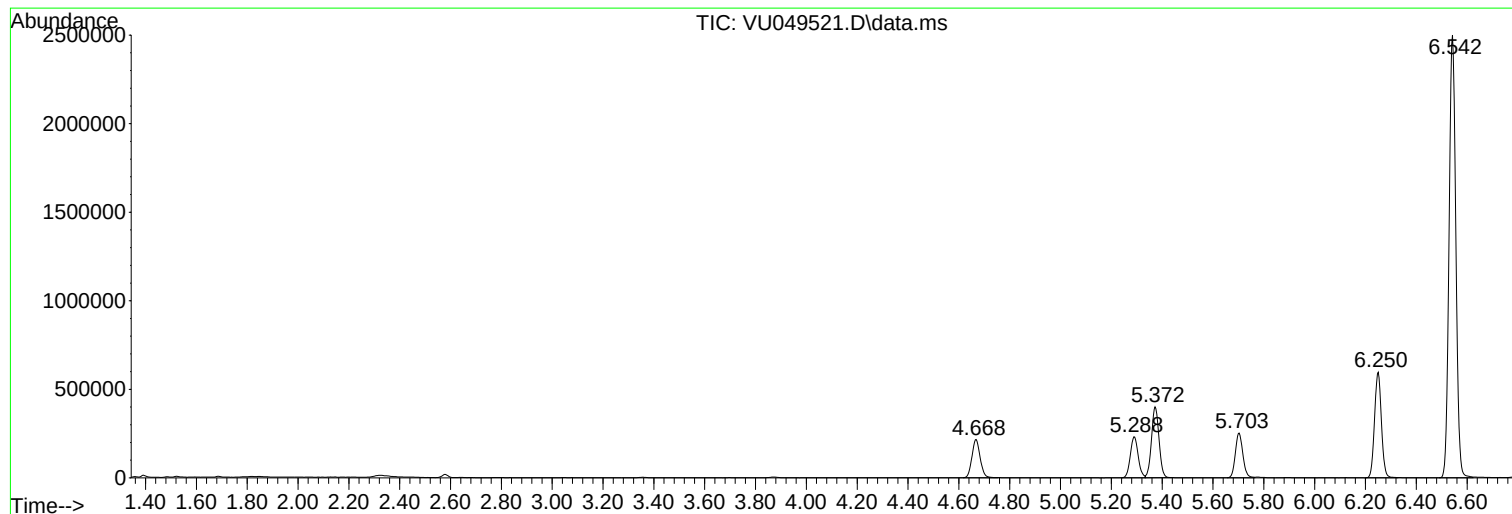

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
Data File : VU049521.D
Acq On : 29 Jun 2022 18:18
Operator : SY/MD
Sample : N3457-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP02-20220617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
Data File : VU049521.D
Acq On : 29 Jun 2022 18:18
Operator : SY/MD
Sample : N3457-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DUP02-20220617

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc