

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
 Data File : VU049534.D
 Acq On : 30 Jun 2022 00:47
 Operator : SY/MD
 Sample : N3517-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 TB-20220627

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M

Title : SW846 8260

Signal : TIC: VU049534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.793	434	452	496	rBV	26594	102880	7.44%	1.365%
2	3.186	558	574	596	rBV2	40746	92817	6.72%	1.232%
3	4.639	1008	1026	1055	rBV	28964	87884	6.36%	1.166%
4	5.288	1213	1228	1241	rBV	213856	450643	32.61%	5.980%
5	5.372	1241	1254	1277	rVB	362644	744019	53.84%	9.873%
6	5.700	1339	1356	1377	rBV	230352	483097	34.96%	6.410%
7	6.247	1511	1526	1549	rBV	537945	1023780	74.08%	13.585%
8	7.896	2026	2039	2060	rBV	798946	1382035	100.00%	18.338%
9	9.417	2498	2512	2540	rBV	724971	1195966	86.54%	15.870%
10	10.632	2877	2890	2919	rBV	549043	883233	63.91%	11.720%
11	11.812	3244	3257	3283	rBV	673713	1089900	78.86%	14.462%




Sum of corrected areas: 7536254

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
Data File : VU049534.D
Acq On : 30 Jun 2022 00:47
Operator : SY/MD
Sample : N3517-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-20220627

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

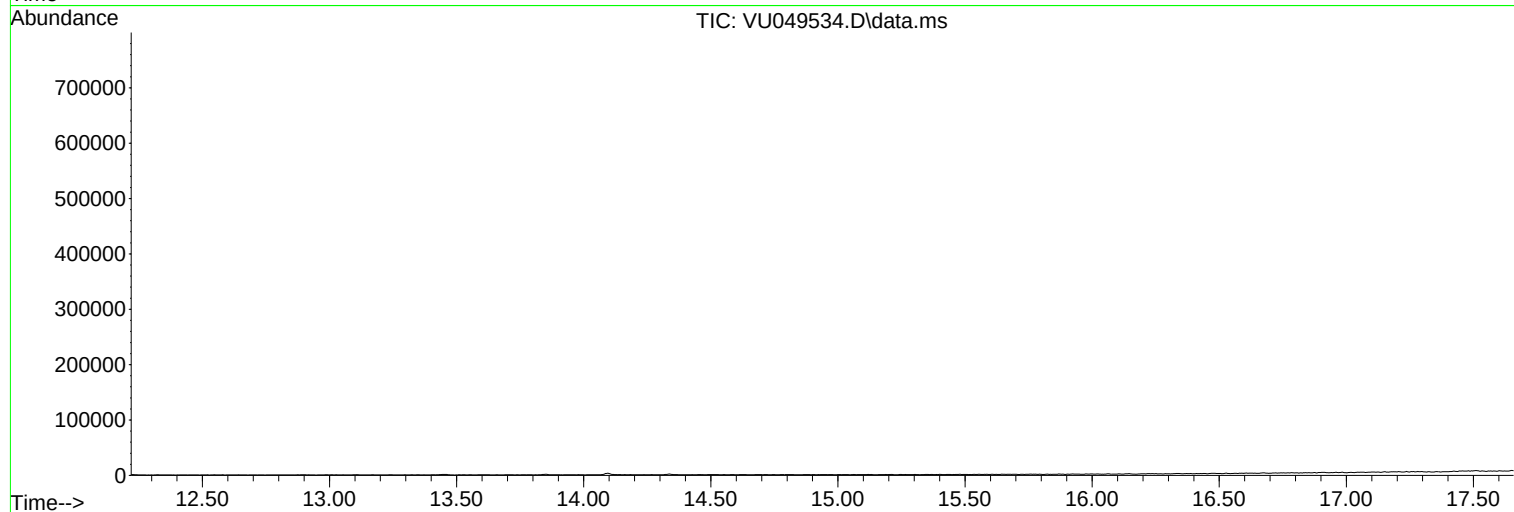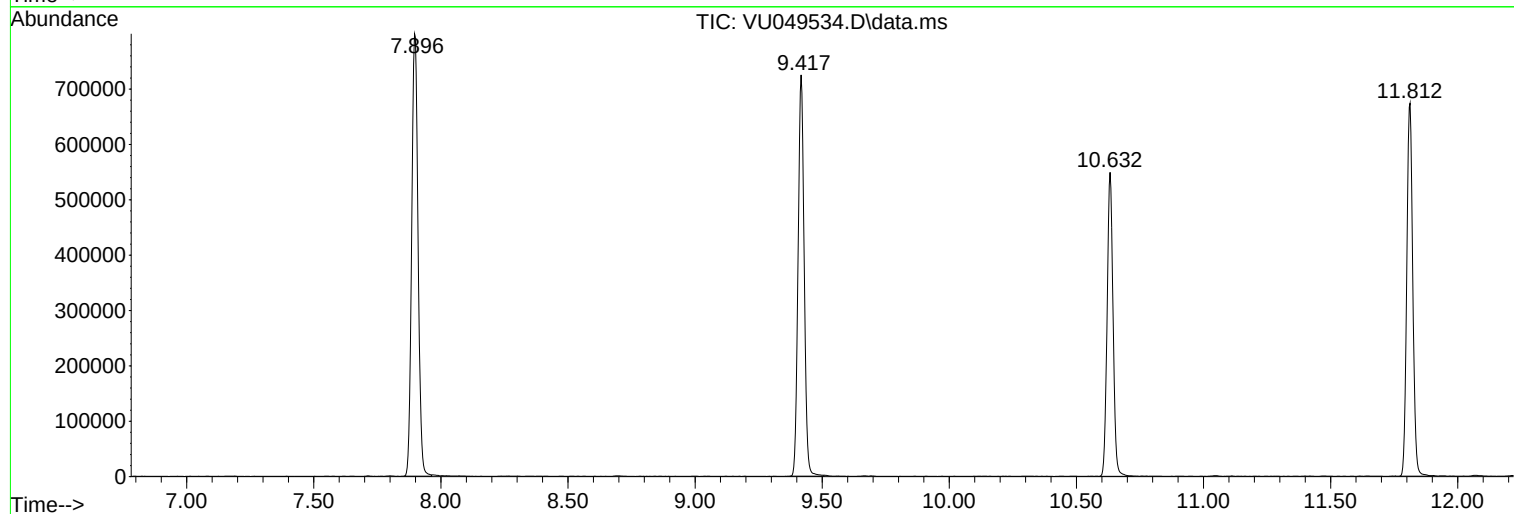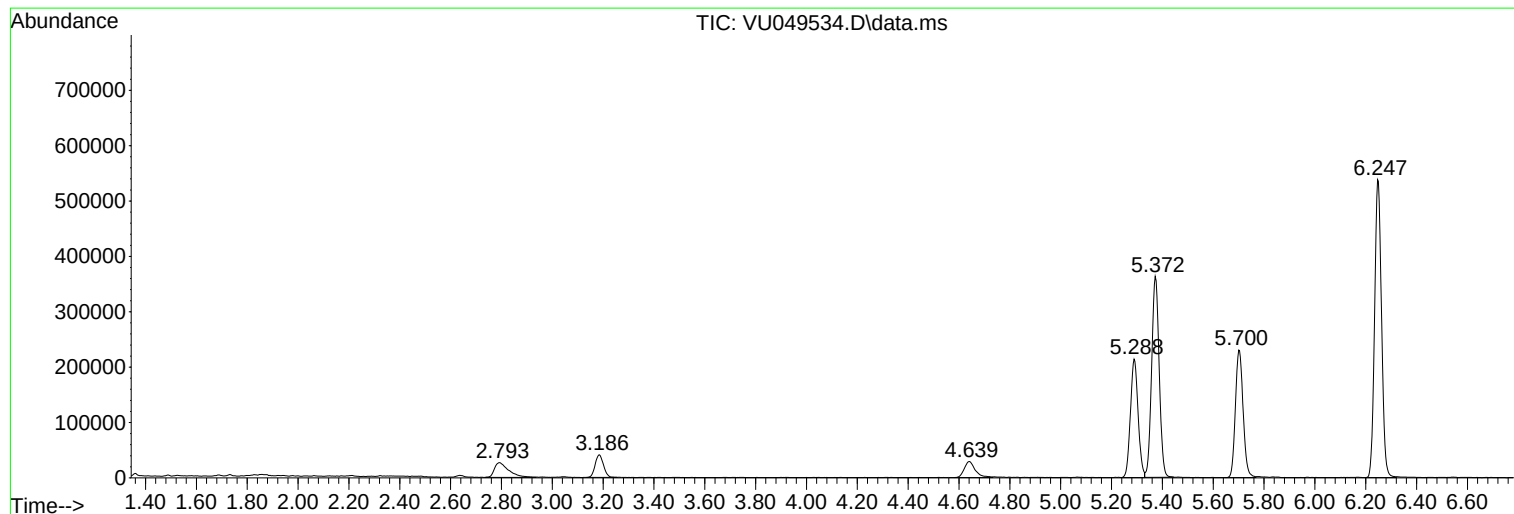

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
Data File : VU049534.D
Acq On : 30 Jun 2022 00:47
Operator : SY/MD
Sample : N3517-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-20220627










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.793	6.91 ug/l	102880	Pentafluorobenzene	5.372

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
2			Propane, 2-ethoxy-	88	C5H12O	000625-54-7	40
3			2-Methyl-4-methoxy-1-butanol	118	C6H14O2	071052-94-3	9
4			2,4-Pentanediol	104	C5H12O2	000625-69-4	9
5			(R)-(-)-2-Pentanol	88	C5H12O	031087-44-2	9

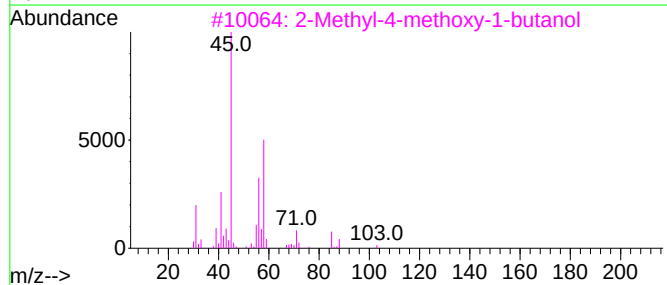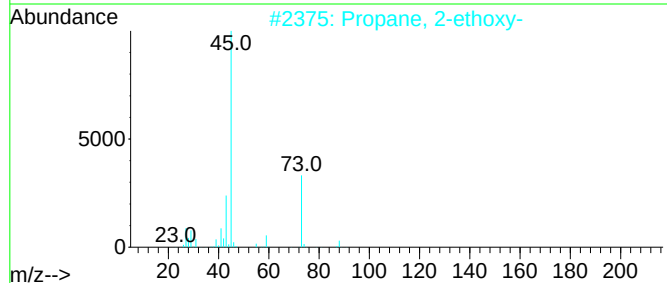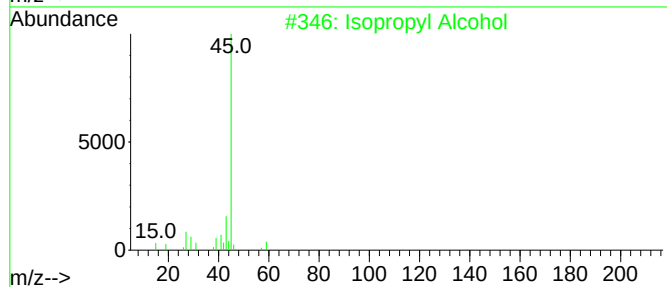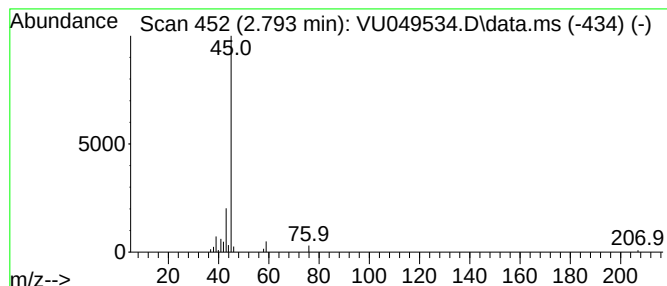

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062922\
Data File : VU049534.D
Acq On : 30 Jun 2022 00:47
Operator : SY/MD
Sample : N3517-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
TB-20220627

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U062722W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.793	6.9	ug/l	102880	1	5.372	744019	50.0