

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062922\  
Data File : VU049537.D  
Acq On : 30 Jun 2022 01:57  
Operator : SY/MD  
Sample : N3505-02  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 40 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
TB-20220624

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U062722W.M

Title : SW846 8260

Signal : TIC: VU049537.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.787       | 437           | 450         | 474          | rBV      | 15620          | 52800         | 3.83%           | 0.724%        |
| 2         | 3.182       | 557           | 573         | 588          | rBV2     | 6954           | 15983         | 1.16%           | 0.219%        |
| 3         | 5.288       | 1211          | 1228        | 1241         | rBV      | 211357         | 451096        | 32.72%          | 6.186%        |
| 4         | 5.372       | 1241          | 1254        | 1278         | rVB      | 358881         | 734684        | 53.29%          | 10.074%       |
| 5         | 5.700       | 1342          | 1356        | 1381         | rBV      | 232316         | 481764        | 34.95%          | 6.606%        |
| 6         | 6.247       | 1512          | 1526        | 1548         | rBV      | 533961         | 1018808       | 73.90%          | 13.970%       |
| 7         | 7.896       | 2024          | 2039        | 2065         | rBV      | 791854         | 1378541       | 100.00%         | 18.903%       |
| 8         | 9.417       | 2498          | 2512        | 2540         | rBV      | 716370         | 1198460       | 86.94%          | 16.434%       |
| 9         | 10.632      | 2877          | 2890        | 2916         | rBV      | 541177         | 876708        | 63.60%          | 12.022%       |
| 10        | 11.812      | 3244          | 3257        | 3284         | rBV      | 682204         | 1083777       | 78.62%          | 14.861%       |




Sum of corrected areas: 7292621

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062922\  
Data File : VU049537.D  
Acq On : 30 Jun 2022 01:57  
Operator : SY/MD  
Sample : N3505-02  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 40 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
TB-20220624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U062722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

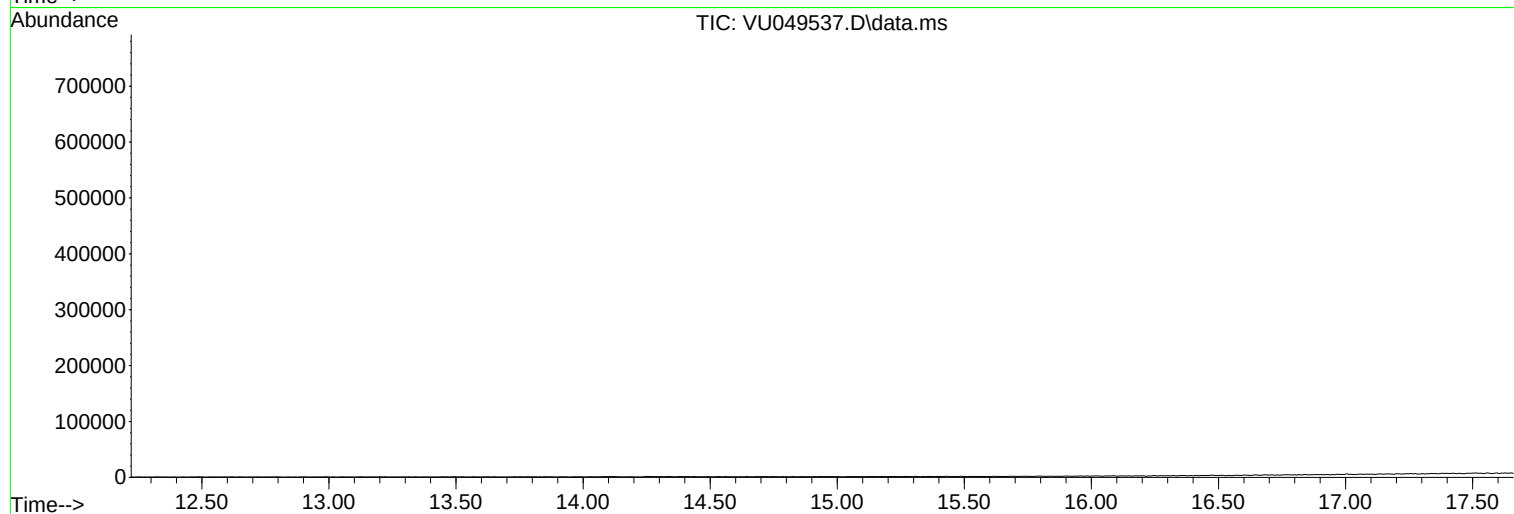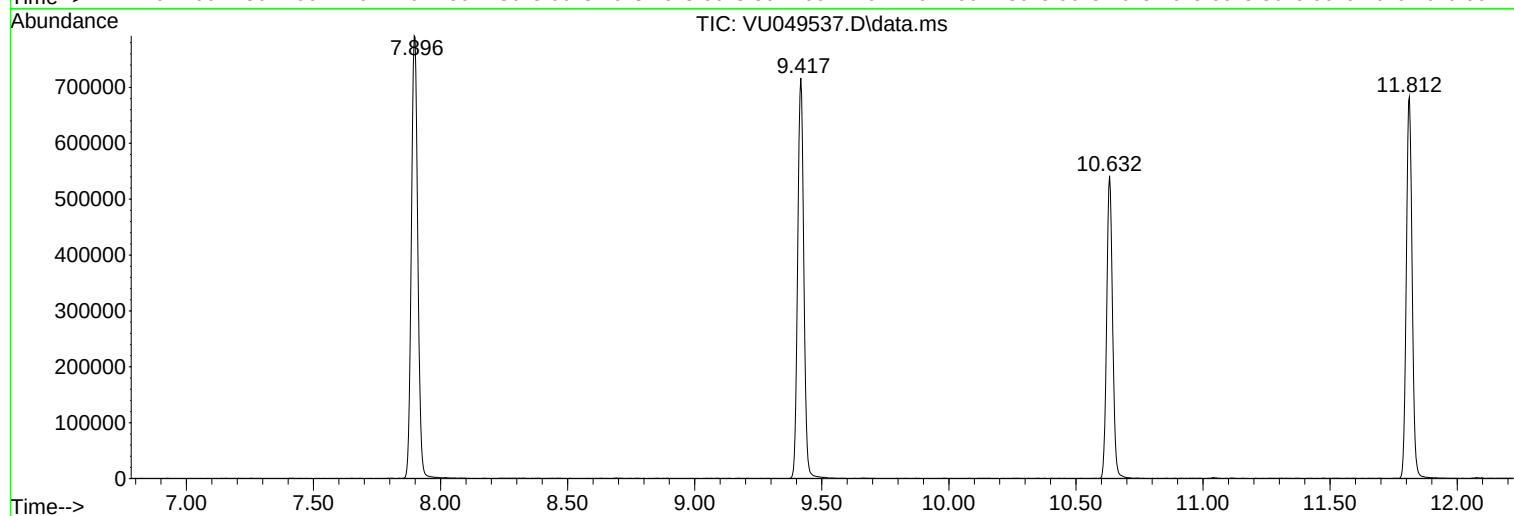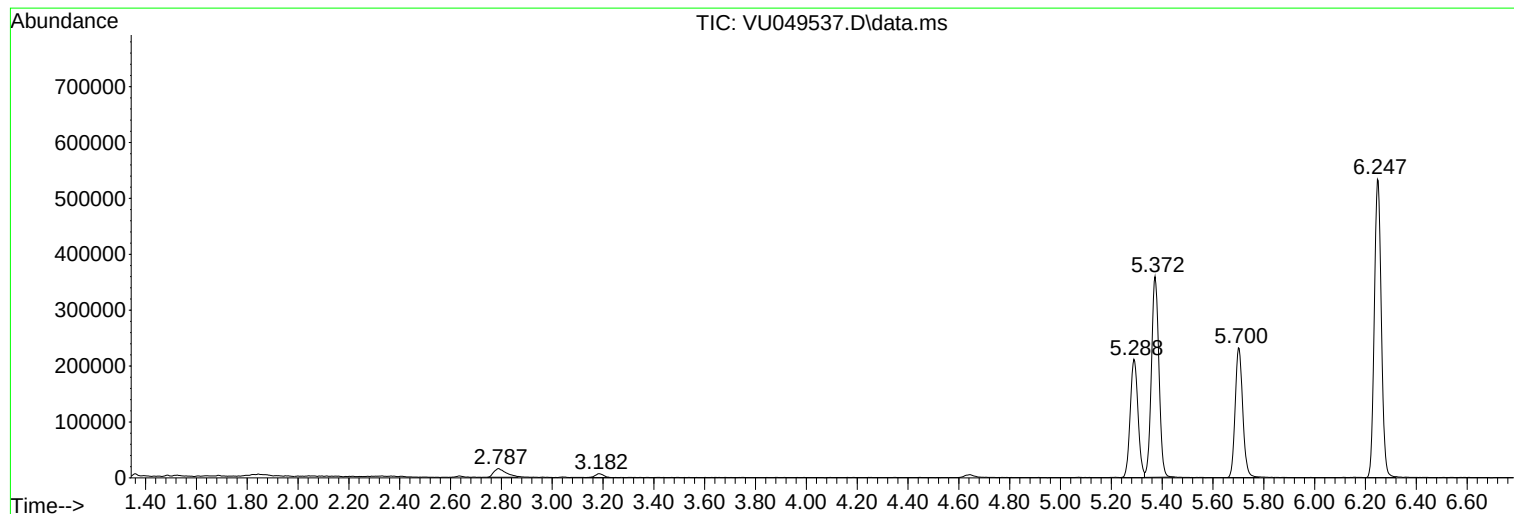

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062922\  
Data File : VU049537.D  
Acq On : 30 Jun 2022 01:57  
Operator : SY/MD  
Sample : N3505-02  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 40 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
TB-20220624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U062722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU062922\  
Data File : VU049537.D  
Acq On : 30 Jun 2022 01:57  
Operator : SY/MD  
Sample : N3505-02  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 40 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
TB-20220624

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U062722W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|