

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062923\
 Data File : VU054692.D
 Acq On : 29 Jun 2023 13:05
 Operator : MD/SY
 Sample : 03457-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0C60

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU054692.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	88	96	110	rBV	117992	143999	14.71%	1.755%
2	1.911	185	193	214	rBV	100109	148412	15.17%	1.809%
3	2.563	384	396	411	rVB	182633	296550	30.30%	3.615%
4	3.181	577	588	603	rVB2	9273	20478	2.09%	0.250%
5	4.631	1024	1039	1069	rBV	142196	417704	42.68%	5.091%
6	5.059	1153	1172	1201	rBV	192607	448381	45.82%	5.465%
7	5.721	1358	1378	1412	rBV2	353043	929916	95.02%	11.335%
8	6.245	1526	1541	1566	rBV	379076	744165	76.04%	9.071%
9	6.689	1664	1679	1697	rBV	221347	447715	45.75%	5.457%
10	7.563	1938	1951	1969	rBV	111055	203565	20.80%	2.481%
11	7.894	2040	2054	2070	rBV	400440	704376	71.98%	8.586%
12	8.177	2130	2142	2161	rBV2	66047	117412	12.00%	1.431%
13	8.631	2270	2283	2309	rBV2	494325	978610	100.00%	11.928%
14	9.412	2511	2526	2548	rBV	531099	901845	92.16%	10.993%
15	9.692	2602	2613	2624	rBV2	11150	18394	1.88%	0.224%
16	10.100	2732	2740	2752	rBV6	5915	9839	1.01%	0.120%
17	10.753	2930	2943	2959	rBV	160907	263533	26.93%	3.212%
18	11.807	3259	3271	3287	rBV	505362	806759	82.44%	9.834%
19	12.190	3377	3390	3412	rBV	361117	602381	61.55%	7.342%




Sum of corrected areas: 8204034

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062923\
Data File : VU054692.D
Acq On : 29 Jun 2023 13:05
Operator : MD/SY
Sample : 03457-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

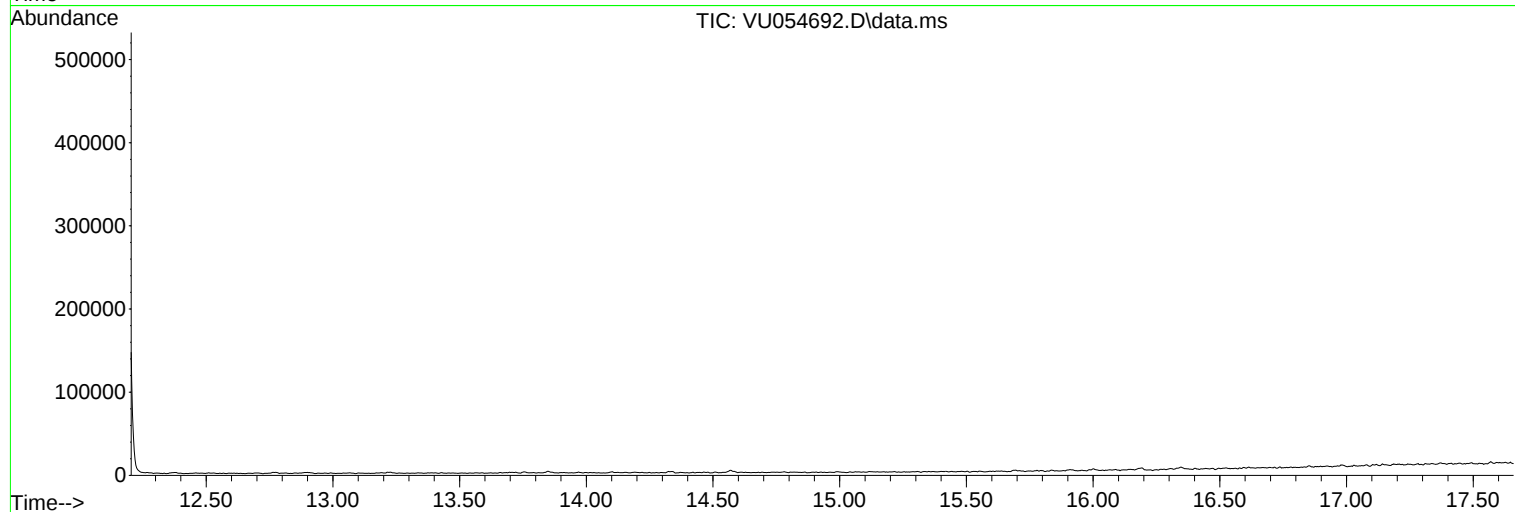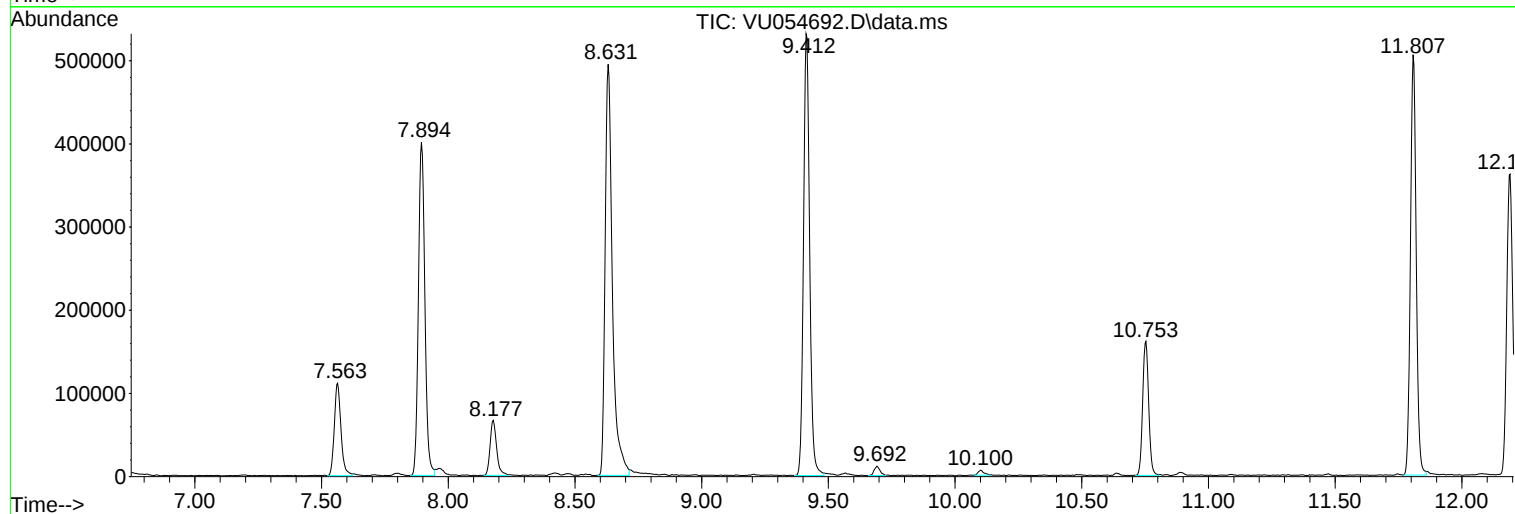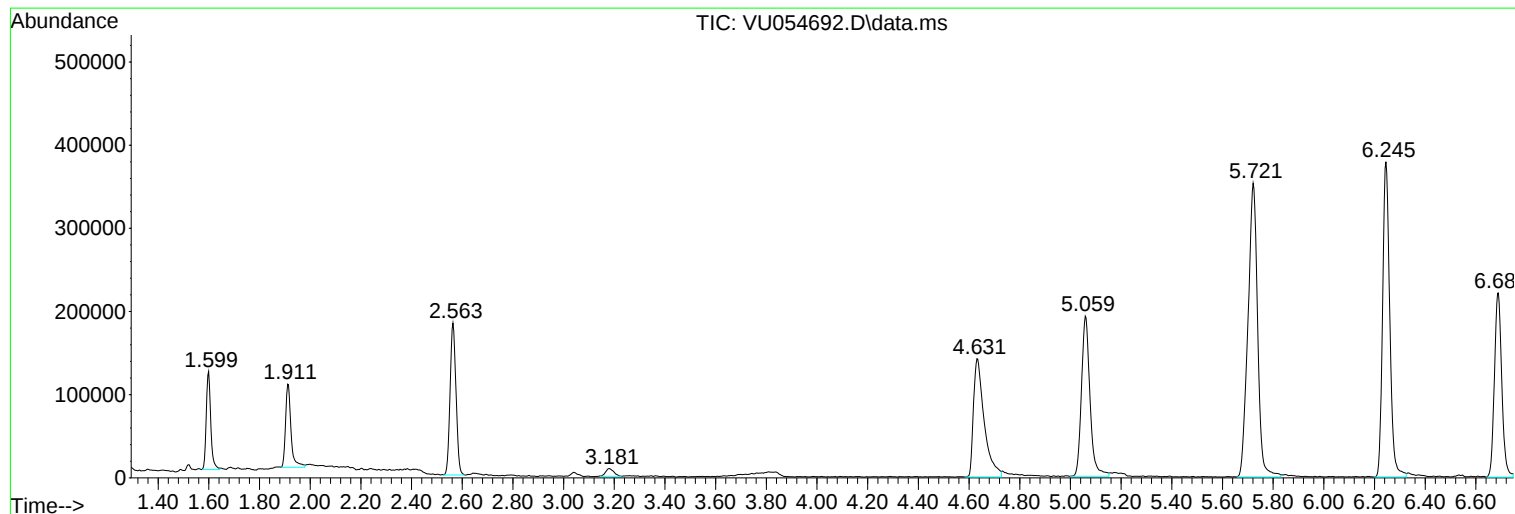

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062923\
Data File : VU054692.D
Acq On : 29 Jun 2023 13:05
Operator : MD/SY
Sample : 03457-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062923\
Data File : VU054692.D
Acq On : 29 Jun 2023 13:05
Operator : MD/SY
Sample : 03457-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0C60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------