


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062923\
Data File : VU054687.D
Acq On : 29 Jun 2023 09:19
Operator : MD/SY
Sample : BFB027
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB027

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR060723WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jun 23 23:55:46 2023

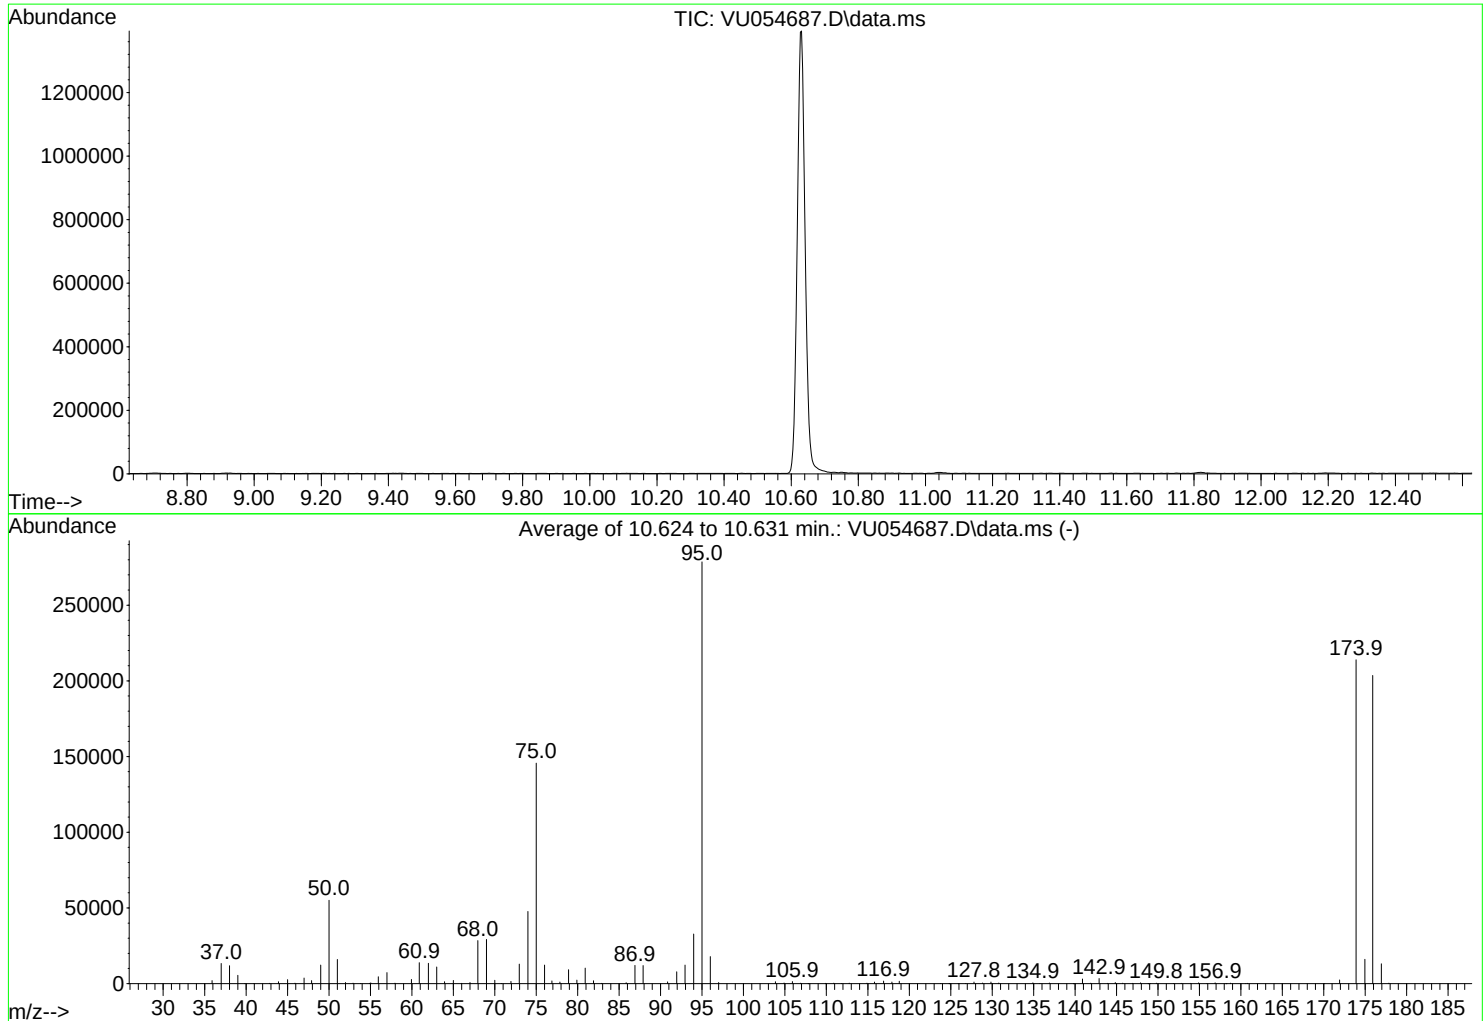

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	55056	PASS
75	95	30	80	52.3	145643	PASS
95	95	100	100	100.0	278613	PASS
96	95	5	9	6.4	17875	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.8	213973	PASS
175	174	5	9	7.5	16016	PASS
176	174	95	101	95.1	203563	PASS
177	176	5	9	6.5	13145	PASS

m/z	Abundance
35.80	102.0
39.80	409.0
43.90	897.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
36.00	1892.0
37.00	12910.0
38.00	11602.0
39.00	5050.0
39.90	561.0
40.90	156.0
42.90	248.0
44.00	2269.0
45.00	2295.0
45.90	344.0
47.00	3778.0
47.90	1998.0
49.00	11539.0
50.00	51632.0
51.00	14728.0
52.00	755.0
52.90	264.0
53.80	133.0
54.90	583.0
55.90	4456.0
57.00	6943.0
58.00	331.0
60.00	2326.0
60.90	13244.0
62.00	12254.0
63.00	10516.0
64.00	1293.0
65.00	1870.0
66.00	258.0
67.00	825.0
68.00	26952.0
69.00	27792.0
70.00	2136.0
70.80	155.0
71.90	1430.0
73.00	12240.0
74.00	44984.0
75.00	138432.0
76.00	12138.0
76.90	1815.0
77.80	887.0
78.90	8704.0
79.90	2274.0
80.90	9897.0
81.90	1857.0
83.00	220.0
85.80	557.0
86.90	11017.0
87.90	11217.0
90.90	1146.0
92.00	7410.0
92.90	11255.0
94.00	30912.0
95.00	260608.0
96.00	16480.0
97.00	704.0
103.80	1179.0
104.90	426.0
105.90	1211.0
106.90	253.0
109.90	229.0
110.90	239.0
111.90	159.0
112.70	311.0
114.90	358.0
115.80	960.0
116.90	1797.0
117.90	1017.0
118.80	1462.0
123.80	159.0
126.80	148.0
127.80	916.0
128.90	348.0
129.90	927.0
130.80	447.0
134.90	464.0
135.70	113.0
136.90	360.0
140.90	2696.0
141.90	269.0
142.90	3314.0
143.90	203.0
145.00	674.0
145.70	315.0
147.00	174.0
147.90	541.0
149.10	101.0
149.80	222.0
151.80	117.0
152.80	211.0
153.90	116.0
154.90	496.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

156.90	535.0
158.70	308.0
160.60	257.0
170.10	120.0
171.90	2251.0
173.90	195136.0
175.00	14840.0
175.90	185280.0
176.90	12412.0
177.90	347.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
35.90	2127.0
37.00	13771.0
38.00	12086.0
39.00	5627.0
39.90	574.0
41.00	173.0
42.80	249.0
43.90	2182.0
45.00	2752.0
45.90	356.0
47.00	3755.0
47.90	2053.0
49.00	12671.0
50.00	57112.0
51.00	16424.0
52.00	812.0
52.90	296.0
53.80	102.0
55.10	693.0
55.90	4667.0
57.00	7346.0
58.00	317.0
59.90	2832.0
60.90	14326.0
62.00	13807.0
63.00	11349.0
64.00	1345.0
65.00	2173.0
66.00	275.0
67.00	779.0
68.00	29144.0
69.00	30256.0
70.00	2261.0
70.80	179.0
71.90	1489.0
72.90	13322.0
74.00	49216.0
75.00	150400.0
76.00	12564.0
76.90	1940.0
77.90	1027.0
78.90	9500.0
79.90	2290.0
80.90	10720.0
81.90	1977.0
82.80	287.0
85.90	722.0
86.90	12616.0
87.90	12334.0
90.90	1242.0
91.90	8201.0
93.00	12595.0
94.00	33824.0
95.00	288064.0
96.00	18576.0
97.00	808.0
103.90	1291.0
104.90	486.0
105.90	1379.0
106.90	307.0
109.90	276.0
110.90	312.0
111.80	155.0
112.80	337.0
114.90	396.0
115.80	1077.0
116.90	1741.0
117.90	1195.0
118.80	1683.0
123.80	190.0
126.80	126.0
127.80	1067.0
128.80	463.0
129.80	1072.0
130.80	436.0
134.90	540.0
135.70	139.0
136.90	443.0
139.80	172.0
140.90	3158.0
141.90	341.0
142.90	3433.0
143.90	221.0
144.80	787.0
145.70	356.0
147.00	210.0
147.90	575.0
149.00	110.0
149.80	303.0
151.90	184.0
152.80	213.0
154.00	197.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

154.90	506.0
155.90	121.0
156.90	599.0
158.70	355.0
160.80	259.0
170.10	160.0
171.90	2511.0
173.90	221568.0
175.00	16576.0
175.90	209536.0
177.00	13643.0
177.90	388.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

m/z	Abundance
35.90	2326.0
37.00	13295.0
38.00	11774.0
39.00	5853.0
39.90	468.0
41.00	150.0
42.80	254.0
43.90	2159.0
45.00	2902.0
45.90	381.0
47.00	3732.0
47.90	1858.0
49.00	12644.0
50.00	56424.0
51.00	16888.0
52.00	792.0
52.90	262.0
55.00	810.0
56.00	4425.0
57.00	7475.0
57.90	291.0
59.90	3114.0
60.90	14013.0
62.00	14191.0
63.00	11147.0
63.90	1246.0
65.00	2198.0
66.00	269.0
67.00	688.0
67.90	29160.0
69.00	29536.0
70.00	2269.0
70.80	139.0
72.00	1464.0
72.90	13119.0
74.00	48928.0
75.00	148096.0
76.00	12182.0
76.90	1797.0
77.90	1190.0
78.90	9399.0
79.90	2302.0
80.90	10324.0
81.90	1929.0
82.90	298.0
85.90	704.0
86.90	12493.0
87.90	12181.0
90.80	1202.0
92.00	8046.0
93.00	12882.0
94.00	33472.0
95.00	287168.0
96.00	18568.0
97.00	701.0
103.90	1291.0
104.90	474.0
105.90	1431.0
106.90	288.0
107.80	103.0
109.90	271.0
110.90	368.0
111.80	177.0
112.80	340.0
114.90	387.0
115.80	1034.0
116.90	1686.0
117.90	1137.0
118.80	1637.0
123.80	176.0
124.80	136.0
125.90	104.0
127.80	1087.0
128.80	543.0
129.80	1049.0
130.80	396.0
134.90	607.0
135.80	126.0
136.90	590.0
140.90	3315.0
141.90	364.0
142.90	3354.0
143.90	188.0
144.80	855.0
145.80	338.0
146.90	216.0
147.90	554.0
148.80	158.0
149.80	333.0
151.90	217.0
152.80	243.0
154.00	254.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027

154.90	560.0
155.90	112.0
156.90	538.0
158.20	105.0
158.80	385.0
160.80	269.0
170.00	142.0
171.90	2471.0
173.90	225216.0
174.90	16632.0
175.90	215872.0
177.00	13380.0
177.80	398.0

Instrument :
MSVOA_U
ClientSampleId :
BFB027