




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059623.D
Acq On : 28 Jun 2024 16:17
Operator : MD/SY
Sample : P3059-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM3

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:57:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

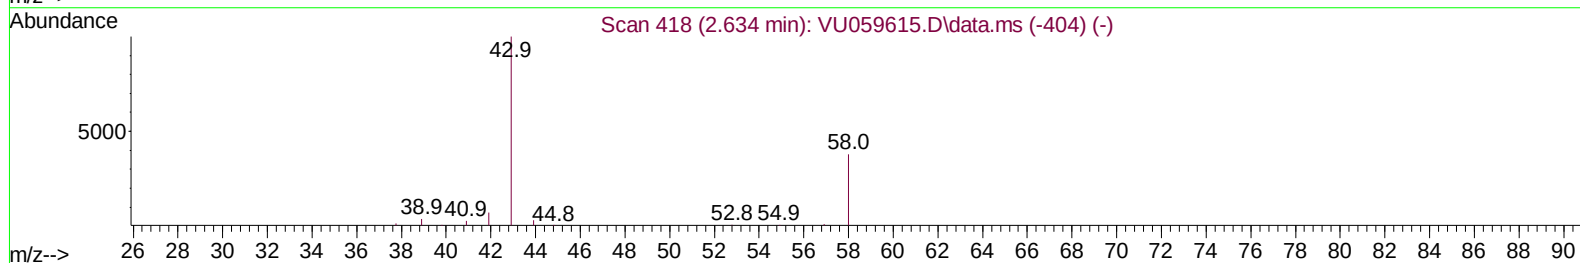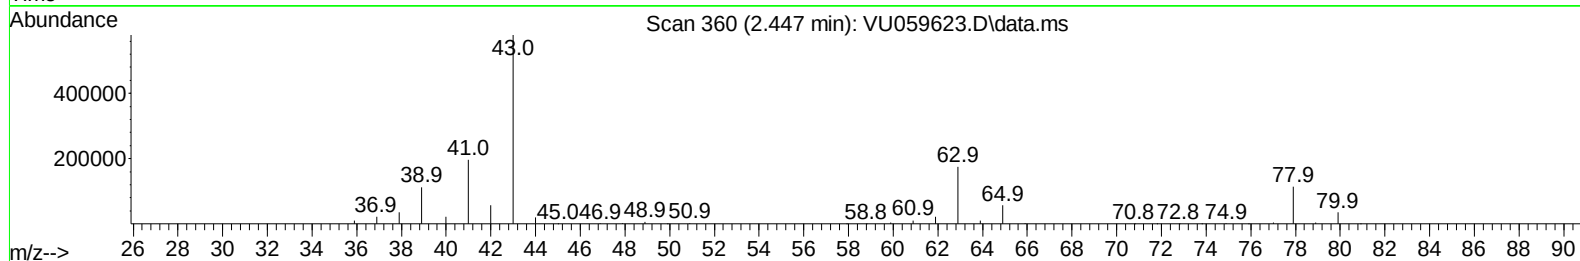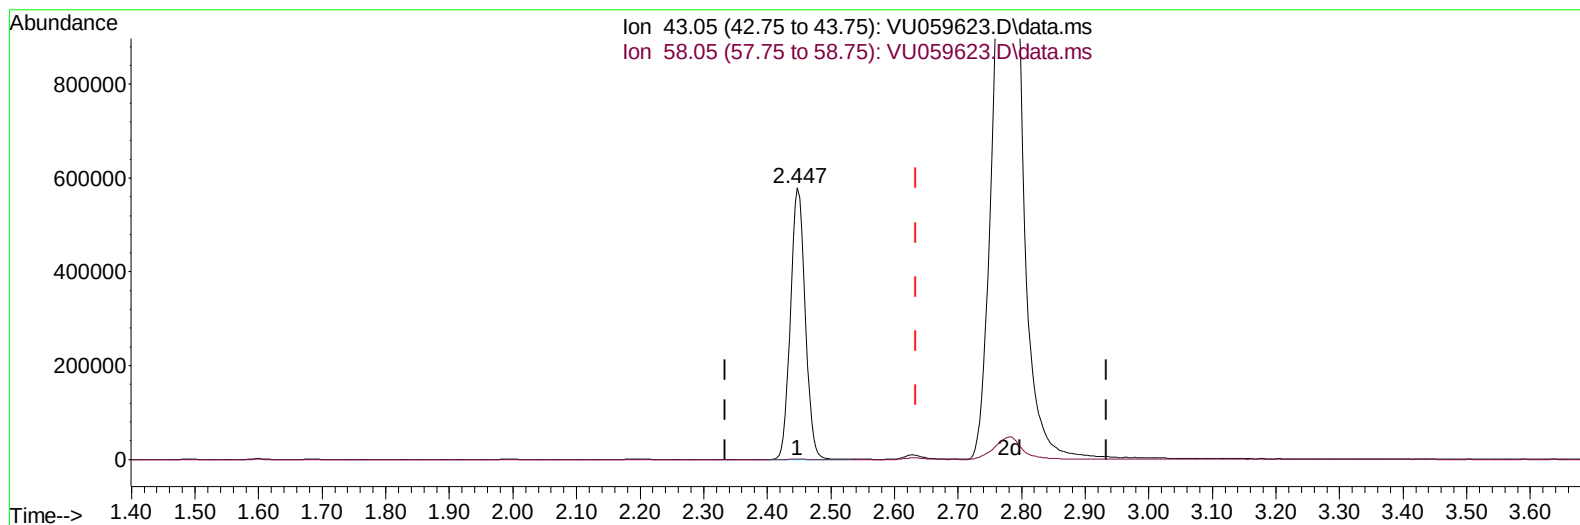

TIC: VU059623.D\data.ms

(13) Acetone (T)

2.447min (-0.187) 707.23 ug/L

response 930998

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	0.80
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059623.D
Acq On : 28 Jun 2024 16:17
Operator : MD/SY
Sample : P3059-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM3

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:57:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

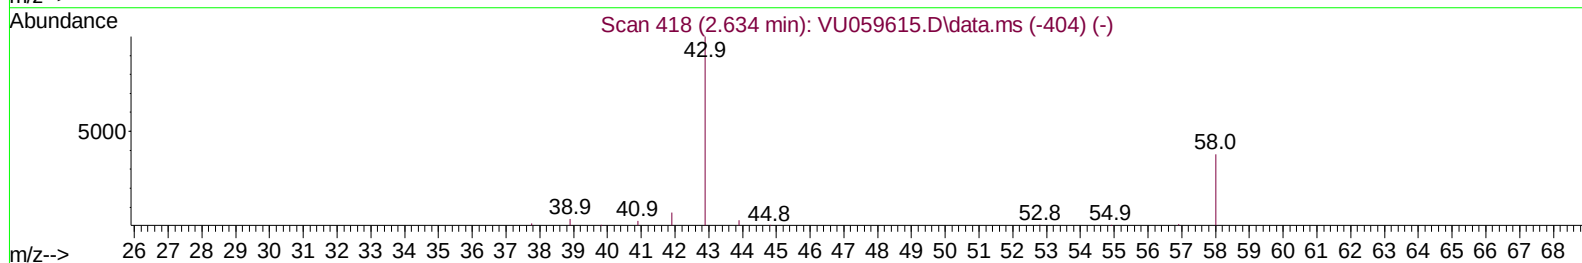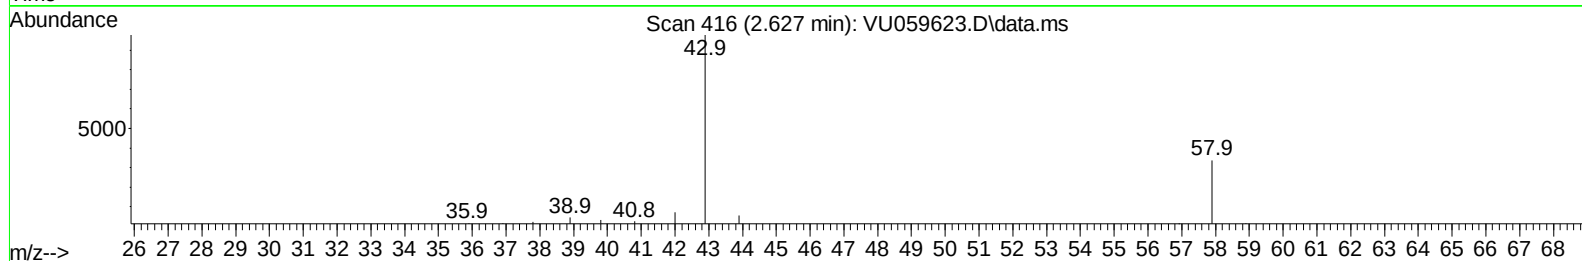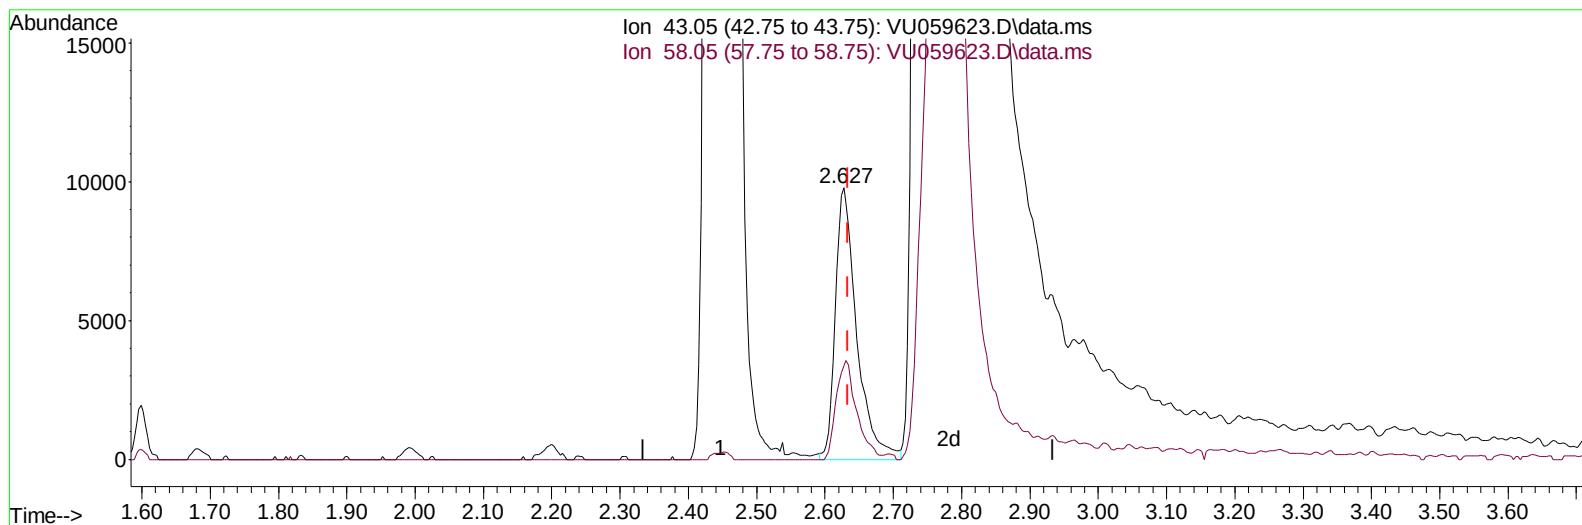

TIC: VU059623.D\data.ms

(13) Acetone (T)

2.627min (-0.007) 16.19 ug/L m

response 21309

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	34.92
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059623.D
 Acq On : 28 Jun 2024 16:17
 Operator : MD/SY
 Sample : P3059-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GM3

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:57:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 28 23:55:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		141681	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		149000	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		66034	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		35348	3.588	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	71.800%	
7) Chloroethane-d5	1.907	69		38161	4.026	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	80.600%	
11) 1,1-Dichloroethene-d2	2.560	65		16403	4.013	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	80.200%	
20) 2-Butanone-d5	4.621	46		100555	49.551	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	99.100%	
24) Chloroform-d	5.055	84		90221	4.462	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	89.200%	
26) 1,2-Dichloroethane-d4	5.695	65		43625	4.479	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	89.600%	
32) Benzene-d6	5.721	84		175771	4.286	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	85.800%	
36) 1,2-Dichloropropane-d6	6.682	67		56324	4.482	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	89.600%	
41) Toluene-d8	7.894	98		145827	3.825	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	76.600%	
43) trans-1,3-Dichloroprop...	8.177	79		17006	4.322	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	86.400%	
46) 2-Hexanone-d5	8.627	63		76924	47.052	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	94.100%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		47434	4.569	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	91.400%	
66) 1,2-Dichlorobenzene-d4	12.190	152		57844	4.922	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	98.400%	
Target Compounds							
13) Acetone	2.627	43		21309m	16.187	ug/L	
18) trans-1,2-Dichloroethene	3.345	96		5189	0.497	ug/L	84
22) cis-1,2-Dichloroethene	4.663	96		9852	0.855	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059623.D
Acq On : 28 Jun 2024 16:17
Operator : MD/SY
Sample : P3059-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM3

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:57:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

