




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059624.D
 Acq On : 28 Jun 2024 16:41
 Operator : MD/SY
 Sample : P3059-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GM4

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:58:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 28 23:55:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

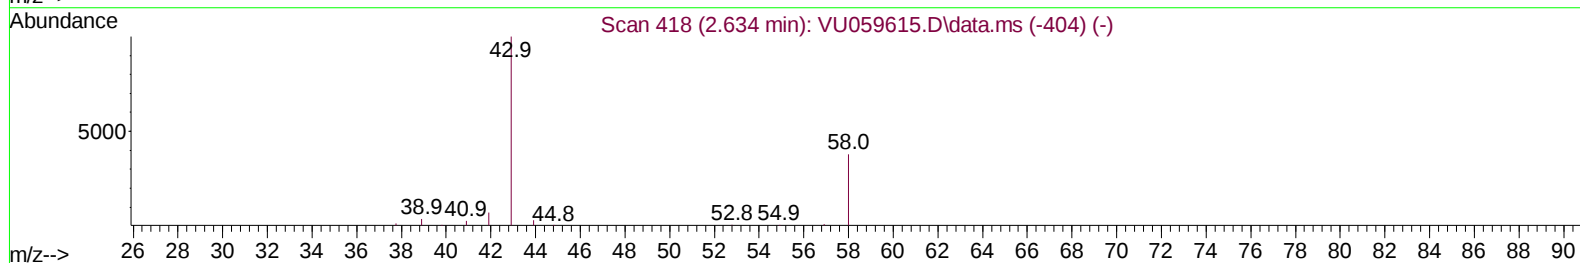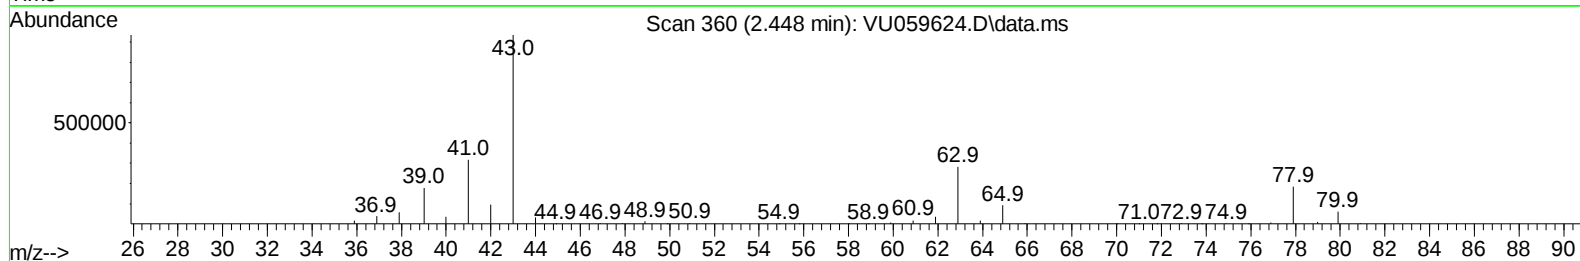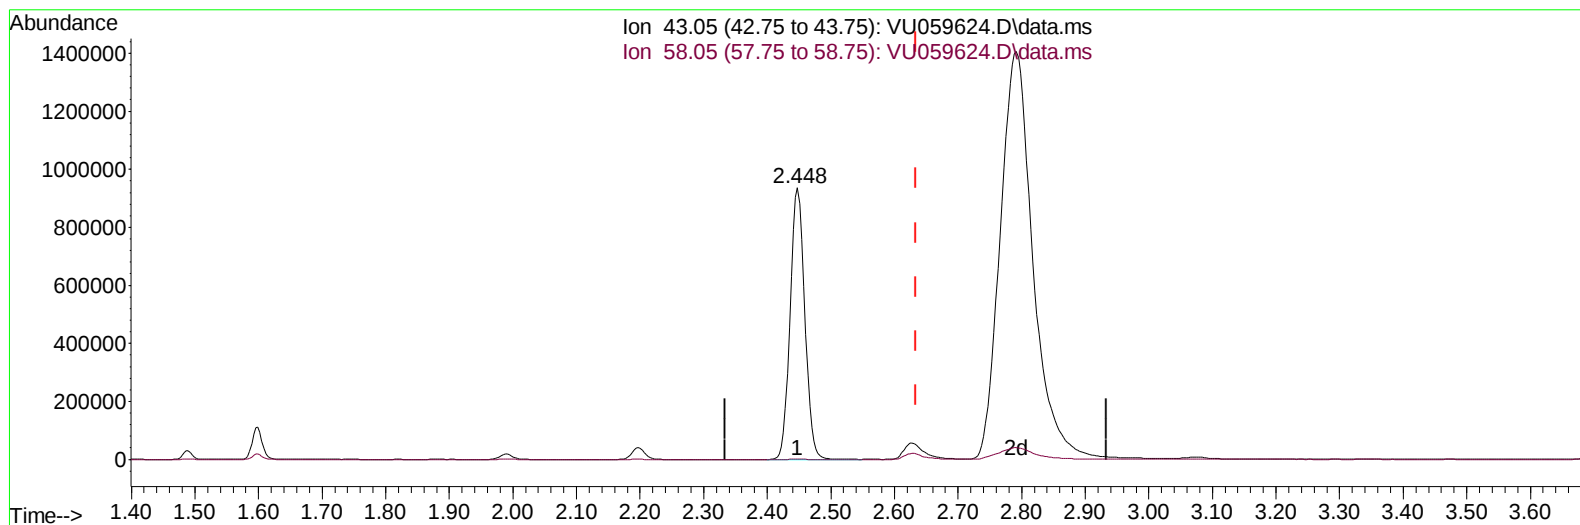

TIC: VU059624.D\data.ms

(13) Acetone (T)

2.448min (-0.186) 1086.07 ug/L

response 1498505

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	3.08
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059624.D
Acq On : 28 Jun 2024 16:41
Operator : MD/SY
Sample : P3059-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM4

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:58:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

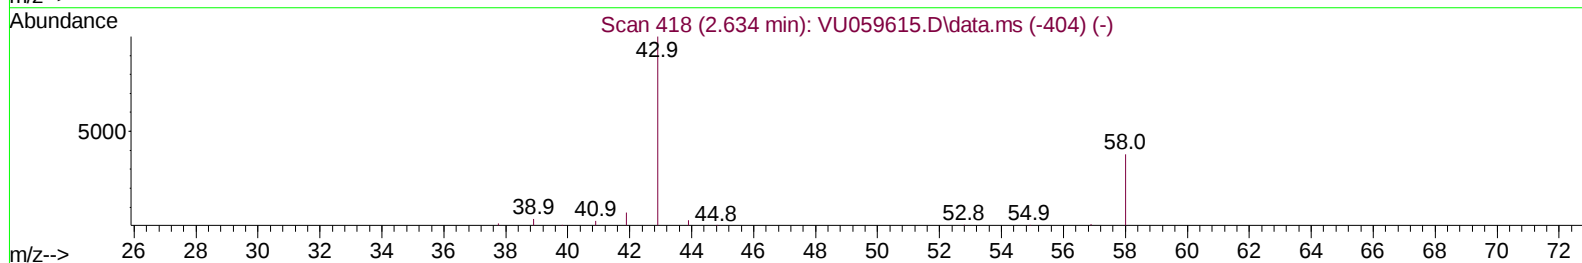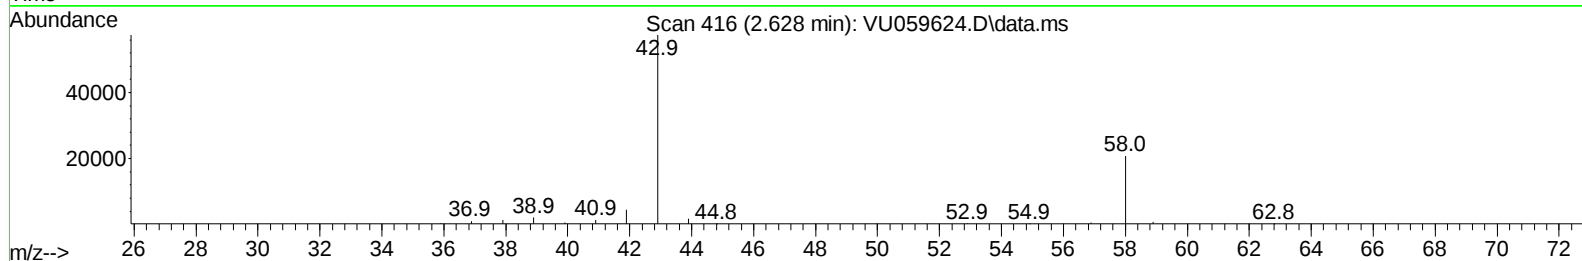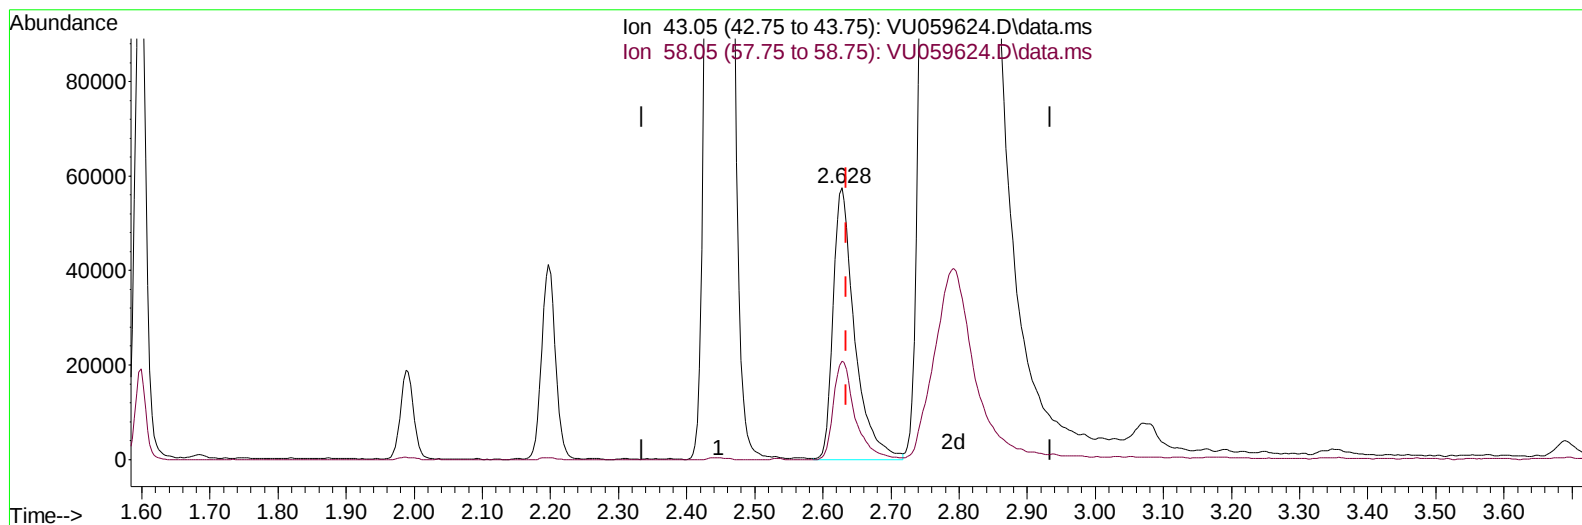

TIC: VU059624.D\data.ms

(13) Acetone (T)

2.628min (-0.006) 91.63 ug/L m

response 126428

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	36.47
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059624.D
 Acq On : 28 Jun 2024 16:41
 Operator : MD/SY
 Sample : P3059-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GM4

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:58:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 28 23:55:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		148500	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		148926	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		66379	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		36670	3.551	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	71.000%		
7) Chloroethane-d5	1.907	69		40292	4.055	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	81.200%		
11) 1,1-Dichloroethene-d2	2.560	65		16214	3.785	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	75.600%		
20) 2-Butanone-d5	4.618	46		112801	53.033	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	106.060%		
24) Chloroform-d	5.055	84		91075	4.297	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	86.000%		
26) 1,2-Dichloroethane-d4	5.695	65		46247	4.530	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	90.600%		
32) Benzene-d6	5.721	84		181753	4.434	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	88.600%		
36) 1,2-Dichloropropane-d6	6.685	67		57978	4.616	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	92.400%		
41) Toluene-d8	7.894	98		149551	3.925	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	78.400%		
43) trans-1,3-Dichloroprop...	8.177	79		17713	4.504	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	90.000%		
46) 2-Hexanone-d5	8.627	63		93823	57.417	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	114.840%		
56) 1,1,2,2-Tetrachloroeth...	10.750	84		51588	4.971	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	99.400%		
66) 1,2-Dichlorobenzene-d4	12.187	152		60264	5.101	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	102.000%		
Target Compounds							
						Qvalue	
13) Acetone	2.628	43		126428m	91.631	ug/L	
18) trans-1,2-Dichloroethene	3.345	96		74807	6.830	ug/L	92
22) cis-1,2-Dichloroethene	4.657	96		283428	23.476	ug/L	94
34) Trichloroethene	6.538	95		44982	3.673	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059624.D
Acq On : 28 Jun 2024 16:41
Operator : MD/SY
Sample : P3059-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM4

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

Quant Time: Jun 28 23:58:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

