




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059625.D
Acq On : 28 Jun 2024 17:05
Operator : MD/SY
Sample : P3059-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:58:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

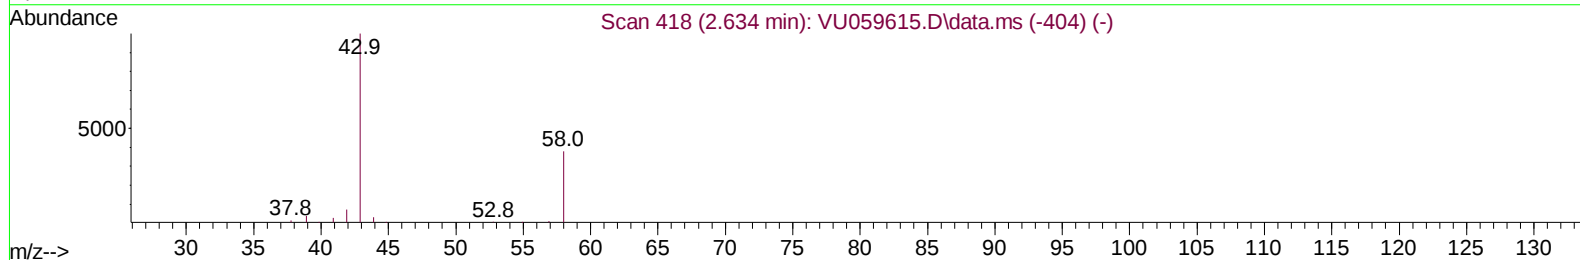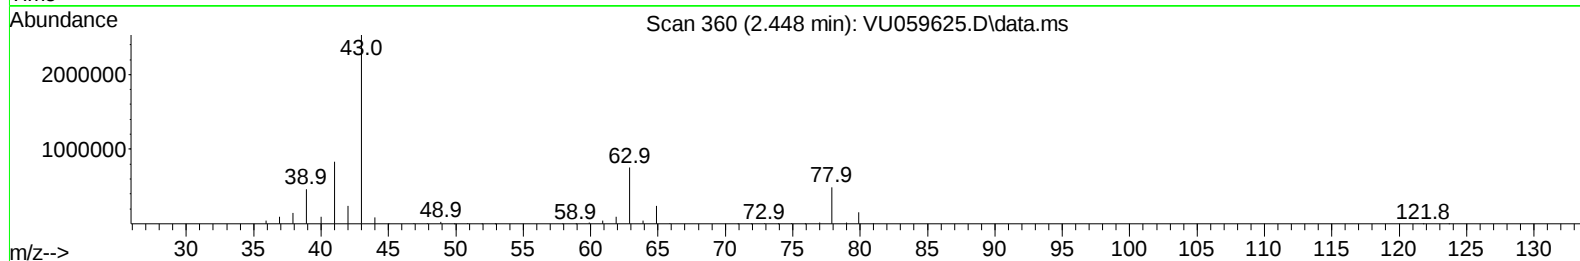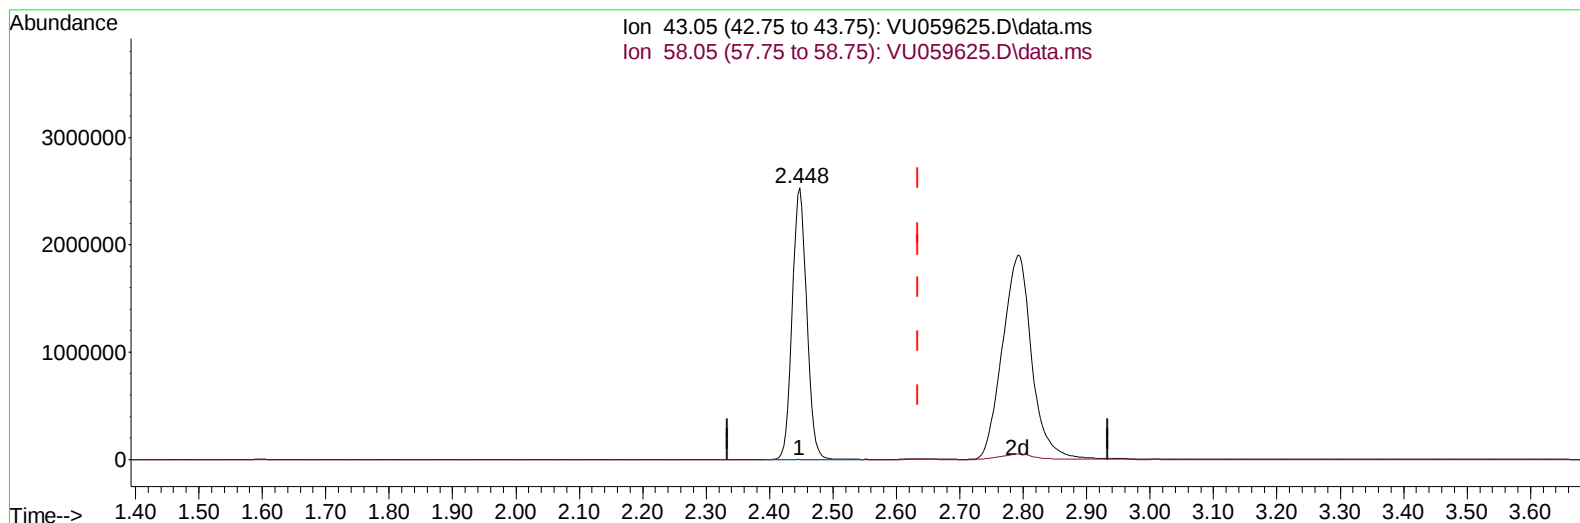

TIC: VU059625.D\data.ms

(13) Acetone (T)

2.448min (-0.186) 3071.71 ug/L

response 4015166

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	0.14
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059625.D
Acq On : 28 Jun 2024 17:05
Operator : MD/SY
Sample : P3059-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:58:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

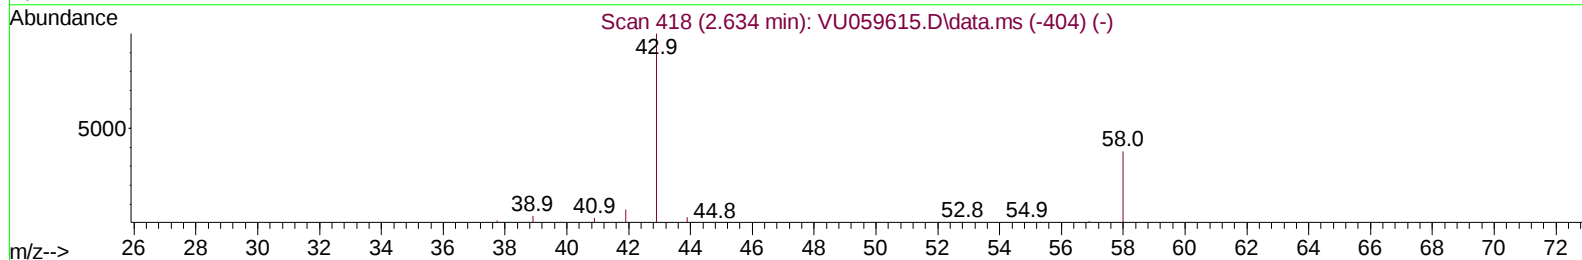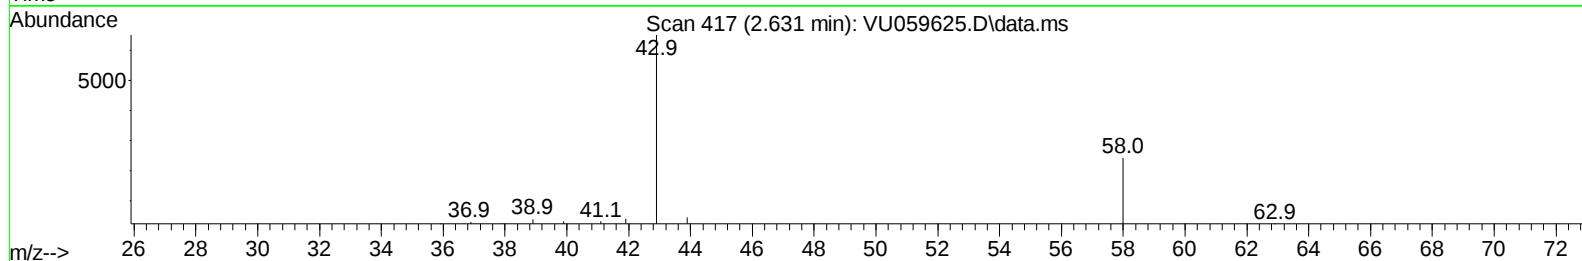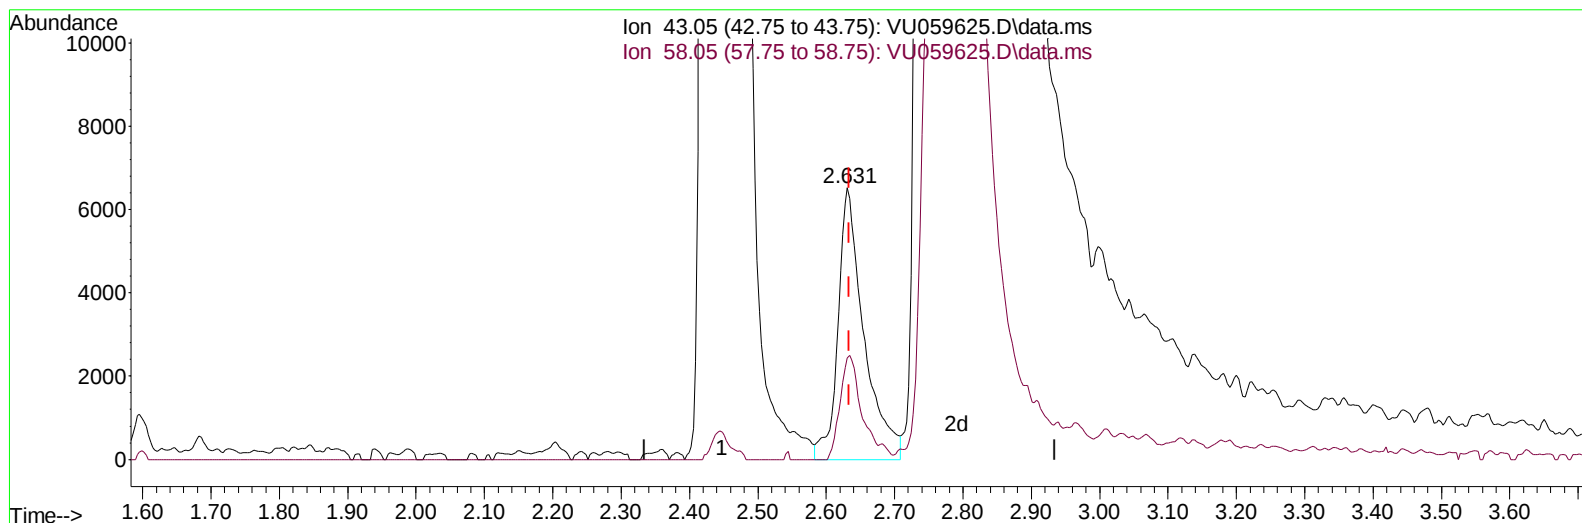

TIC: VU059625.D\data.ms

(13) Acetone (T)

2.631min (-0.003) 13.13 ug/L m

response 17165

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	33.07
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059625.D
 Acq On : 28 Jun 2024 17:05
 Operator : MD/SY
 Sample : P3059-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GM5

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:58:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 28 23:55:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		140685	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		146960	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		64262	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		37188	3.801	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.000%	
7) Chloroethane-d5	1.907	69		40245	4.276	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.600%	
11) 1,1-Dichloroethene-d2	2.560	65		16668	4.107	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	82.200%	
20) 2-Butanone-d5	4.618	46		117109	58.117	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.240%	
24) Chloroform-d	5.055	84		90677	4.516	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%	
26) 1,2-Dichloroethane-d4	5.695	65		45742	4.729	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.600%	
32) Benzene-d6	5.721	84		180076	4.452	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.000%	
36) 1,2-Dichloropropane-d6	6.685	67		57046	4.603	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.000%	
41) Toluene-d8	7.894	98		148955	3.962	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.200%	
43) trans-1,3-Dichloroprop...	8.174	79		17877	4.606	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	92.200%	
46) 2-Hexanone-d5	8.627	63		91188	56.551	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	113.100%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		52416	5.119	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.400%	
66) 1,2-Dichlorobenzene-d4	12.190	152		57489	5.026	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.600%	
Target Compounds							
13) Acetone	2.631	43		17165m	13.132	ug/L	
47) Tetrachloroethene	8.547	164		9682	1.032	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059625.D
Acq On : 28 Jun 2024 17:05
Operator : MD/SY
Sample : P3059-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM5

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

Quant Time: Jun 28 23:58:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

