




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059627.D
Acq On : 28 Jun 2024 17:53
Operator : MD/SY
Sample : P3059-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM7

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:58:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

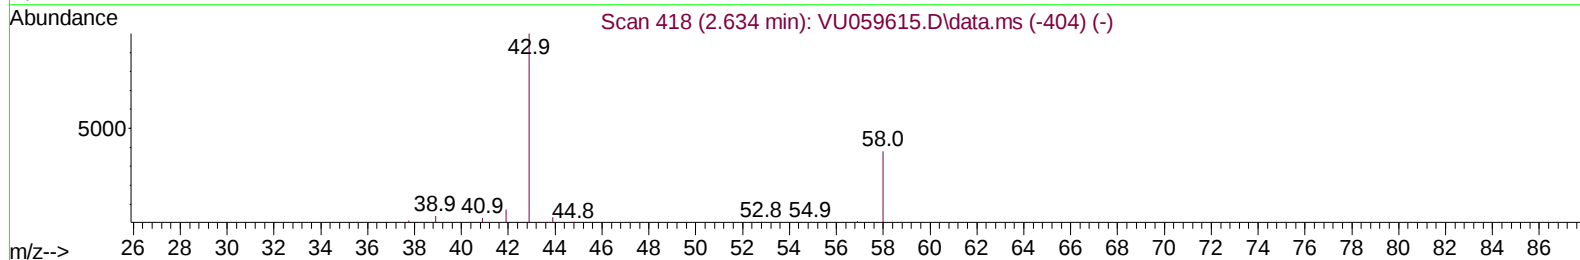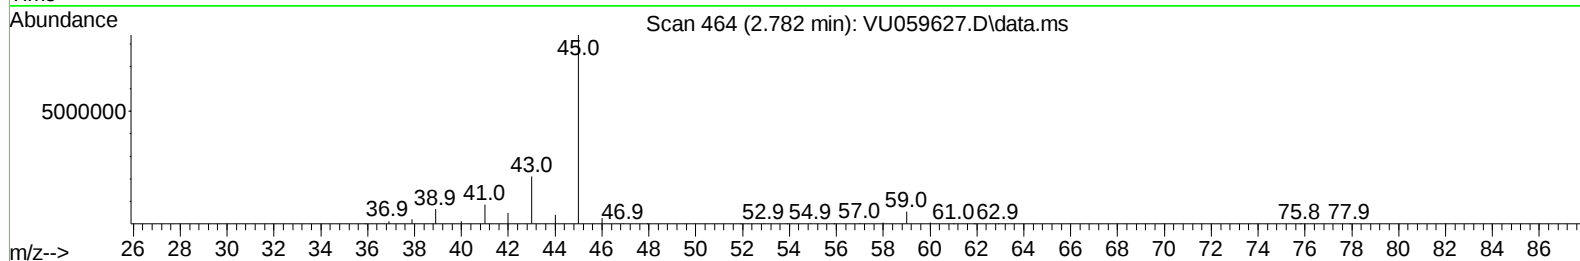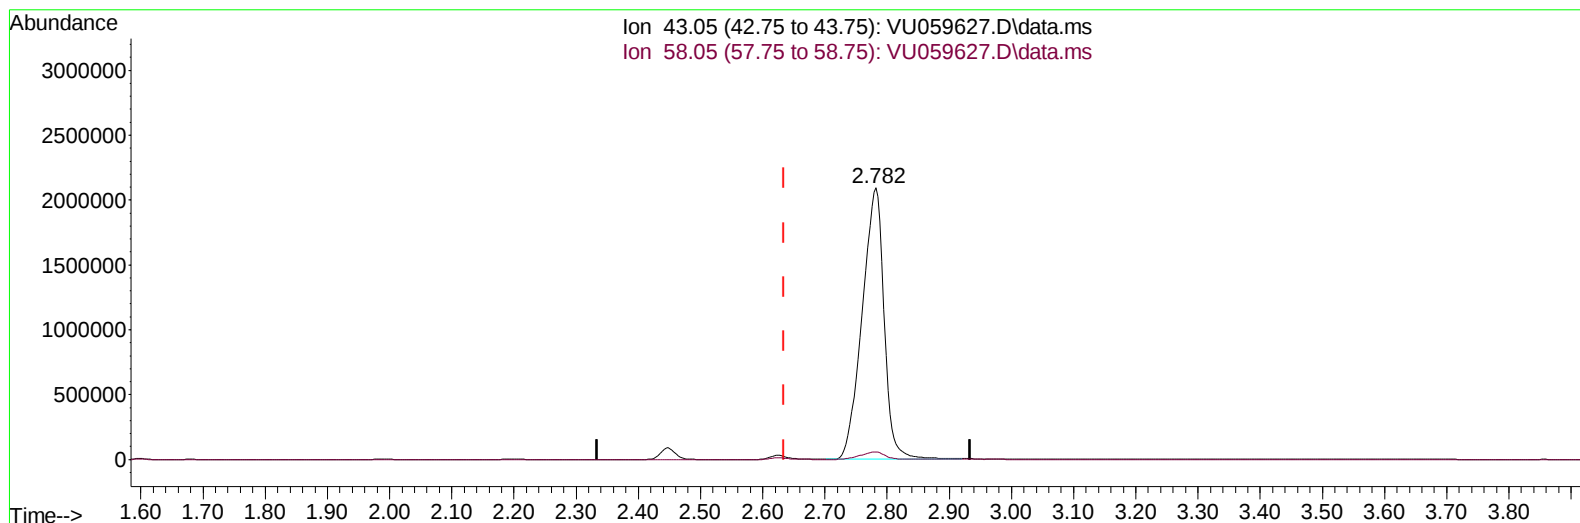

TIC: VU059627.D\data.ms

(13) Acetone (T)

2.782min (+ 0.148) 3962.89 ug/L

response 5155514

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	3.16
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059627.D
Acq On : 28 Jun 2024 17:53
Operator : MD/SY
Sample : P3059-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM7

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:58:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

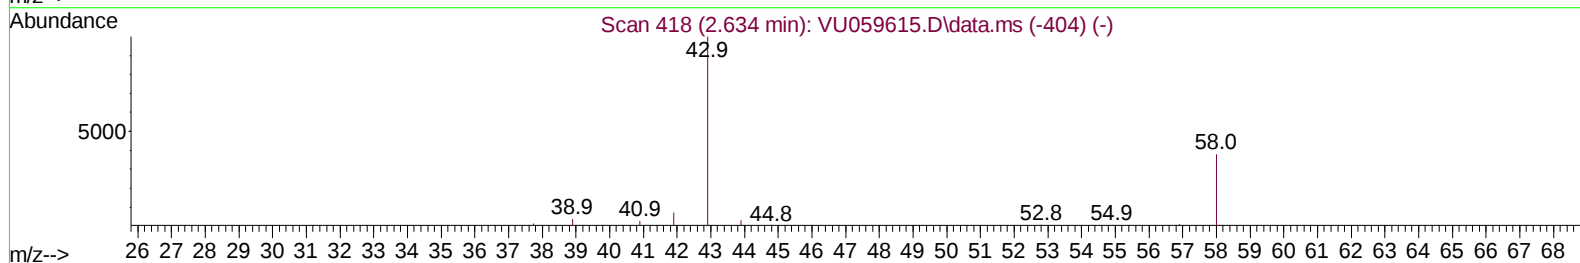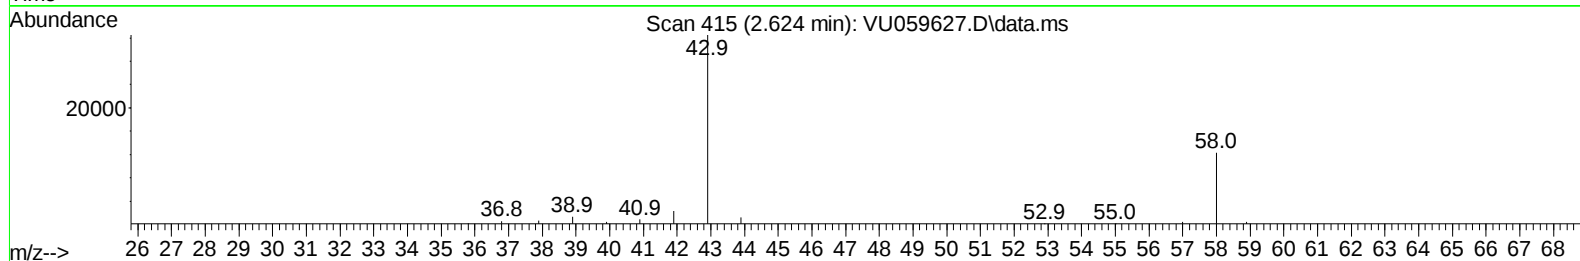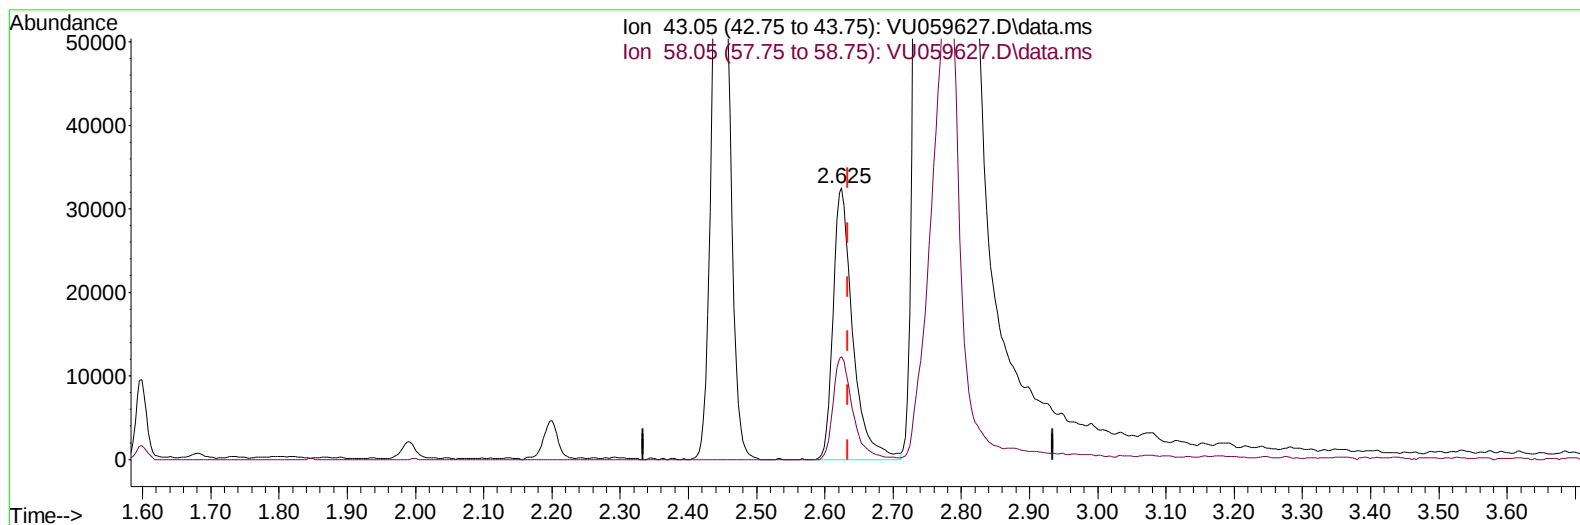

TIC: VU059627.D\data.ms

(13) Acetone (T)

2.624min (-0.010) 49.84 ug/L m

response 64843

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	251.62#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059627.D
 Acq On : 28 Jun 2024 17:53
 Operator : MD/SY
 Sample : P3059-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GM7

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:58:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 28 23:55:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		140018	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		143912	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		63973	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		36842	3.784	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	75.600%		
7) Chloroethane-d5	1.907	69		38881	4.150	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	83.000%		
11) 1,1-Dichloroethene-d2	2.560	65		15676	3.881	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	77.600%		
20) 2-Butanone-d5	4.615	46		115122	57.403	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	114.800%		
24) Chloroform-d	5.055	84		89662	4.487	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	89.800%		
26) 1,2-Dichloroethane-d4	5.695	65		45991	4.778	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	95.600%		
32) Benzene-d6	5.721	84		178017	4.495	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	89.800%		
36) 1,2-Dichloropropane-d6	6.685	67		58174	4.793	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	95.800%		
41) Toluene-d8	7.891	98		148051	4.021	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	80.400%		
43) trans-1,3-Dichloroprop...	8.177	79		16937	4.457	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	89.200%		
46) 2-Hexanone-d5	8.627	63		91015	57.639	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	115.280%		
56) 1,1,2,2-Tetrachloroeth...	10.750	84		52686	5.254	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	105.000%		
66) 1,2-Dichlorobenzene-d4	12.190	152		56696	4.979	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	99.600%		
Target Compounds							
13) Acetone	2.624	43		64843m	49.843	ug/L	
22) cis-1,2-Dichloroethene	4.660	96		15079	1.325	ug/L	92
34) Trichloroethene	6.541	95		8393	0.709	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

