




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059628.D
 Acq On : 28 Jun 2024 18:17
 Operator : MD/SY
 Sample : P3059-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GM8

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:59:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 28 23:55:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

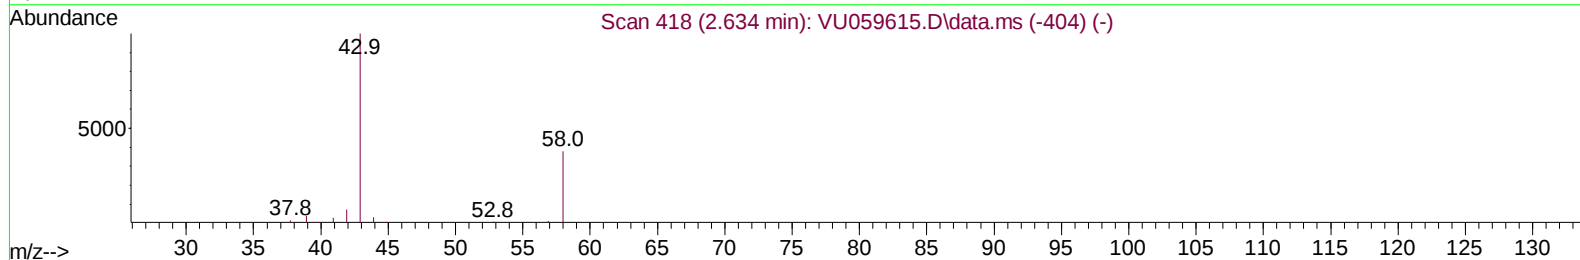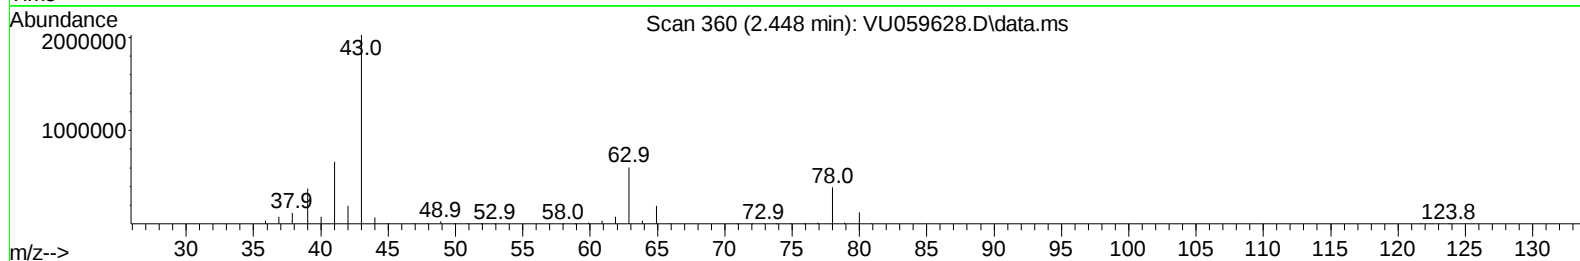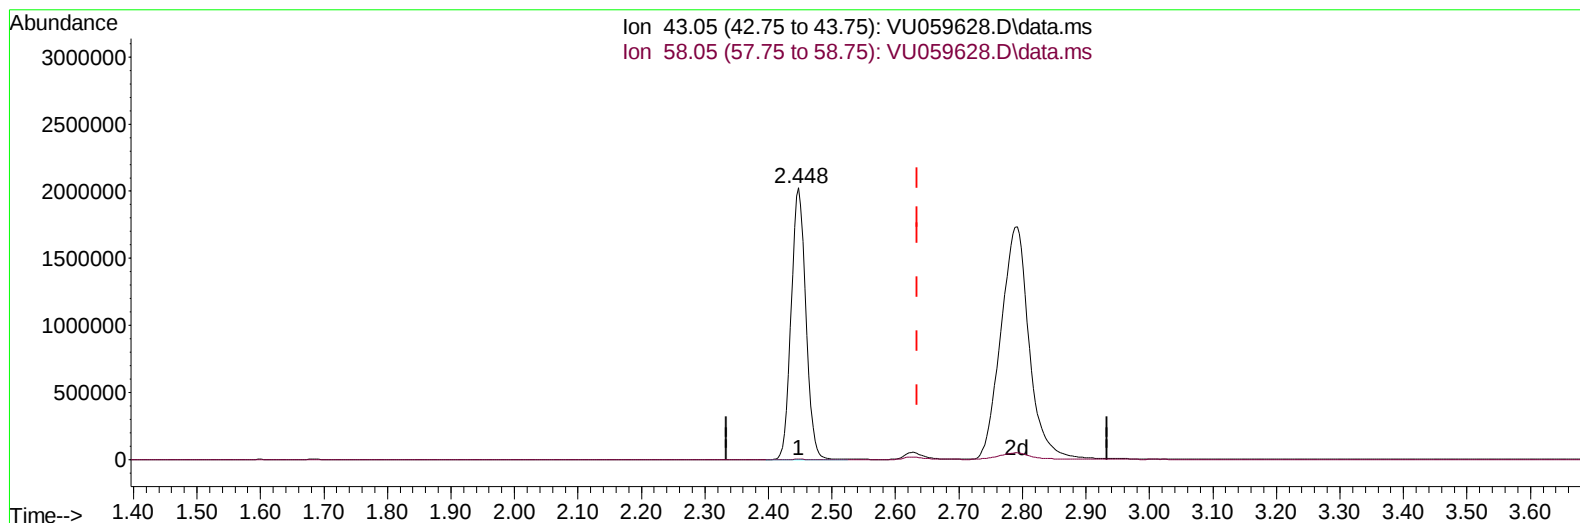

TIC: VU059628.D\data.ms

(13) Acetone (T)

2.448min (-0.187) 2480.05 ug/L

response 3232614

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	1.30
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059628.D
Acq On : 28 Jun 2024 18:17
Operator : MD/SY
Sample : P3059-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM8

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:59:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

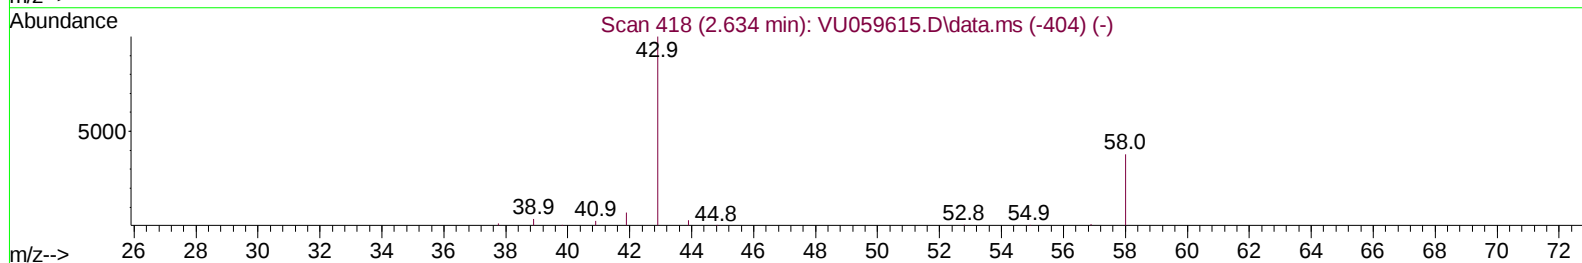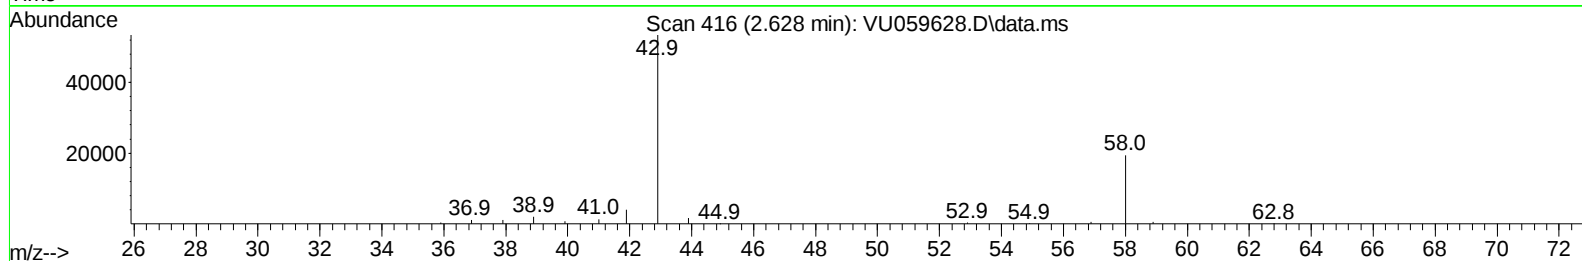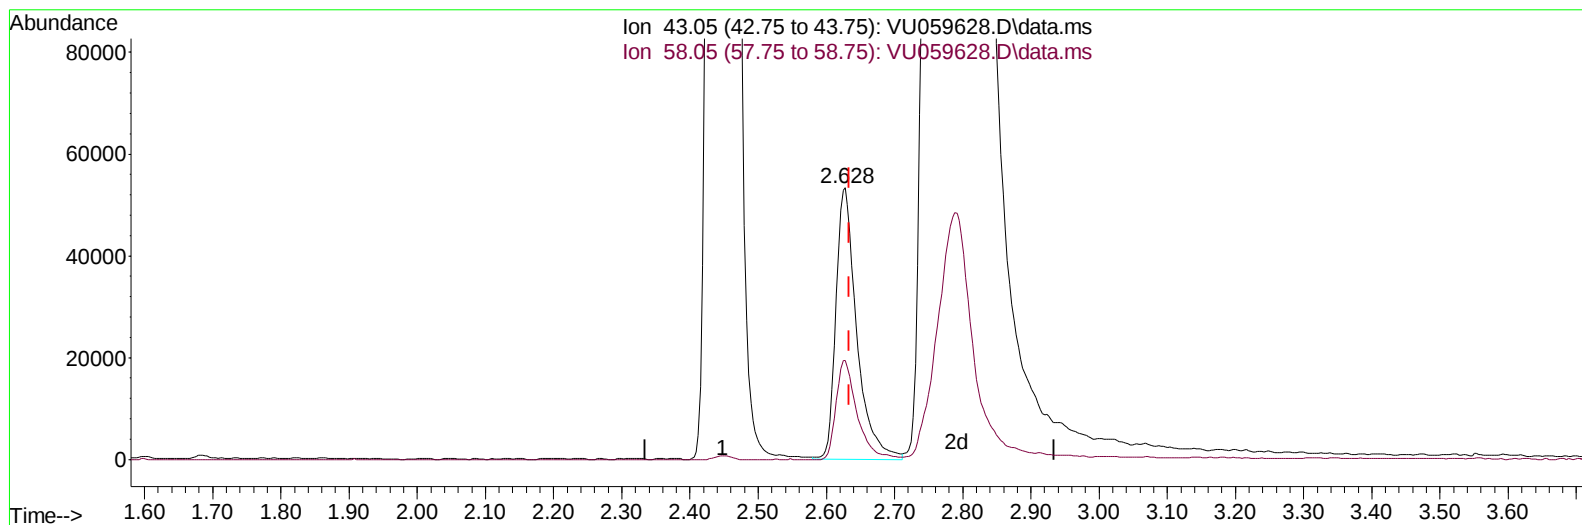

TIC: VU059628.D\data.ms

(13) Acetone (T)

2.628min (-0.006) 87.20 ug/L m

response 113662

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	36.85
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059628.D
 Acq On : 28 Jun 2024 18:17
 Operator : MD/SY
 Sample : P3059-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GM8

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:59:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 28 23:55:24 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		140287	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		147748	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		63680	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		37382	3.832	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	76.600%	
7) Chloroethane-d5	1.907	69		39738	4.234	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	84.600%	
11) 1,1-Dichloroethene-d2	2.560	65		16124	3.984	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	79.600%	
20) 2-Butanone-d5	4.618	46		115070	57.267	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	114.540%	
24) Chloroform-d	5.055	84		90894	4.540	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	90.800%	
26) 1,2-Dichloroethane-d4	5.695	65		46590	4.831	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	96.600%	
32) Benzene-d6	5.721	84		182016	4.476	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	89.600%	
36) 1,2-Dichloropropane-d6	6.682	67		57875	4.645	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	92.800%	
41) Toluene-d8	7.894	98		150044	3.969	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	79.400%	
43) trans-1,3-Dichloroprop...	8.177	79		17794	4.561	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	91.200%	
46) 2-Hexanone-d5	8.627	63		94008	57.989	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	115.980%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		53992	5.245	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	104.800%	
66) 1,2-Dichlorobenzene-d4	12.190	152		58472	5.159	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	103.200%	
Target Compounds							
						Qvalue	
13) Acetone	2.628	43		113662m	87.201	ug/L	
22) cis-1,2-Dichloroethene	4.666	96		2089	0.183	ug/L	88
34) Trichloroethene	6.541	95		5038	0.415	ug/L	92
37) 1,2-Dichloropropane	6.785	63		25123	2.164	ug/L	99
47) Tetrachloroethene	8.547	164		21864	2.319	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059628.D
Acq On : 28 Jun 2024 18:17
Operator : MD/SY
Sample : P3059-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM8

Manual IntegrationsAPPROVED

Quant Time: Jun 28 23:59:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 28 23:55:24 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

