




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059645.D
 Acq On : 29 Jun 2024 01:00
 Operator : MD/SY
 Sample : P3059-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GN2

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

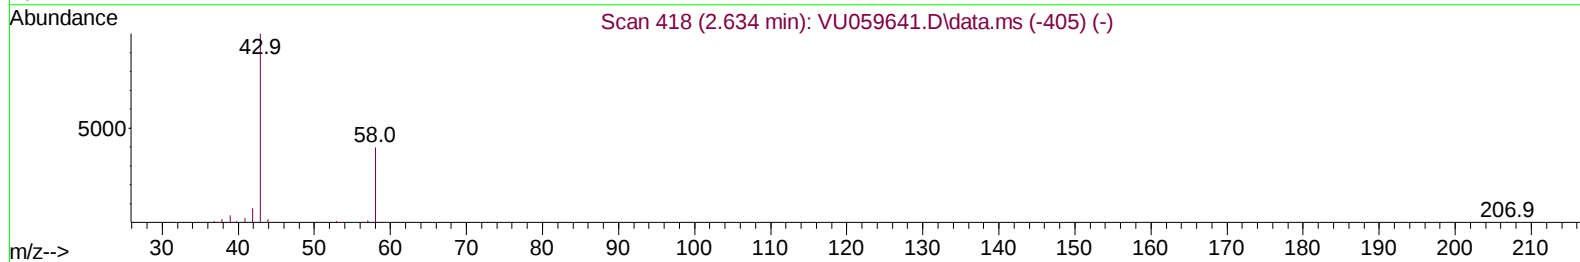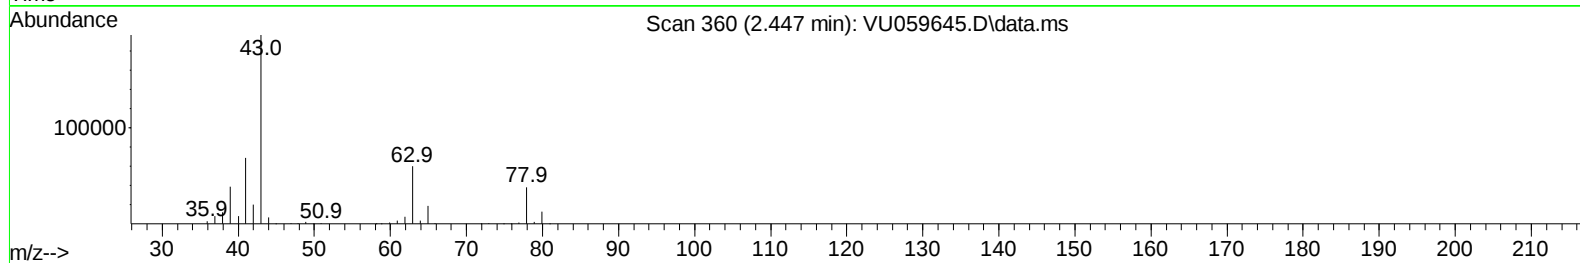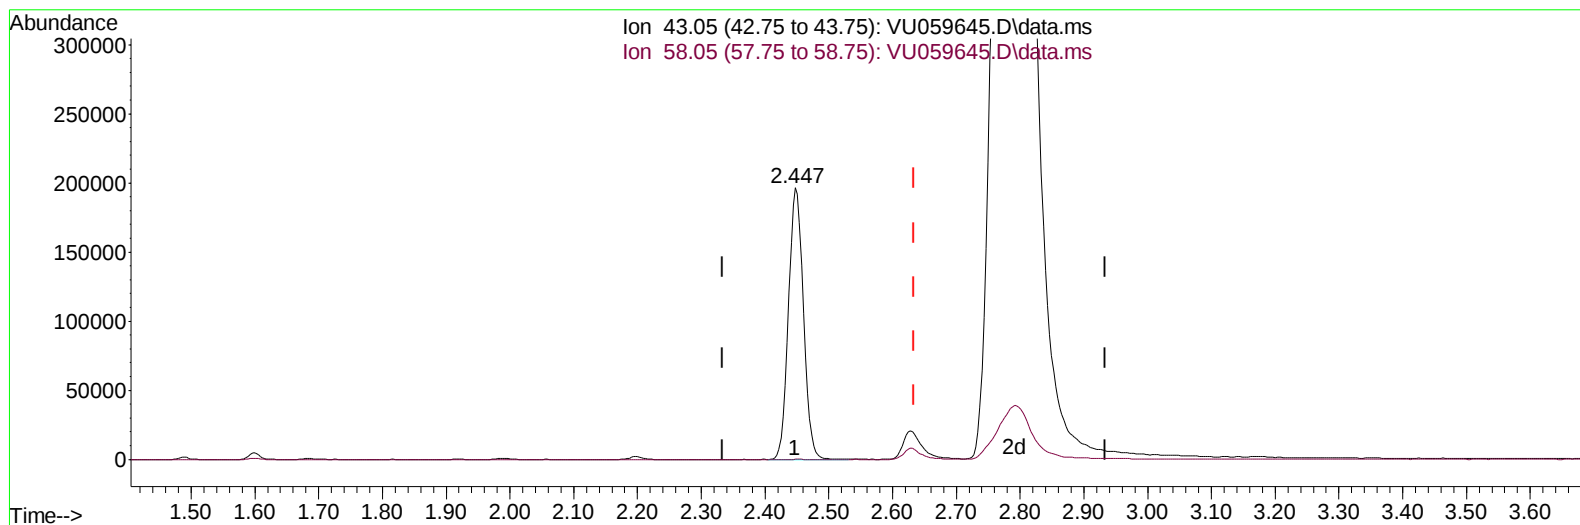

TIC: VU059645.D\data.ms

(13) Acetone (T)

2.447min (-0.186) 247.14 ug/L

response 319935

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	5.05
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059645.D
Acq On : 29 Jun 2024 01:00
Operator : MD/SY
Sample : P3059-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN2

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

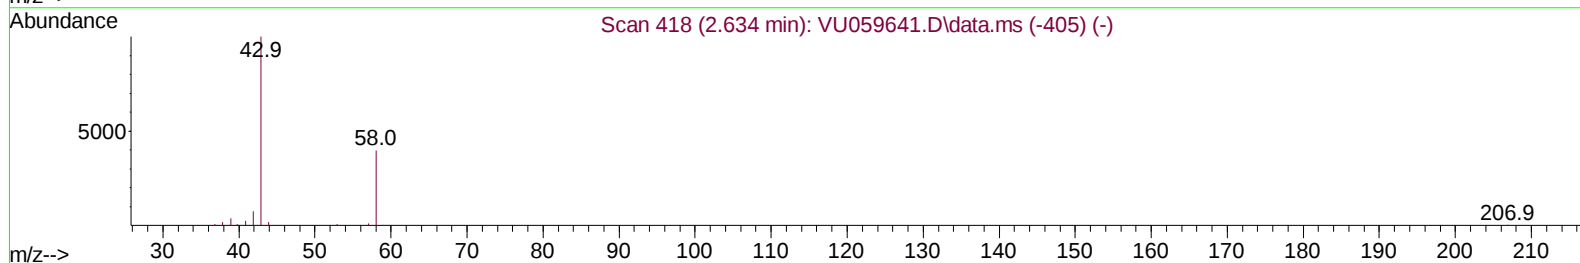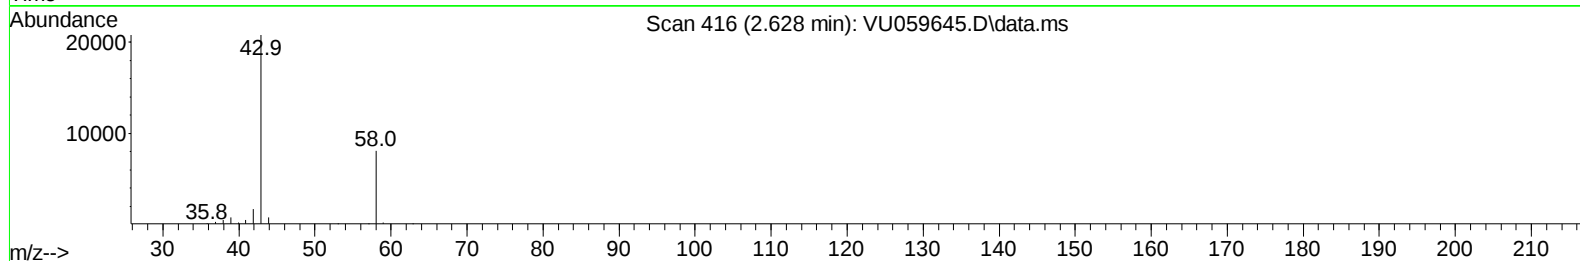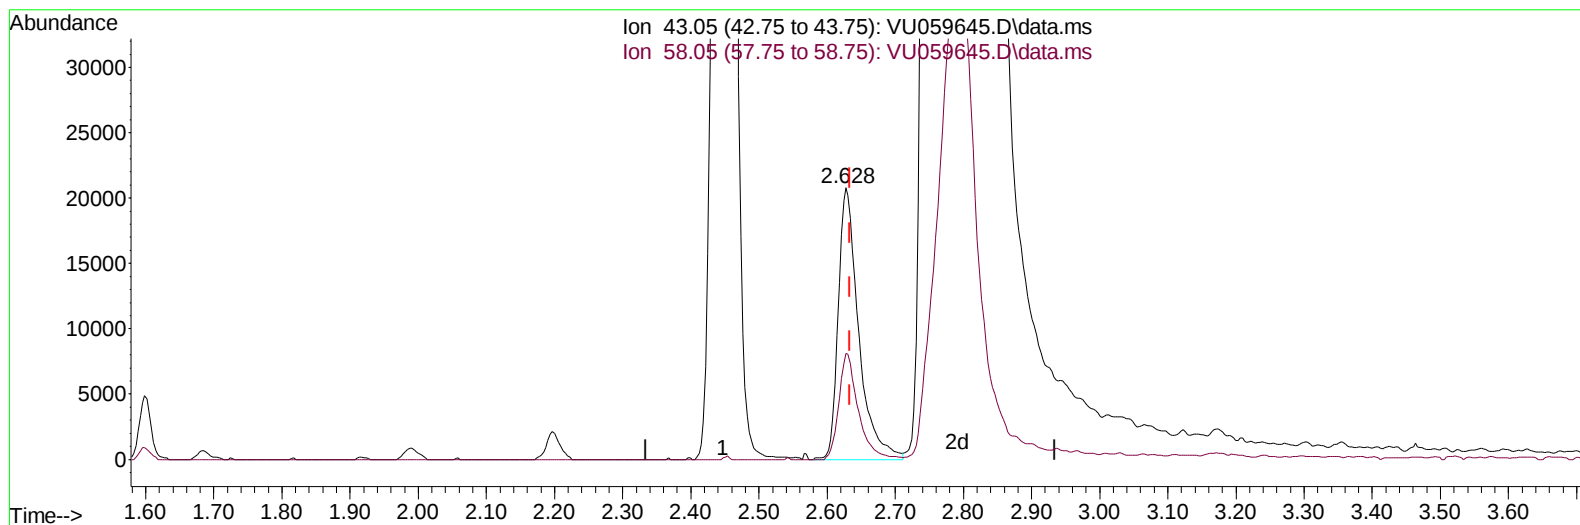

TIC: VU059645.D\data.ms

(13) Acetone (T)

2.628min (-0.006) 33.37 ug/L m

response 43200

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	37.38
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059645.D
 Acq On : 29 Jun 2024 01:00
 Operator : MD/SY
 Sample : P3059-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GN2

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:00 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		139329	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		147686	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		64071	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		34698	3.581	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	71.600%	
7) Chloroethane-d5	1.907	69		38976	4.181	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	83.600%	
11) 1,1-Dichloroethene-d2	2.560	65		15393	3.830	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	76.600%	
20) 2-Butanone-d5	4.618	46		102020	51.121	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	102.240%	
24) Chloroform-d	5.055	84		91422	4.597	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	92.000%	
26) 1,2-Dichloroethane-d4	5.695	65		45074	4.705	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	94.200%	
32) Benzene-d6	5.717	84		179427	4.414	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	88.200%	
36) 1,2-Dichloropropane-d6	6.682	67		57355	4.605	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	92.200%	
41) Toluene-d8	7.891	98		148840	3.939	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	78.800%	
43) trans-1,3-Dichloroprop...	8.177	79		16210	4.156	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	83.200%	
46) 2-Hexanone-d5	8.627	63		76059	46.937	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	93.880%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		50455	4.903	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	98.000%	
66) 1,2-Dichlorobenzene-d4	12.187	152		58453	5.126	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	102.600%	
Target Compounds							
13) Acetone	2.628	43		43200m	33.371	ug/L	
18) trans-1,2-Dichloroethene	3.351	96		2635	0.256	ug/L	82
19) 1,1-Dichloroethane	3.862	63		13217	0.697	ug/L	97
22) cis-1,2-Dichloroethene	4.656	96		76662	6.768	ug/L	92
34) Trichloroethene	6.537	95		9017	0.742	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059645.D
Acq On : 29 Jun 2024 01:00
Operator : MD/SY
Sample : P3059-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN2

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:00 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

