




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059646.D
Acq On : 29 Jun 2024 01:24
Operator : MD/SY
Sample : P3059-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN3

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

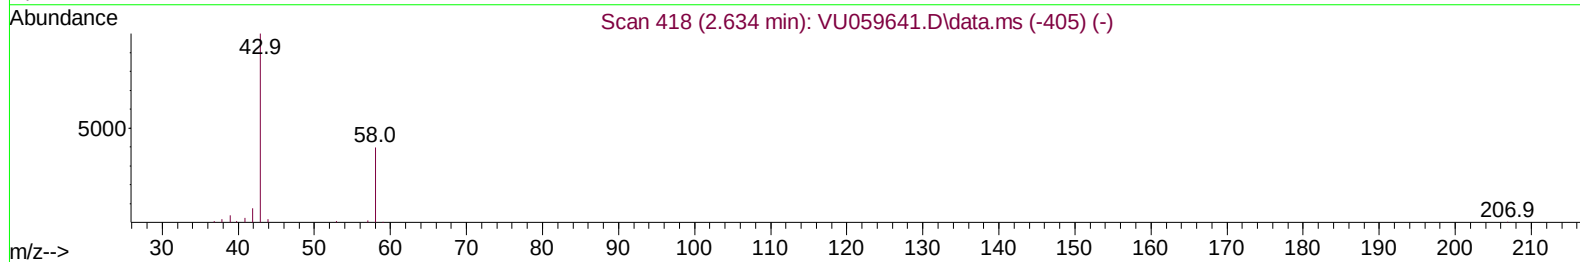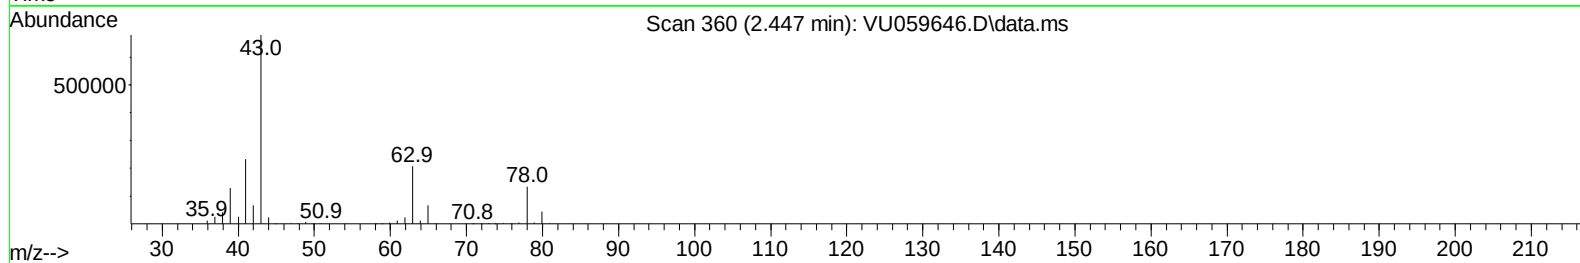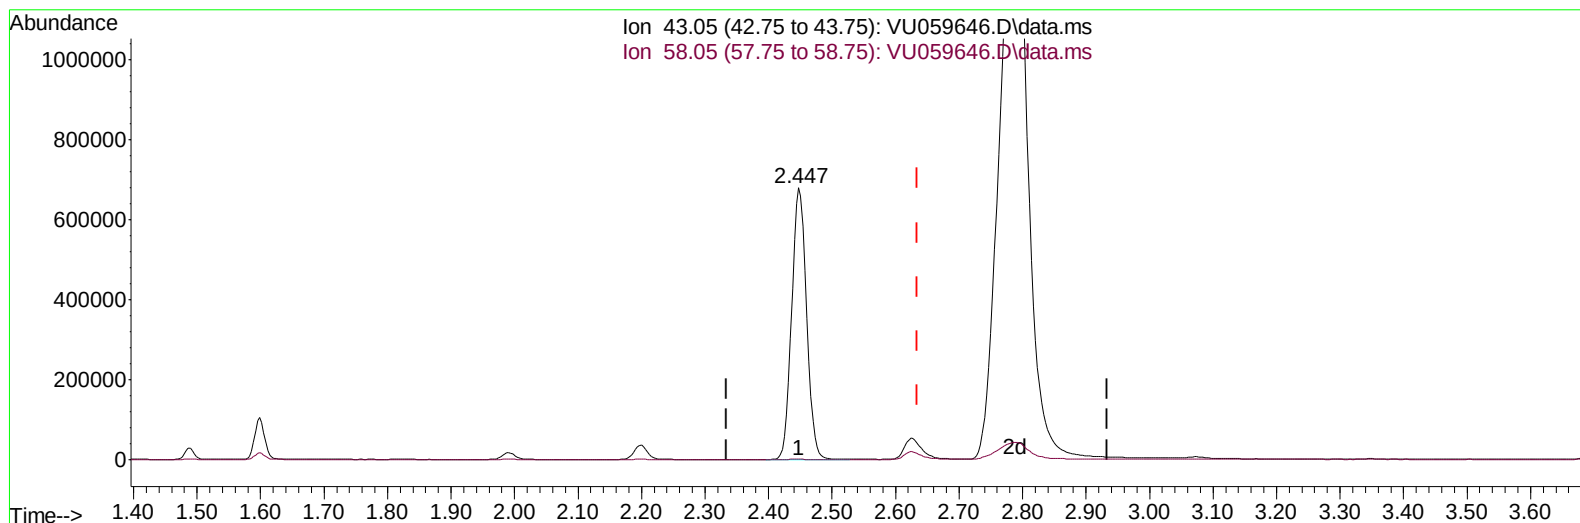

TIC: VU059646.D\data.ms

(13) Acetone (T)

2.447min (-0.186) 820.37 ug/L

response 1100276

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	3.52
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059646.D
Acq On : 29 Jun 2024 01:24
Operator : MD/SY
Sample : P3059-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN3

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

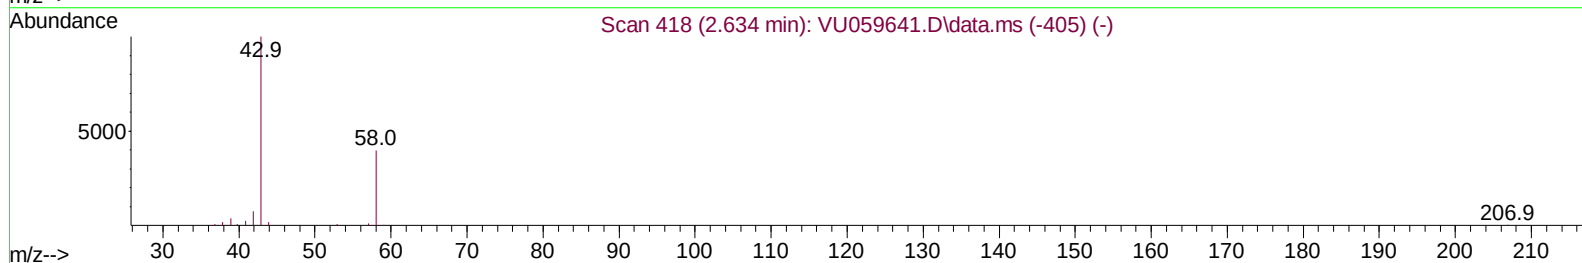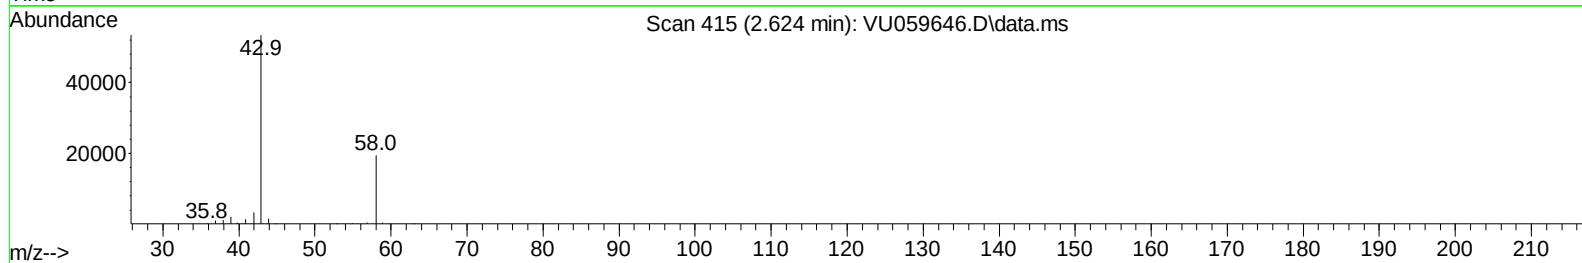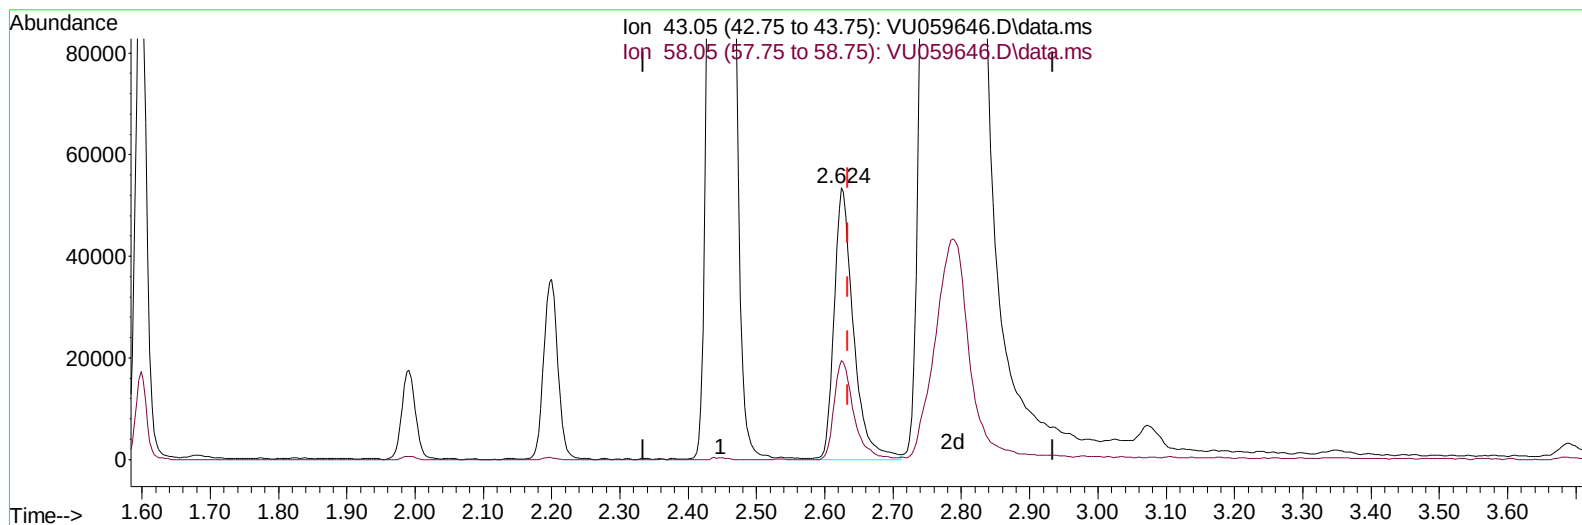

TIC: VU059646.D\data.ms

(13) Acetone (T)

2.624min (-0.010) 78.37 ug/L m

response 105115

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	36.90
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059646.D
 Acq On : 29 Jun 2024 01:24
 Operator : MD/SY
 Sample : P3059-12
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GN3

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		144349	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		147711	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		65308	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		34424	3.430	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	68.600%		
7) Chloroethane-d5	1.907	69		37512	3.884	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	77.600%		
11) 1,1-Dichloroethene-d2	2.560	65		15787	3.791	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	75.800%		
20) 2-Butanone-d5	4.618	46		105436	50.996	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	102.000%		
24) Chloroform-d	5.055	84		90843	4.409	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	88.200%		
26) 1,2-Dichloroethane-d4	5.695	65		45360	4.571	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	91.400%		
32) Benzene-d6	5.721	84		180858	4.449	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	89.000%		
36) 1,2-Dichloropropane-d6	6.685	67		57833	4.643	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	92.800%		
41) Toluene-d8	7.891	98		149358	3.952	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	79.000%		
43) trans-1,3-Dichloroprop...	8.177	79		16295	4.177	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	83.600%		
46) 2-Hexanone-d5	8.627	63		80552	49.701	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	99.400%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84		49817	4.840	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	96.800%		
66) 1,2-Dichlorobenzene-d4	12.187	152		58027	4.992	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	99.800%		
Target Compounds							
13) Acetone	2.624	43		105115m	78.375	ug/L	
18) trans-1,2-Dichloroethene	3.345	96		74227	6.972	ug/L	90
22) cis-1,2-Dichloroethene	4.656	96		282743	24.093	ug/L	95
34) Trichloroethene	6.534	95		44473	3.661	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059646.D
Acq On : 29 Jun 2024 01:24
Operator : MD/SY
Sample : P3059-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN3

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

Quant Time: Jun 29 04:13:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

