




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059647.D
Acq On : 29 Jun 2024 01:48
Operator : MD/SY
Sample : P3059-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN4

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

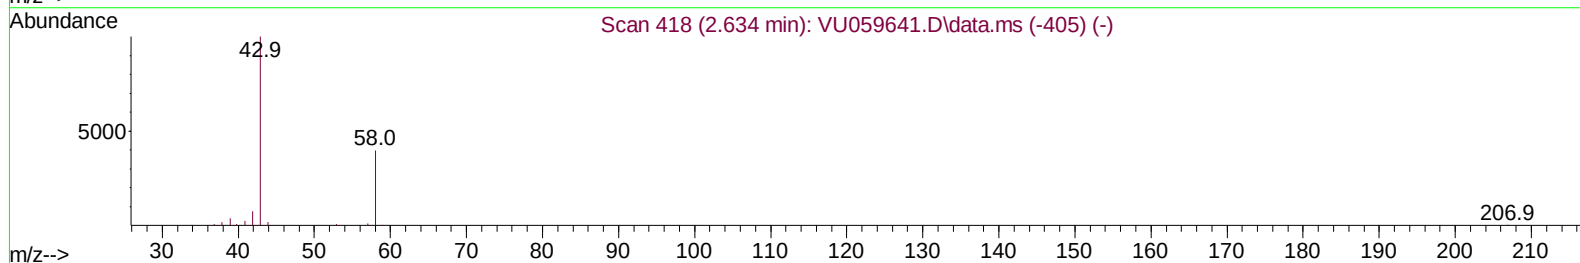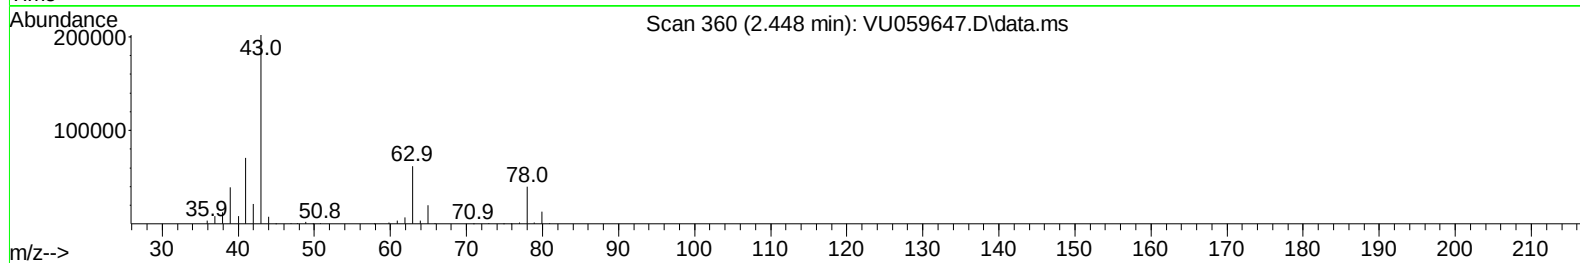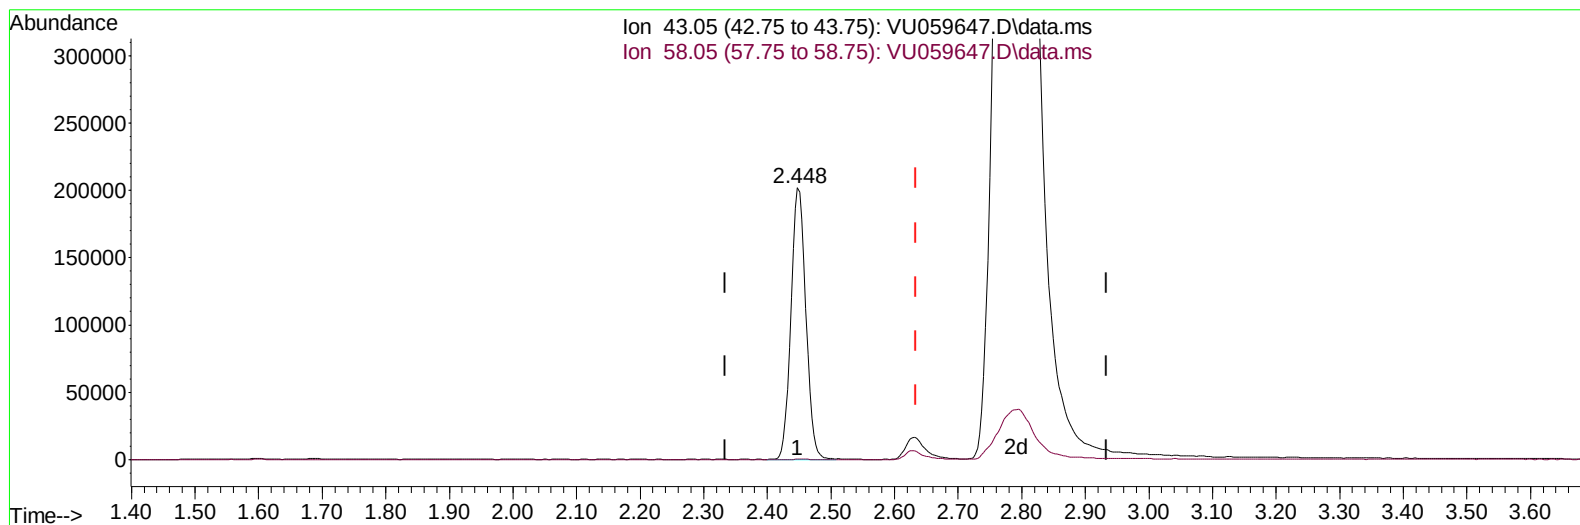

TIC: VU059647.D\data.ms

(13) Acetone (T)

2.448min (-0.186) 250.72 ug/L

response 327780

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	4.18
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059647.D
Acq On : 29 Jun 2024 01:48
Operator : MD/SY
Sample : P3059-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN4

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

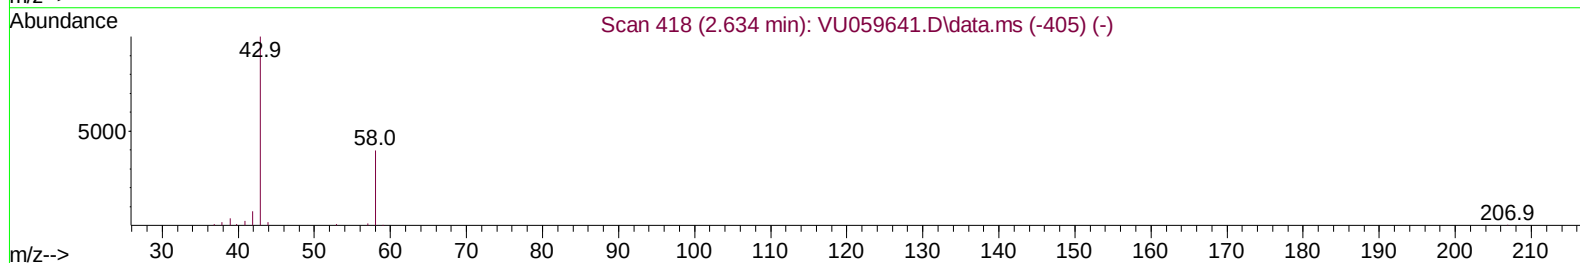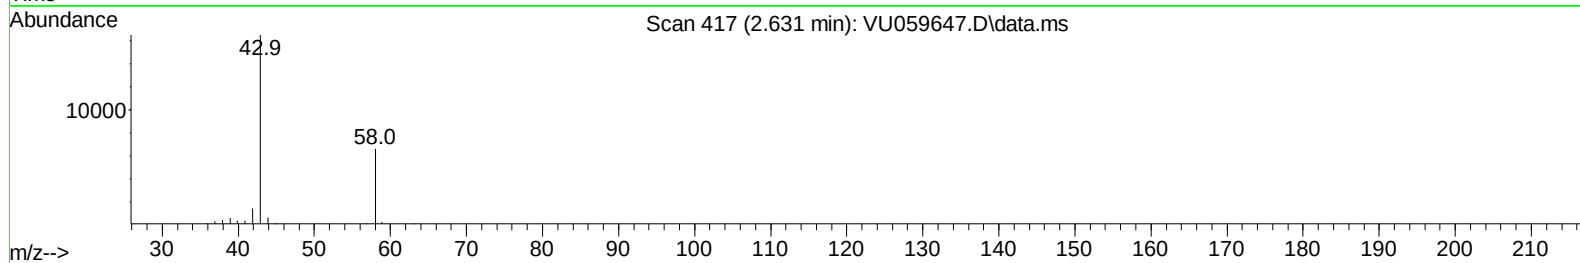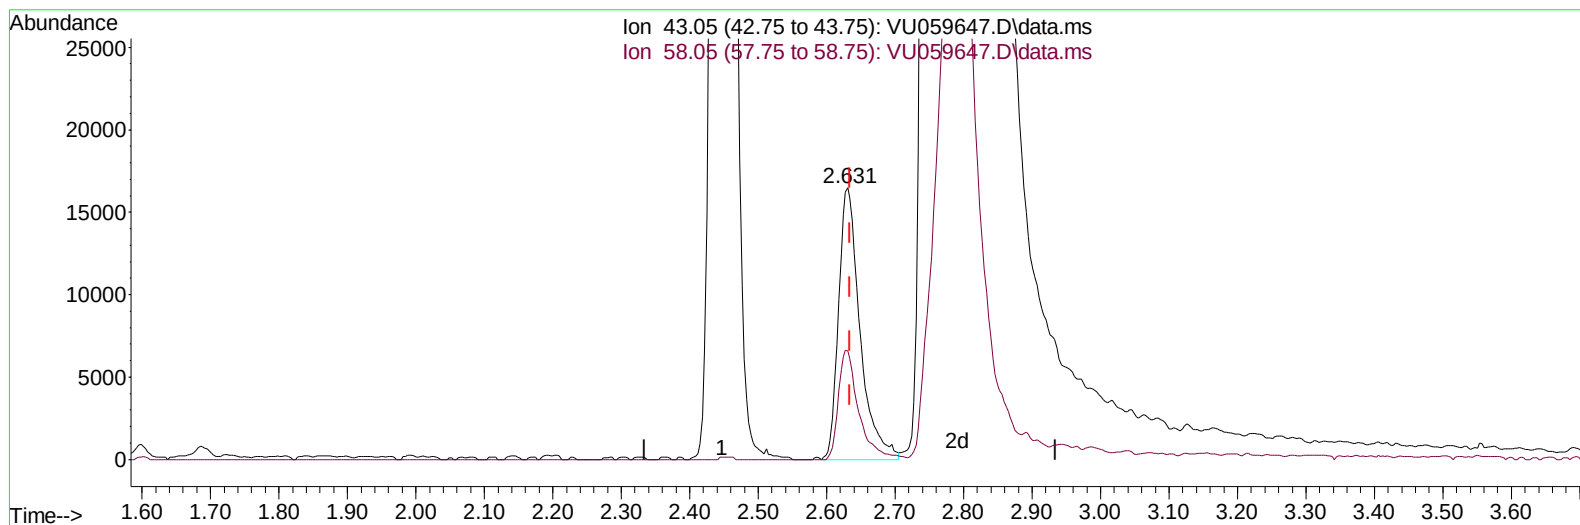

TIC: VU059647.D\data.ms

(13) Acetone (T)

2.631min (-0.003) 27.43 ug/L m

response 35865

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	38.22
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059647.D
 Acq On : 29 Jun 2024 01:48
 Operator : MD/SY
 Sample : P3059-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GN4

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		140705	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		147868	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		63995	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		33756	3.450	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery =	69.000%		
7) Chloroethane-d5	1.907	69		38122	4.049	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery =	81.000%		
11) 1,1-Dichloroethene-d2	2.560	65		15866	3.909	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery =	78.200%		
20) 2-Butanone-d5	4.618	46		101143	50.186	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery =	100.380%		
24) Chloroform-d	5.055	84		90262	4.495	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	89.800%		
26) 1,2-Dichloroethane-d4	5.695	65		45331	4.686	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	93.800%		
32) Benzene-d6	5.721	84		179225	4.404	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery =	88.000%		
36) 1,2-Dichloropropane-d6	6.682	67		56532	4.533	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery =	90.600%		
41) Toluene-d8	7.894	98		147511	3.899	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery =	78.000%		
43) trans-1,3-Dichloroprop...	8.177	79		16256	4.163	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery =	83.200%		
46) 2-Hexanone-d5	8.627	63		80676	49.725	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery =	99.440%		
56) 1,1,2,2-Tetrachloroeth...	10.749	84		49776	4.831	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery =	96.600%		
66) 1,2-Dichlorobenzene-d4	12.187	152		58331	5.121	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery =	102.400%		
Target Compounds							
13) Acetone	2.631	43		35865m	27.434	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059647.D
Acq On : 29 Jun 2024 01:48
Operator : MD/SY
Sample : P3059-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN4

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

