




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059648.D
 Acq On : 29 Jun 2024 02:12
 Operator : MD/SY
 Sample : P3059-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GN5

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

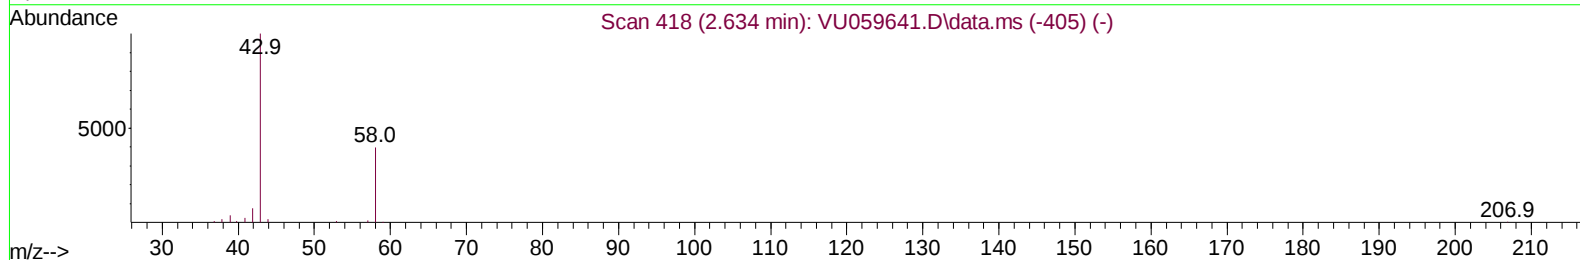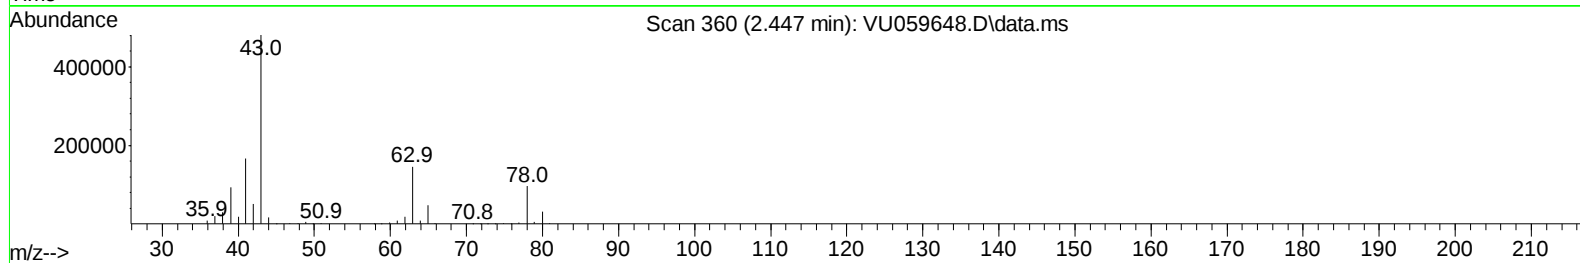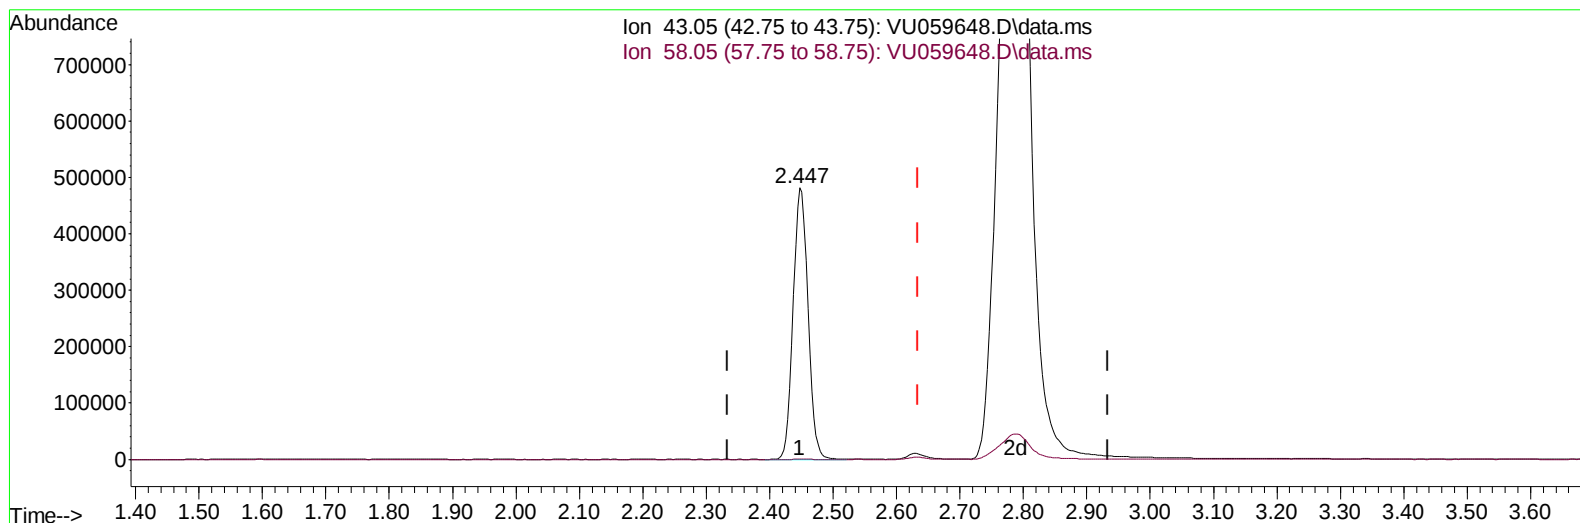

TIC: VU059648.D\data.ms

(13) Acetone (T)

2.447min (-0.186) 606.85 ug/L

response 785665

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	1.06
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059648.D
Acq On : 29 Jun 2024 02:12
Operator : MD/SY
Sample : P3059-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN5

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

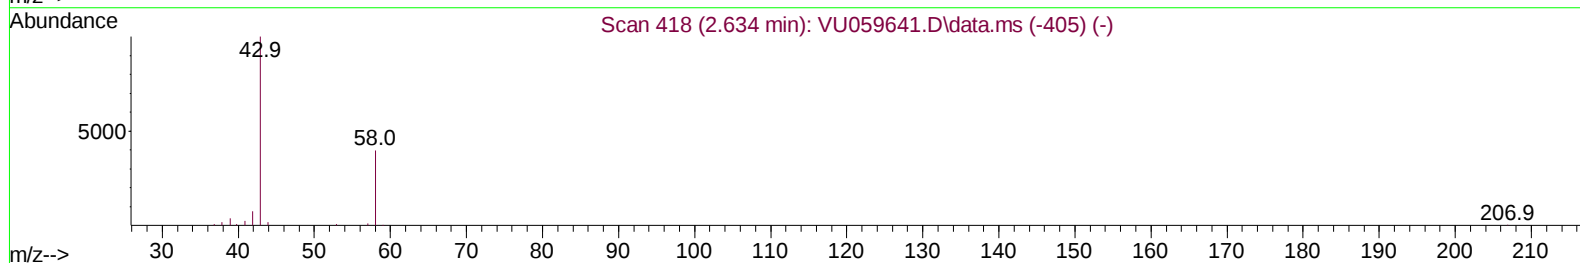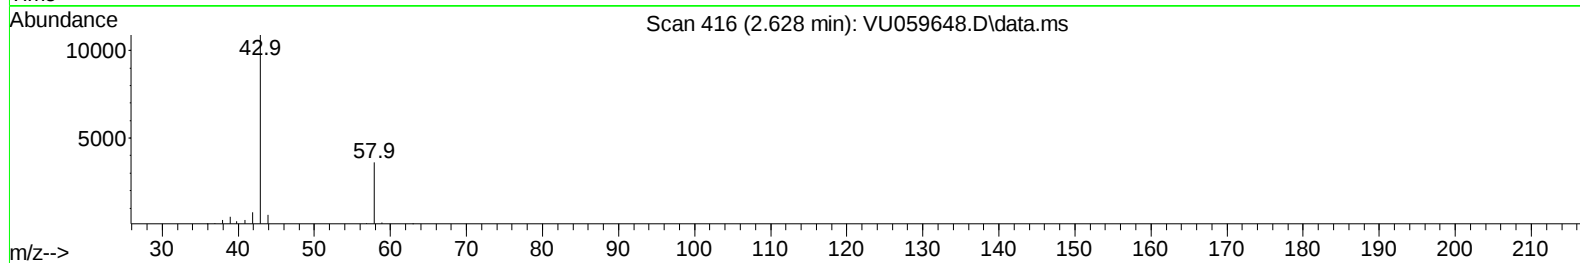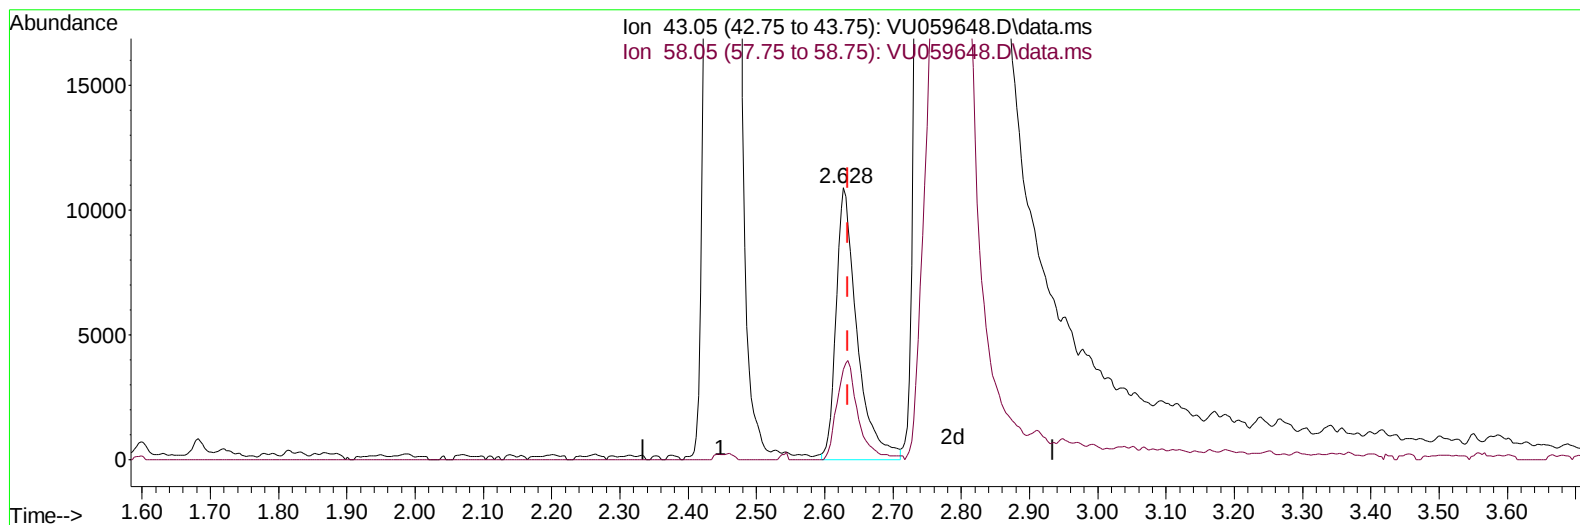

TIC: VU059648.D\data.ms

(13) Acetone (T)

2.628min (-0.006) 17.83 ug/L m

response 23084

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	36.10
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059648.D
 Acq On : 29 Jun 2024 02:12
 Operator : MD/SY
 Sample : P3059-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GN5

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		139341	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		146136	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		60605	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		33374	3.445	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.800%	
7) Chloroethane-d5	1.907	69		37711	4.045	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	81.000%	
11) 1,1-Dichloroethene-d2	2.563	65		14579	3.627	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.600%	
20) 2-Butanone-d5	4.618	46		101039	50.625	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.260%	
24) Chloroform-d	5.055	84		89064	4.478	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.600%	
26) 1,2-Dichloroethane-d4	5.695	65		44530	4.648	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.000%	
32) Benzene-d6	5.721	84		175390	4.361	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%	
36) 1,2-Dichloropropane-d6	6.682	67		55661	4.516	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	90.400%	
41) Toluene-d8	7.894	98		143430	3.836	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.800%	
43) trans-1,3-Dichloroprop...	8.174	79		16152	4.185	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.800%	
46) 2-Hexanone-d5	8.627	63		78693	49.077	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	98.160%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		49034	4.815	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.400%	
66) 1,2-Dichlorobenzene-d4	12.190	152		55580	5.153	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	103.000%	
Target Compounds							
13) Acetone	2.628	43		23084m	17.830	ug/L	
16) Methylene chloride	3.039	84		2023	0.173	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059648.D
Acq On : 29 Jun 2024 02:12
Operator : MD/SY
Sample : P3059-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GN5

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:13:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

