




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059651.D
Acq On : 29 Jun 2024 03:24
Operator : MD/SY
Sample : P3059-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP4

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:14:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

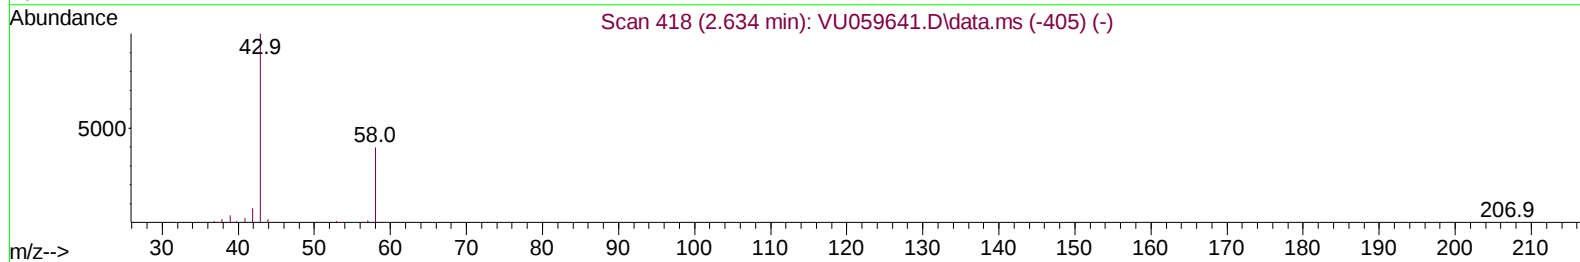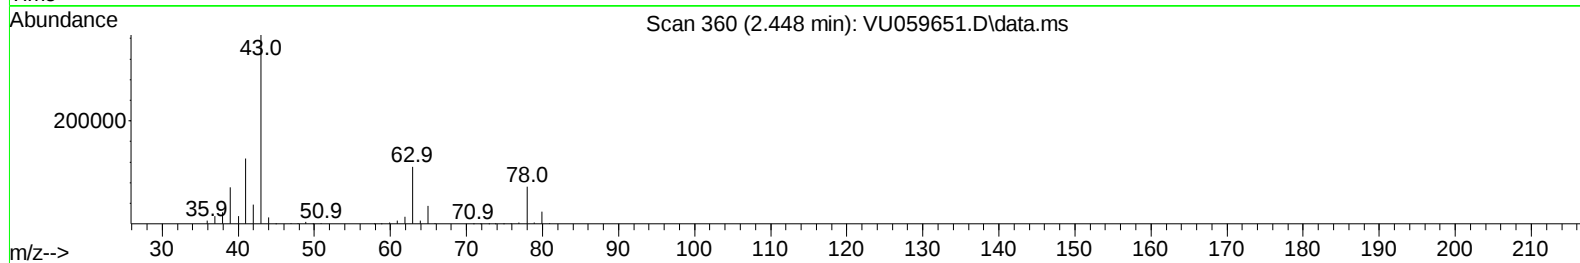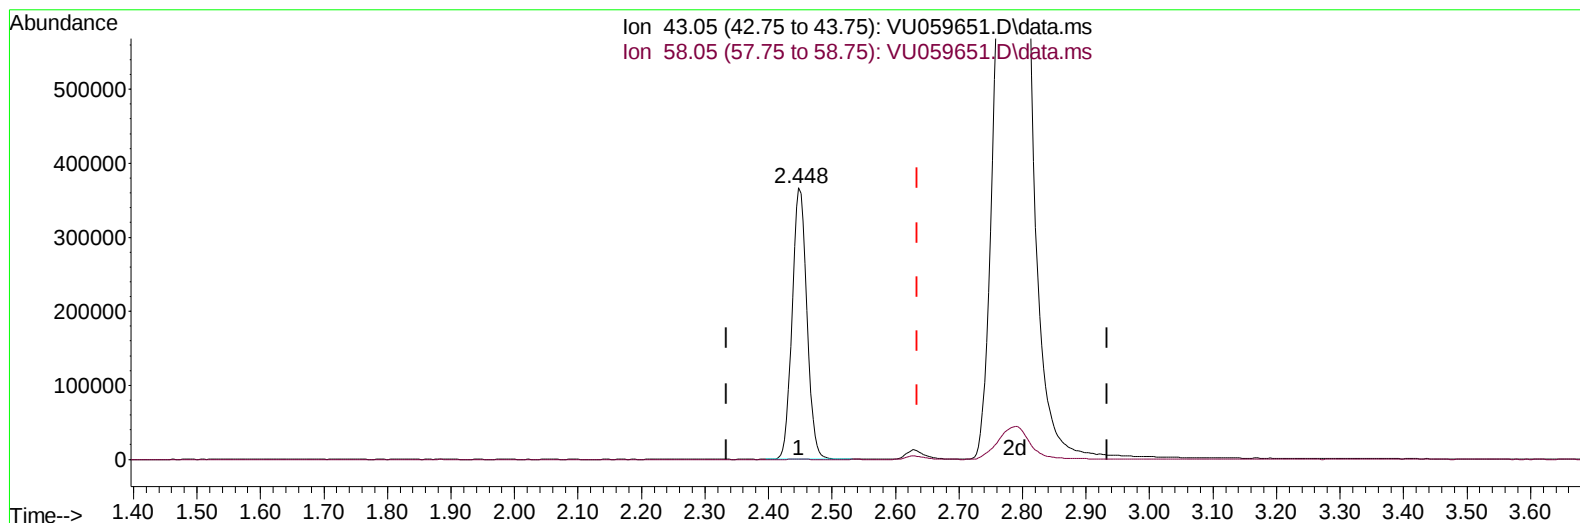

TIC: VU059651.D\data.ms

(13) Acetone (T)

2.448min (-0.186) 441.40 ug/L

response 592750

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	1.74
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059651.D
Acq On : 29 Jun 2024 03:24
Operator : MD/SY
Sample : P3059-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP4

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:14:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

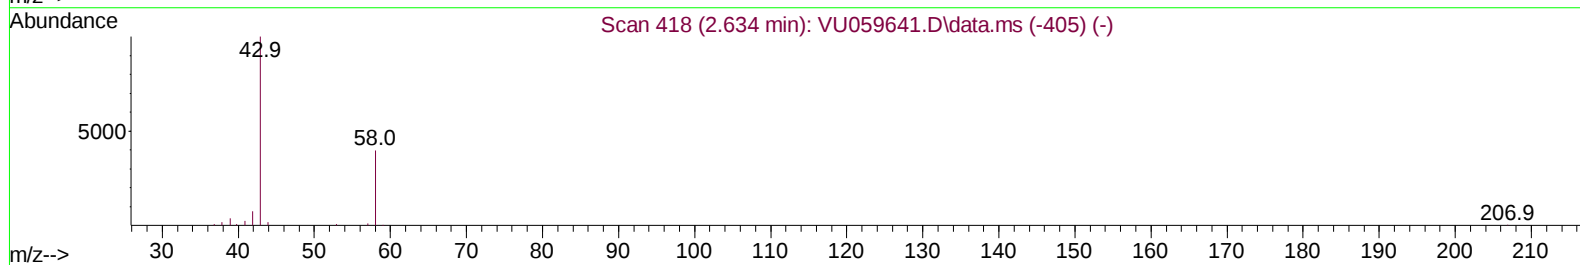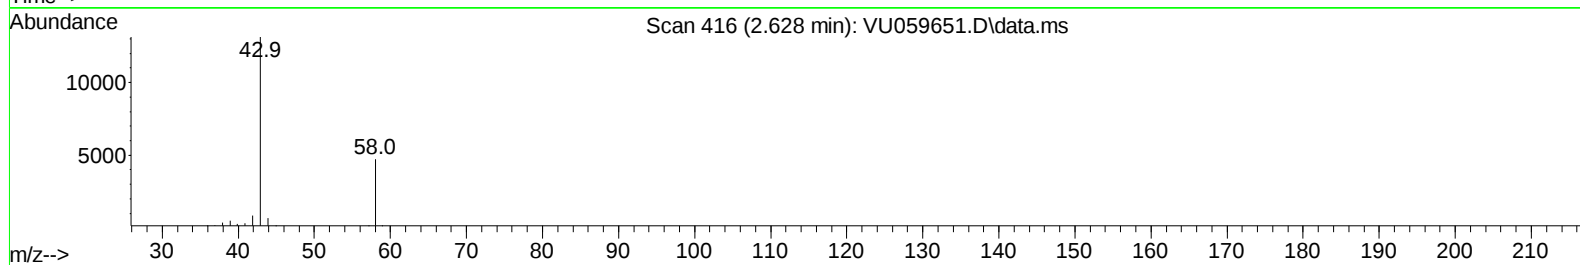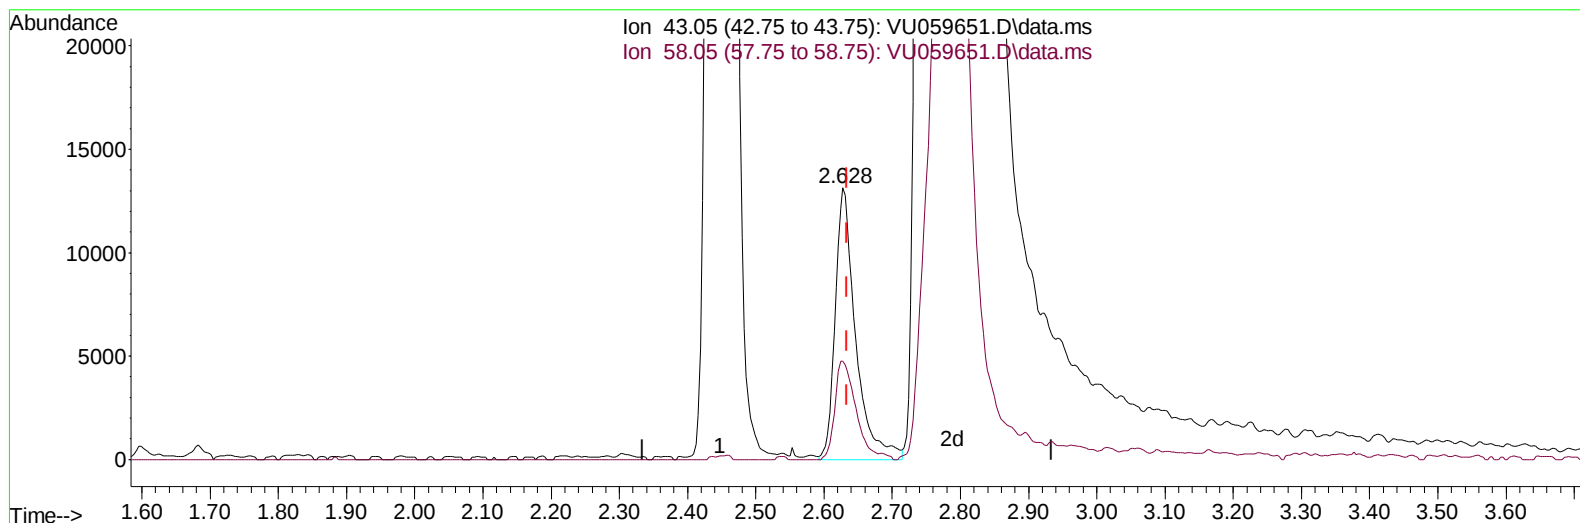

TIC: VU059651.D\data.ms

(13) Acetone (T)

2.628min (-0.006) 20.40 ug/L m

response 27394

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	37.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059651.D
 Acq On : 29 Jun 2024 03:24
 Operator : MD/SY
 Sample : P3059-17
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GP4

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:14:30 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		144533	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		146934	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		65984	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.595	65		33559	3.339	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	66.800%	
7) Chloroethane-d5	1.907	69		37379	3.865	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	77.400%	
11) 1,1-Dichloroethene-d2	2.563	65		15594	3.740	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	74.800%	
20) 2-Butanone-d5	4.618	46		105038	50.739	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	101.480%	
24) Chloroform-d	5.052	84		91160	4.419	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	88.400%	
26) 1,2-Dichloroethane-d4	5.695	65		45480	4.577	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	91.600%	
32) Benzene-d6	5.721	84		177836	4.398	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	88.000%	
36) 1,2-Dichloropropane-d6	6.682	67		57706	4.657	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	93.200%	
41) Toluene-d8	7.891	98		148236	3.943	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	78.800%	
43) trans-1,3-Dichloroprop...	8.177	79		16582	4.274	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	85.400%	
46) 2-Hexanone-d5	8.627	63		77791	48.251	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	96.500%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84		49943	4.878	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	97.600%	
66) 1,2-Dichlorobenzene-d4	12.187	152		60303	5.135	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	102.600%	
Target Compounds							
13) Acetone	2.628	43		27394m	20.399	ug/L	
16) Methylene chloride	3.039	84		3216	0.265	ug/L	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059651.D
Acq On : 29 Jun 2024 03:24
Operator : MD/SY
Sample : P3059-17
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP4

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:14:30 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

