




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059653.D
Acq On : 29 Jun 2024 04:11
Operator : MD/SY
Sample : P3059-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP6

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:44:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

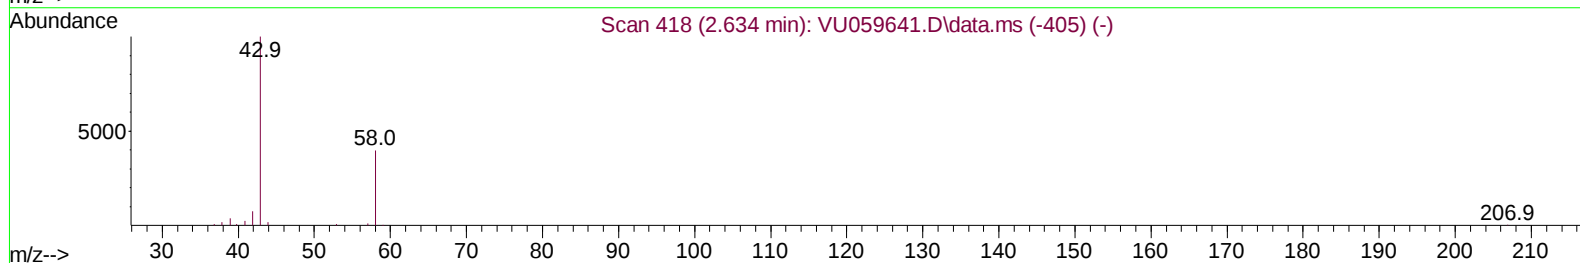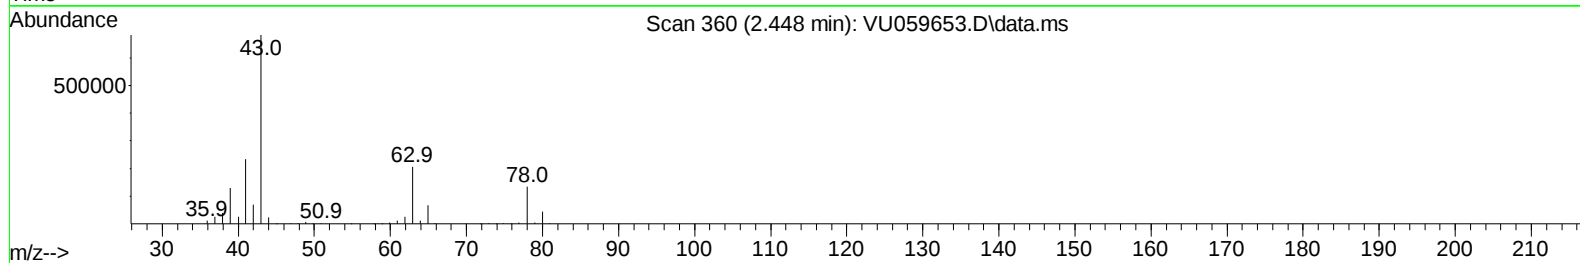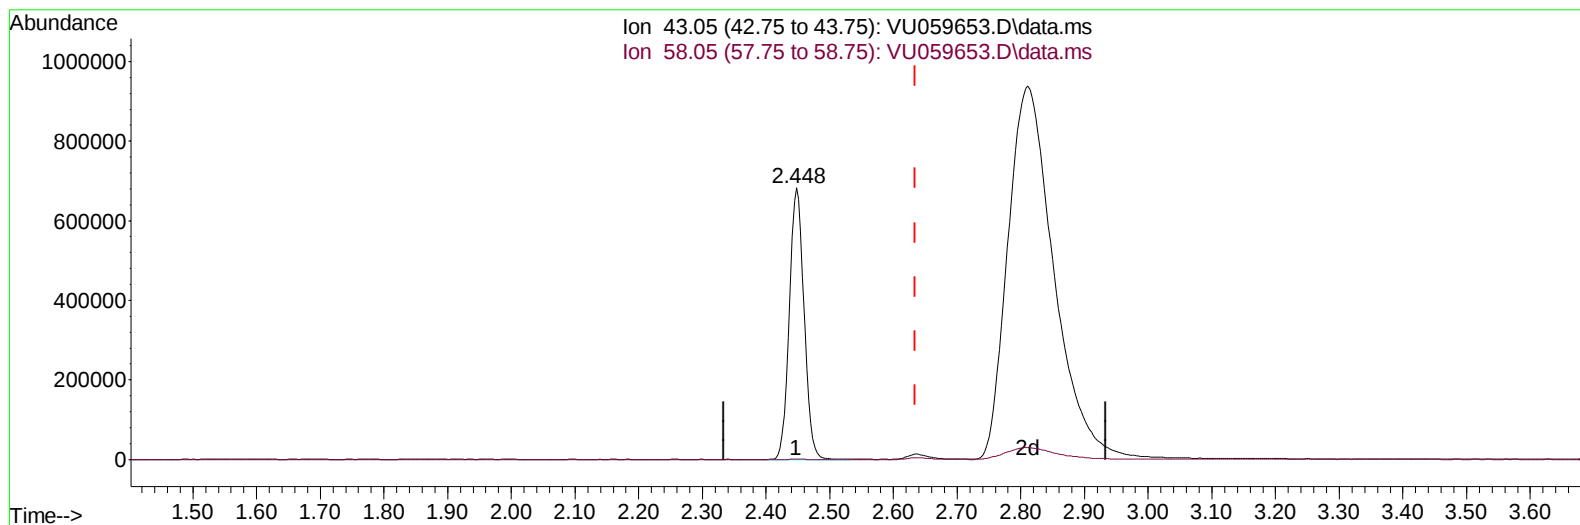

TIC: VU059653.D\data.ms

(13) Acetone (T)

2.448min (-0.186) 808.49 ug/L

response 1093545

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	1.04
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059653.D
Acq On : 29 Jun 2024 04:11
Operator : MD/SY
Sample : P3059-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP6

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:44:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

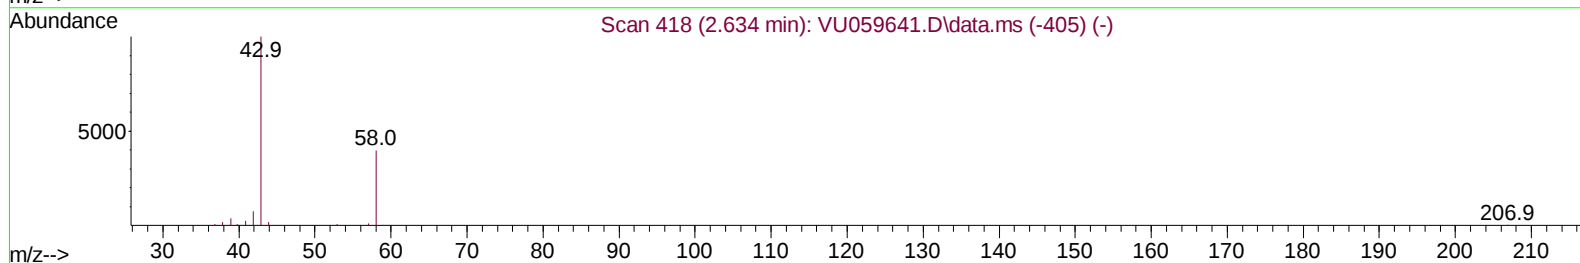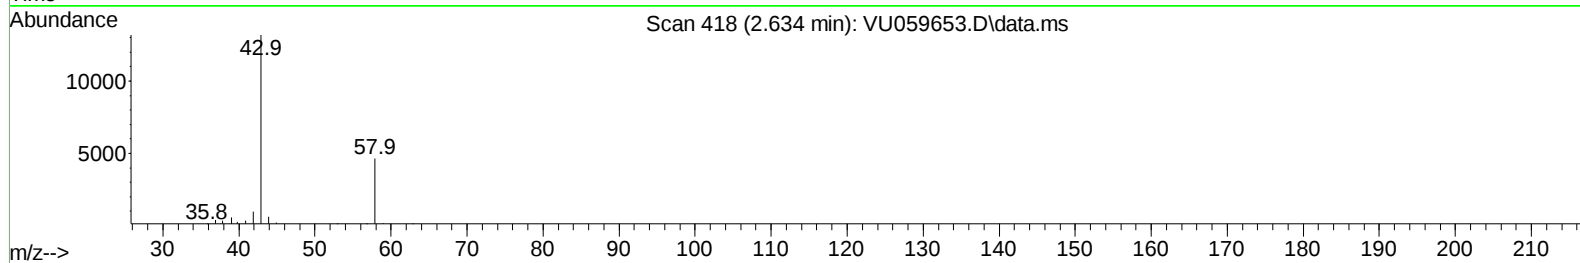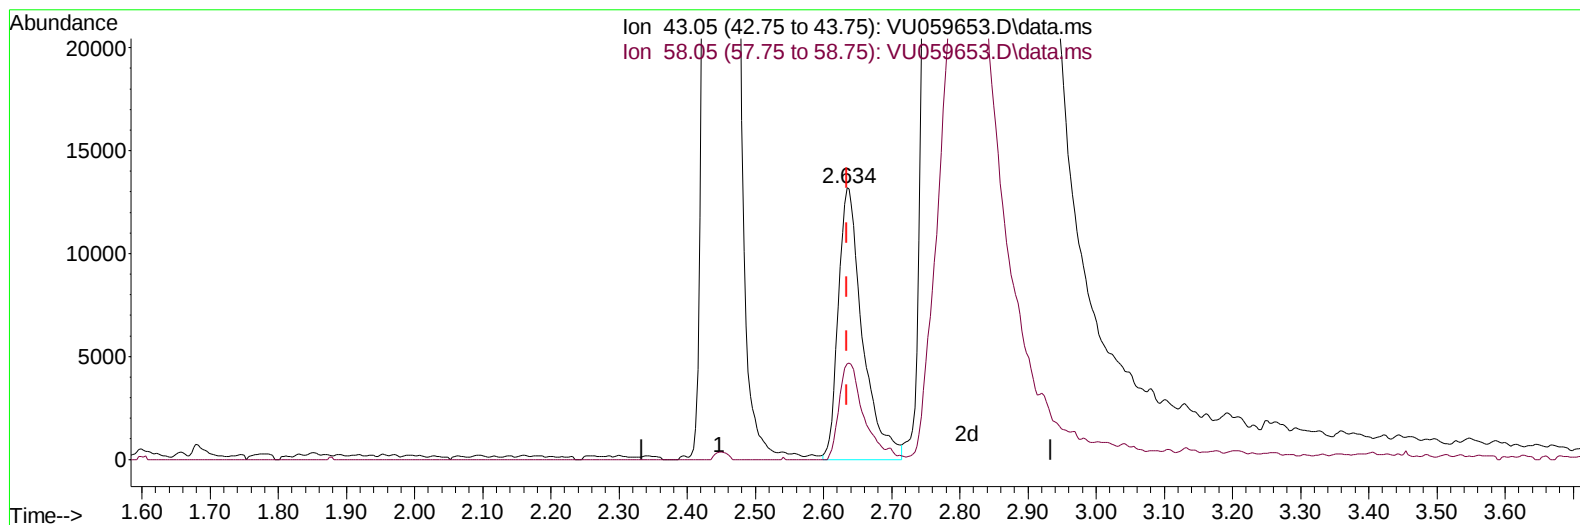

TIC: VU059653.D\data.ms

(13) Acetone (T)

2.634min (+ 0.000) 24.11 ug/L m

response 32615

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	34.99
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059653.D
 Acq On : 29 Jun 2024 04:11
 Operator : MD/SY
 Sample : P3059-19
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GP6

Manual IntegrationsAPPROVED

Quant Time: Jun 29 04:44:28 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		145574	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		151521	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		66736	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		32106	3.172	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	63.400%	
7) Chloroethane-d5	1.908	69		36416	3.739	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	74.800%	
11) 1,1-Dichloroethene-d2	2.560	65		15127	3.602	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	72.000%	
20) 2-Butanone-d5	4.621	46		105300	50.501	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	101.000%	
24) Chloroform-d	5.052	84		89225	4.294	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	85.800%	
26) 1,2-Dichloroethane-d4	5.692	65		43915	4.388	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	87.800%	
32) Benzene-d6	5.721	84		174664	4.188	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	83.800%	
36) 1,2-Dichloropropane-d6	6.682	67		55897	4.374	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	87.400%	
41) Toluene-d8	7.891	98		147421	3.803	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	76.000%	
43) trans-1,3-Dichloroprop...	8.174	79		14961	3.739	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	74.800%	
46) 2-Hexanone-d5	8.628	63		81308	48.906	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	97.820%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		49420	4.681	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	93.600%	
66) 1,2-Dichlorobenzene-d4	12.187	152		58689	4.941	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	98.800%	
Target Compounds							
						Qvalue	
13) Acetone	2.634	43		32615m	24.113	ug/L	
14) Carbon disulfide	2.789	76		47544	1.380	ug/L	98
16) Methylene chloride	3.036	84		3031	0.248	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059653.D
Acq On : 29 Jun 2024 04:11
Operator : MD/SY
Sample : P3059-19
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GP6

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

Quant Time: Jun 29 04:44:28 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

