

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
 Data File : VU059647.D
 Acq On : 29 Jun 2024 01:48
 Operator : MD/SY
 Sample : P3059-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E1GN4

Manual Integrations
 APPROVED

Reviewed By :Mahesh Dadoda 07/01/2024
 Supervised By :Semsettin Yesilyurt 07/01/2024

Quant Time: Jun 29 04:13:29 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Jun 29 01:51:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	140705	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	147868	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	63995	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.595	65	33756	3.450	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	69.000%	
7) Chloroethane-d5	1.907	69	38122	4.049	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	81.000%	
11) 1,1-Dichloroethene-d2	2.560	65	15866	3.909	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.200%	
20) 2-Butanone-d5	4.618	46	101143	50.186	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	100.380%	
24) Chloroform-d	5.055	84	90262	4.495	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	89.800%	
26) 1,2-Dichloroethane-d4	5.695	65	45331	4.686	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	93.800%	
32) Benzene-d6	5.721	84	179225	4.404	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	88.000%	
36) 1,2-Dichloropropane-d6	6.682	67	56532	4.533	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	90.600%	
41) Toluene-d8	7.894	98	147511	3.899	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	78.000%	
43) trans-1,3-Dichloroprop...	8.177	79	16256	4.163	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	83.200%	
46) 2-Hexanone-d5	8.627	63	80676	49.725	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	99.440%	
56) 1,1,2,2-Tetrachloroeth...	10.749	84	49776	4.831	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.600%	
66) 1,2-Dichlorobenzene-d4	12.187	152	58331	5.121	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	102.400%	
Target Compounds					Qvalue	
13) Acetone	2.631	43	35865m	27.434	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059647.D
Acq On : 29 Jun 2024 01:48
Operator : MD/SY
Sample : P3059-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
E1GN4

Quant Time: Jun 29 04:13:29 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Jun 29 01:51:23 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

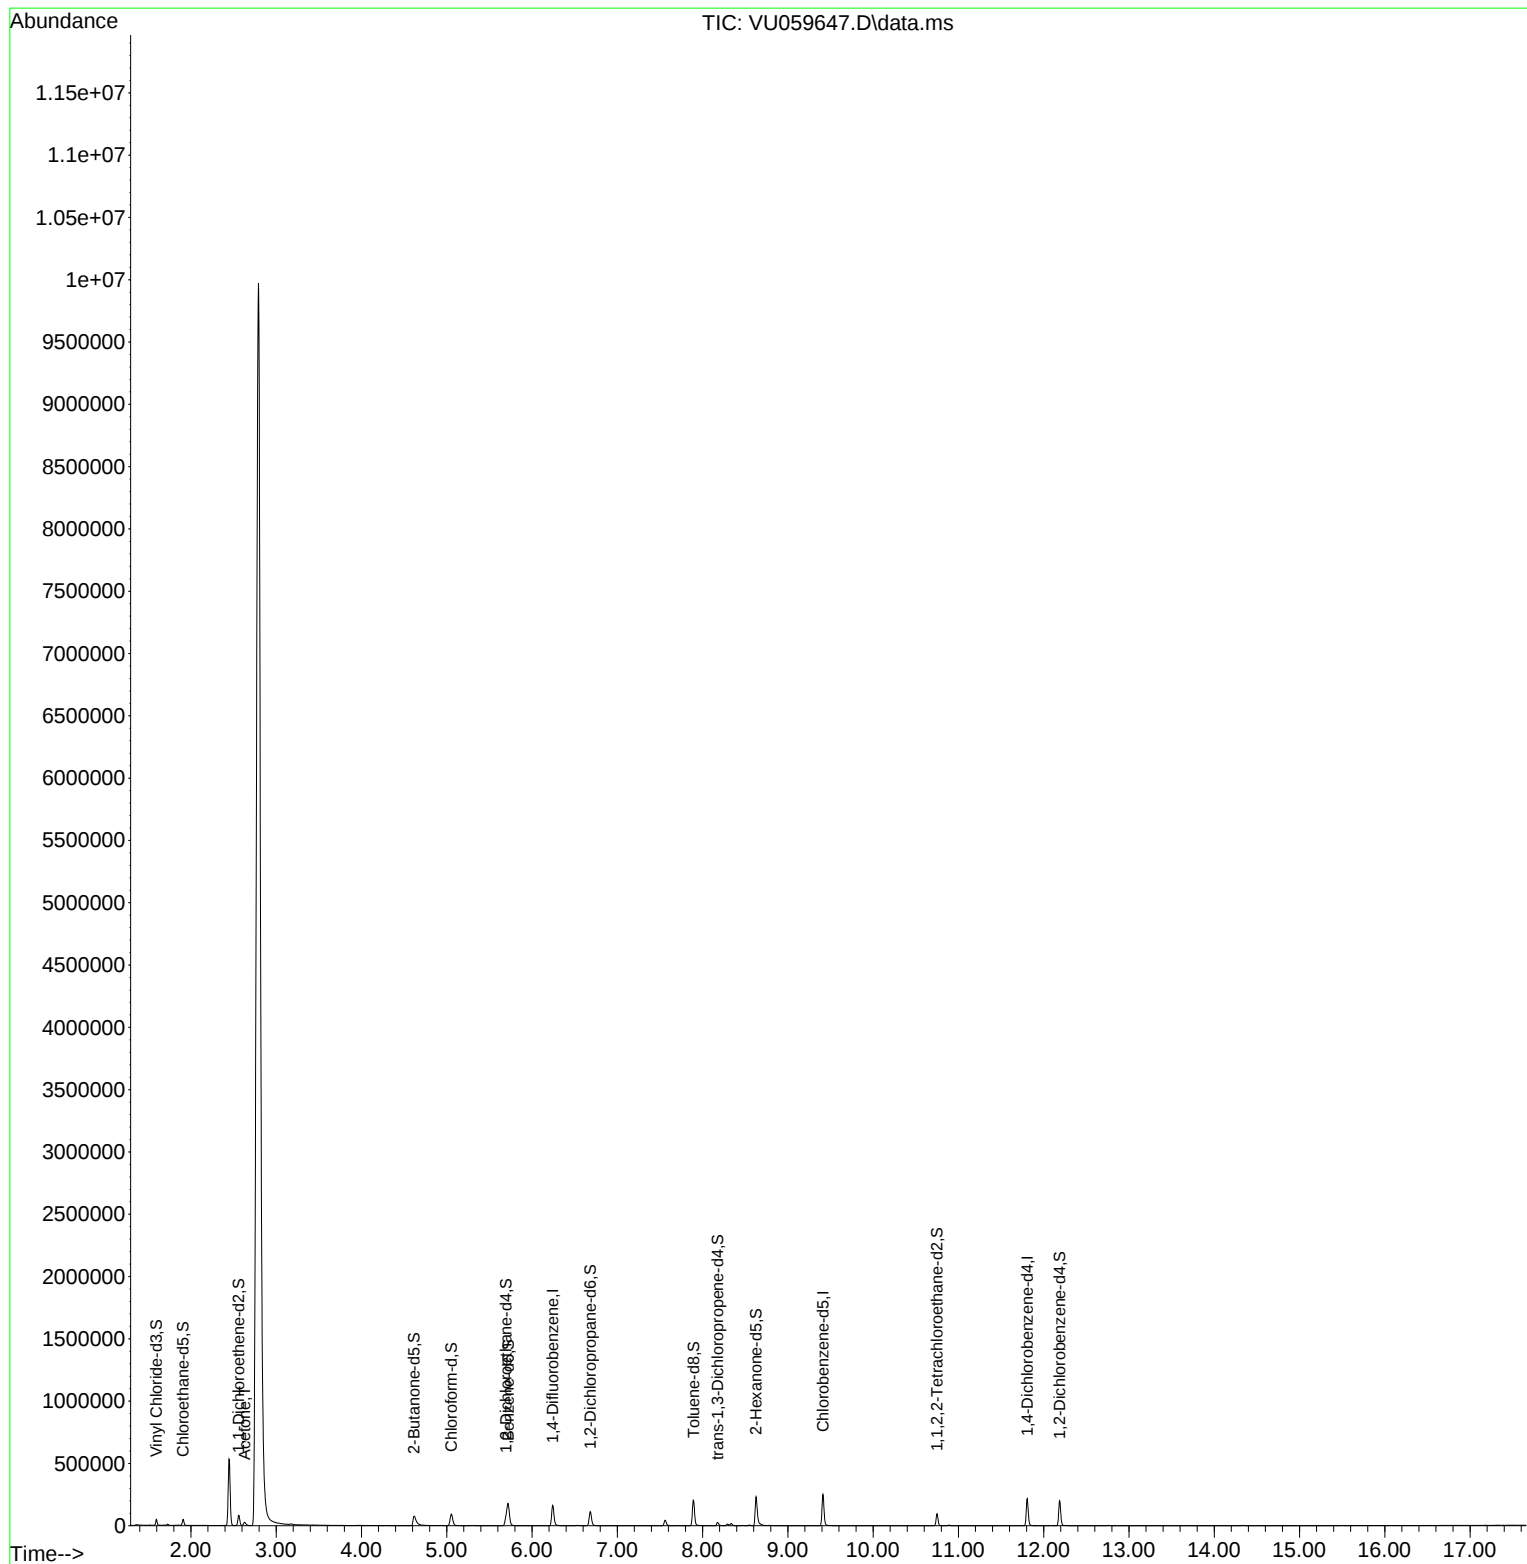

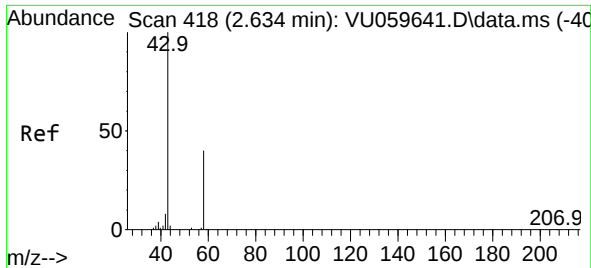

#13
Acetone
Concen: 27.434 ug/L m
RT: 2.631 min Scan# 41
Delta R.T. -0.003 min
Lab File: VU059647.D
Acq: 29 Jun 2024 01:48

Instrument :
MSVOA_U
ClientSampleId :
E1GN4

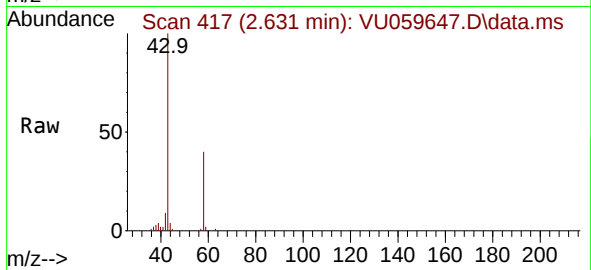

Tgt Ion: 43 Resp: 3586
Ion Ratio Lower Upper
43 100
58 38.2 0.0 68.0

Manual Integrations
APPROVED

Reviewed By :Mahesh Dadoda 07/01/2024
Supervised By :Semsettin Yesilyurt 07/01/2024

