

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059625.D
Acq On : 28 Jun 2024 17:05
Operator : MD/SY
Sample : P3059-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM5

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.1 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Title : TRACE VOA SFAM1.0

Signal : TIC: VU059625.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.448	343	360	384	rBV	6503137	10384129	20.94%	17.316%
2	2.792	439	467	551	rBV2	15234877	49583867	100.00%	82.684%




Sum of corrected areas: 59967996

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059625.D
Acq On : 28 Jun 2024 17:05
Operator : MD/SY
Sample : P3059-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

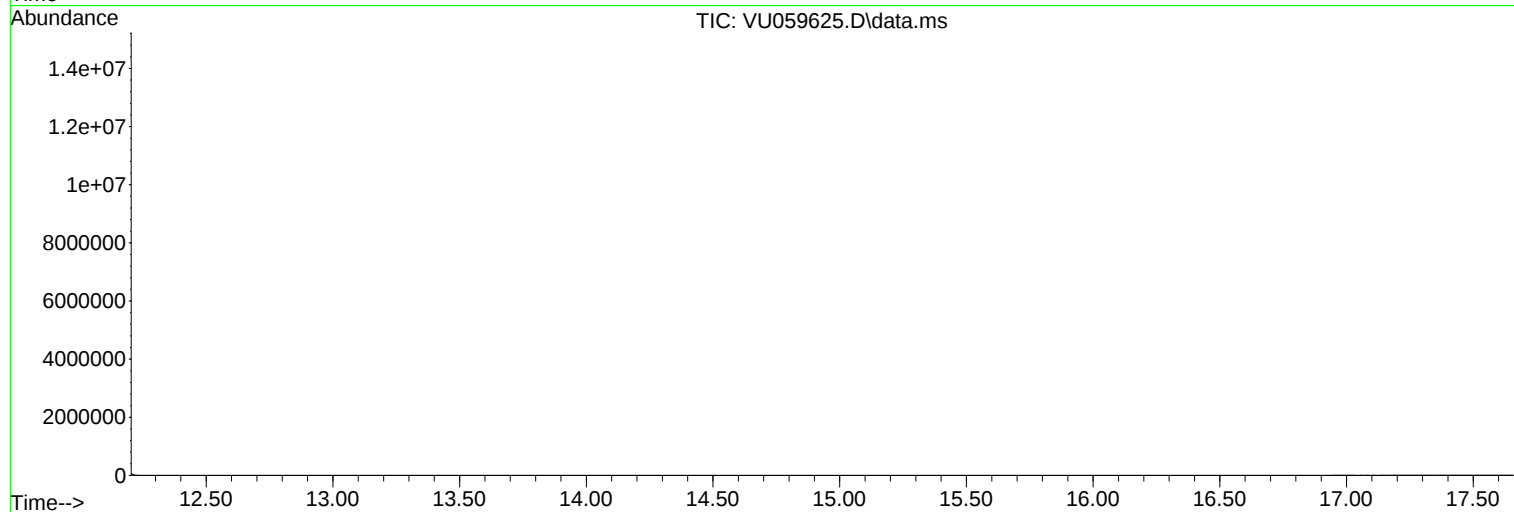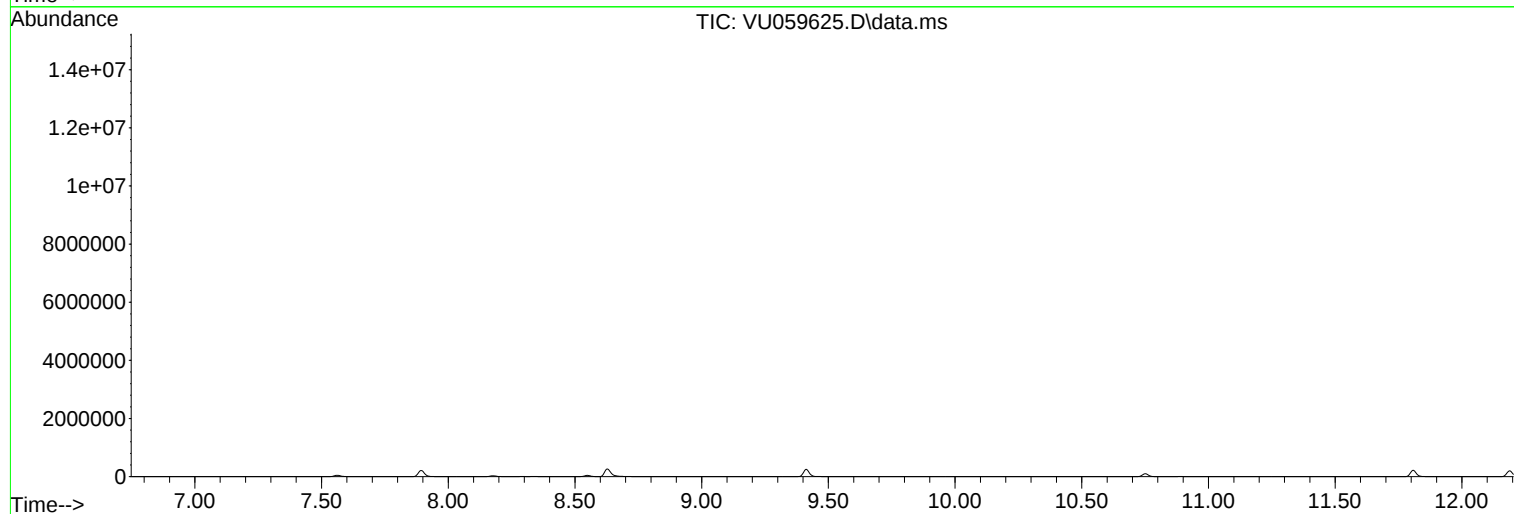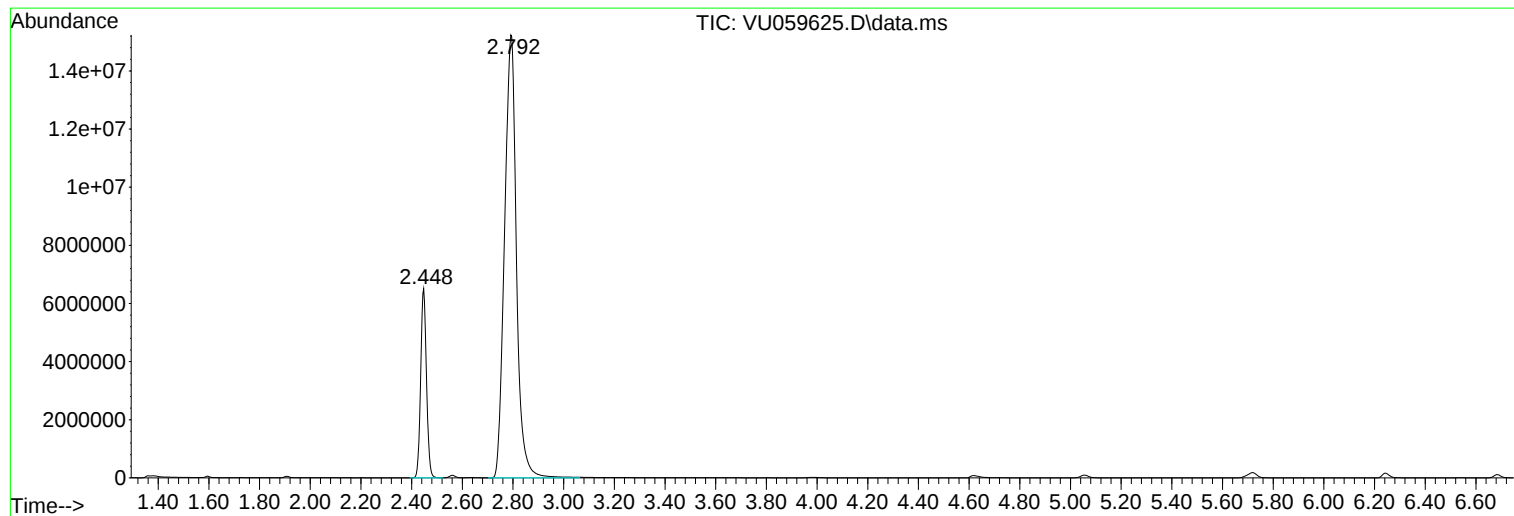

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059625.D
Acq On : 28 Jun 2024 17:05
Operator : MD/SY
Sample : P3059-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.448	1.05 ug/L	10384100	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	91
2	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	64
3	Propane, 2-chloro-			78	C3H7Cl	000075-29-6	42
4	Propane, 2-nitro-			89	C3H7NO2	000079-46-9	9
5	Acetyl chloride			78	C2H3ClO	000075-36-5	9

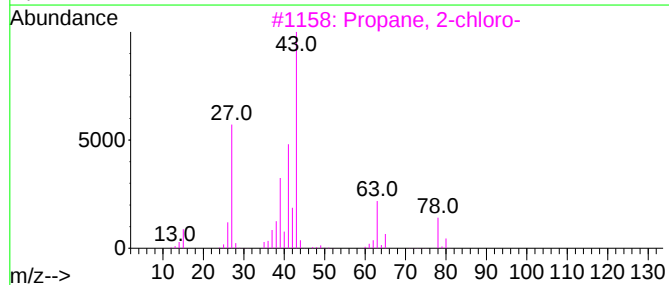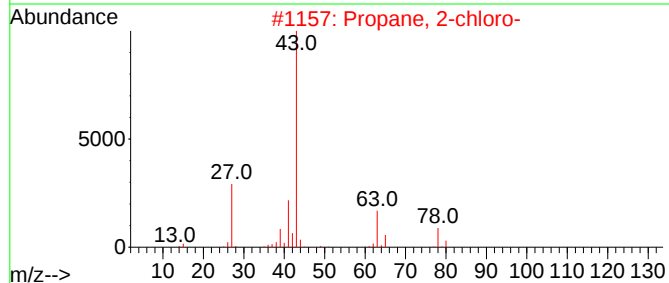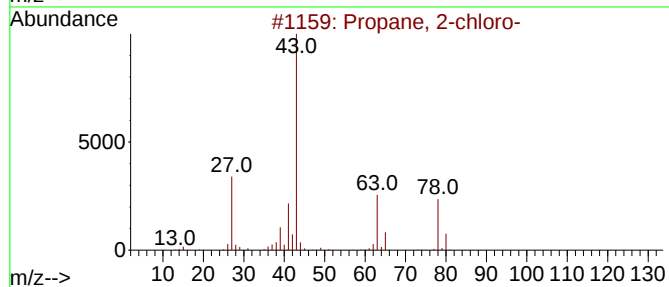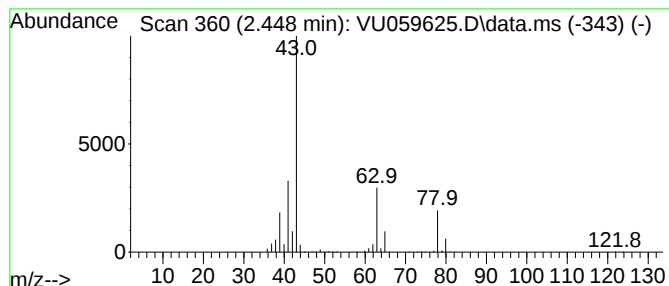

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059625.D
Acq On : 28 Jun 2024 17:05
Operator : MD/SY
Sample : P3059-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.792	5.00 ug/L	49583900	1,4-Difluorobenzene	6.242

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Isopropyl Alcohol			60	C3H8O	000067-63-0	86
2	Isopropyl Alcohol			60	C3H8O	000067-63-0	78
3	Isopropyl Alcohol			60	C3H8O	000067-63-0	64
4	Isopropyl Alcohol			60	C3H8O	000067-63-0	56
5	Isopropyl Alcohol			60	C3H8O	000067-63-0	9

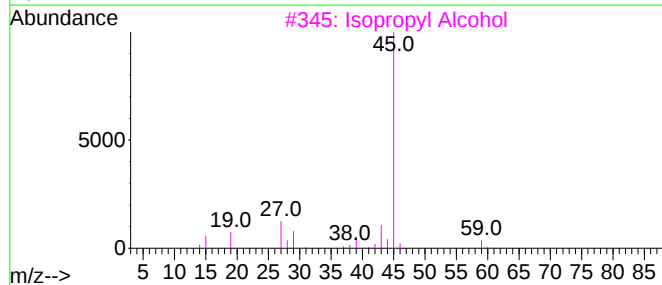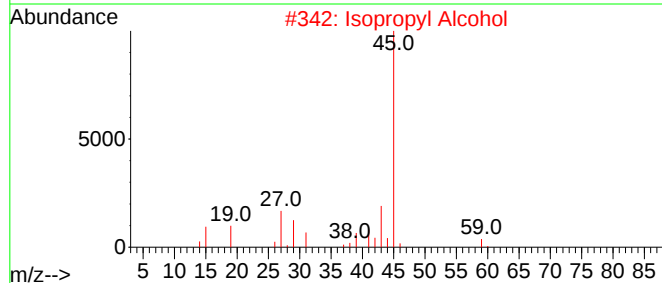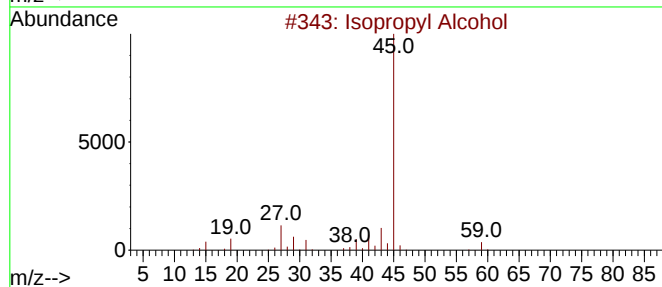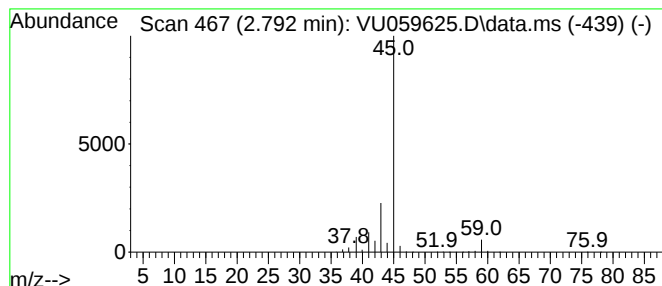

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU062924\
Data File : VU059625.D
Acq On : 28 Jun 2024 17:05
Operator : MD/SY
Sample : P3059-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E1GM5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR061724WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.448	1.1	ug/L	10384100	1	6.242	49583900	5.0
Isopropyl Alcohol	2.792	5.0	ug/L	49583900	1	6.242	49583900	5.0